

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070125\
Data File : FB031994.D
Signal(s) : FID2B.CH
Acq On : 1 Jul 2025 15:23
Operator : YP/AJ
Sample : Q2458-10
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
FB-06272025

Integration File: Calibration.e
Quant Time: Jul 02 00:02:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.806	179153	11.612 ng/ml
Target Compounds			
8) t m-Xylene	13.201	3039	0.093 ng/ml
9) t O-Xylene	13.921	6514	0.210 ng/ml
10) t 1,2,4-Trimethylbenzene	16.204	10479	0.396 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070125\
Data File : FB031994.D
Signal(s) : FID2B.CH
Acq On : 1 Jul 2025 15:23
Operator : YP/AJ
Sample : Q2458-10
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
FB-06272025

Integration File: Calibration.e
Quant Time: Jul 02 00:02:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

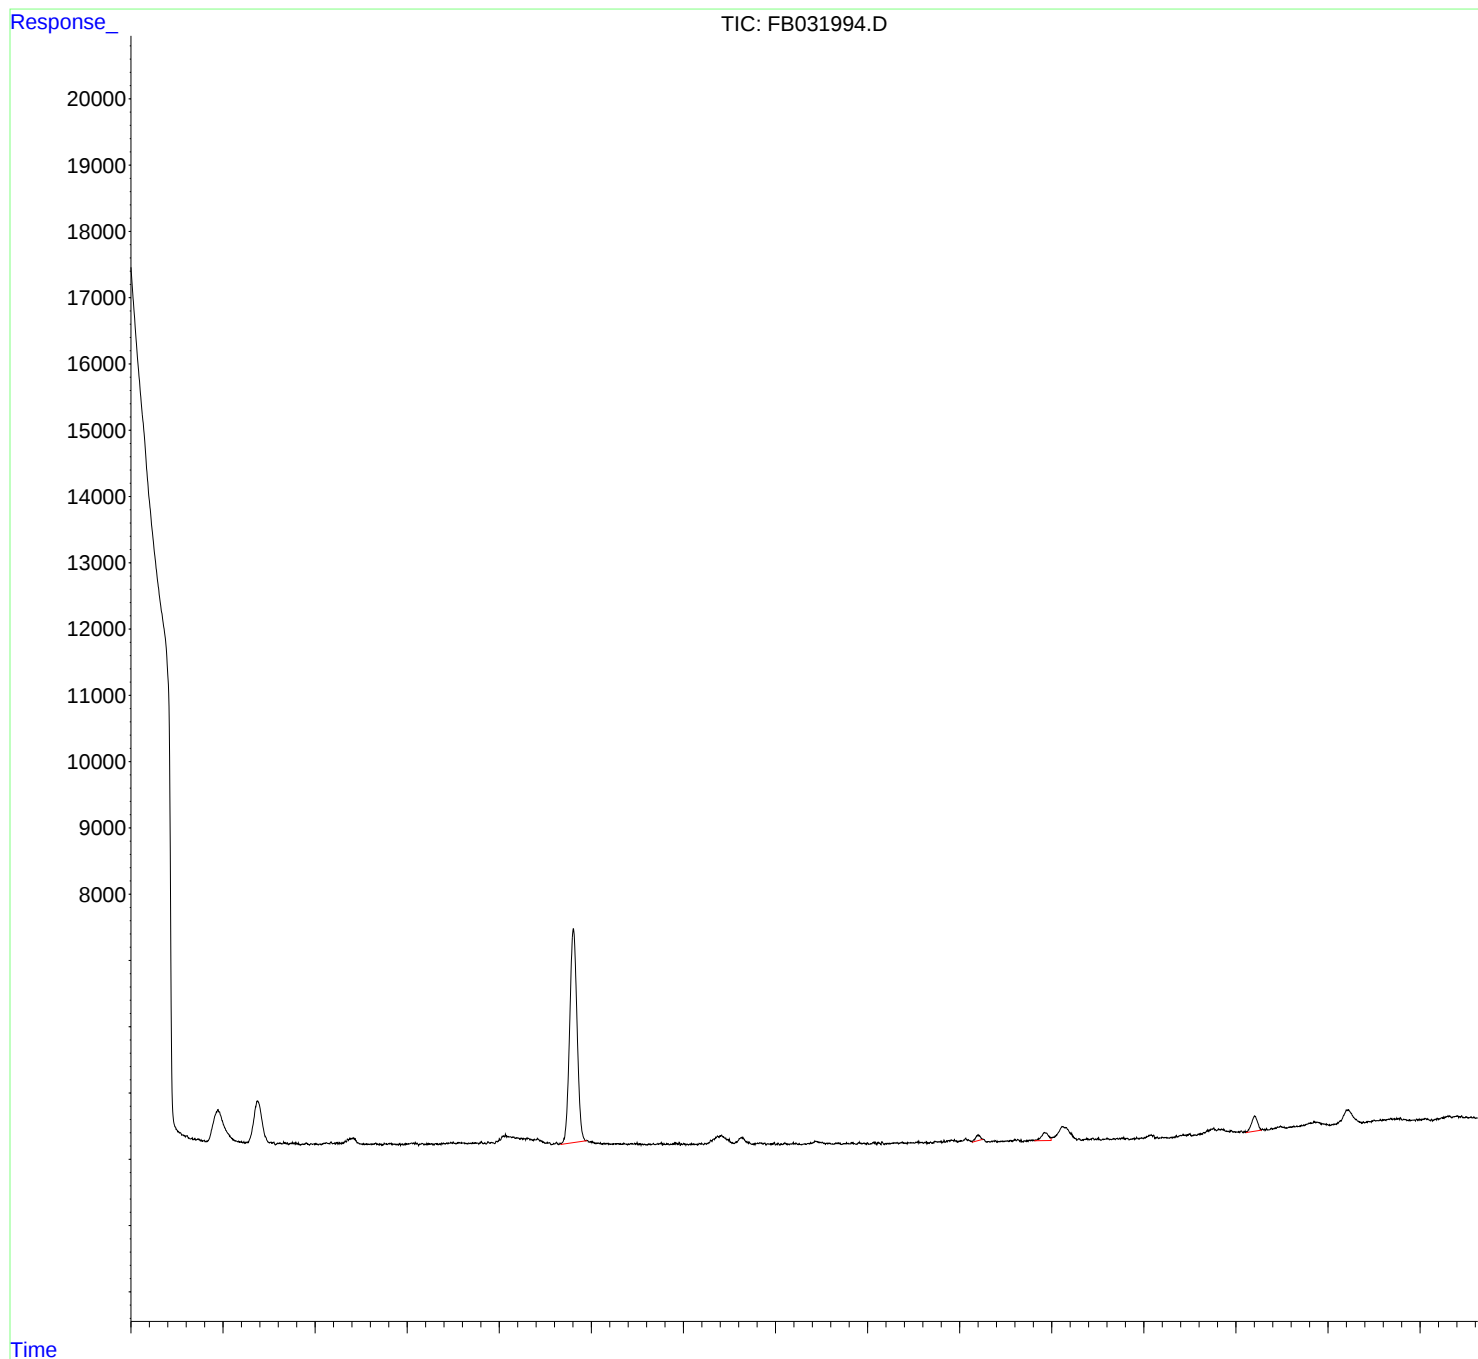


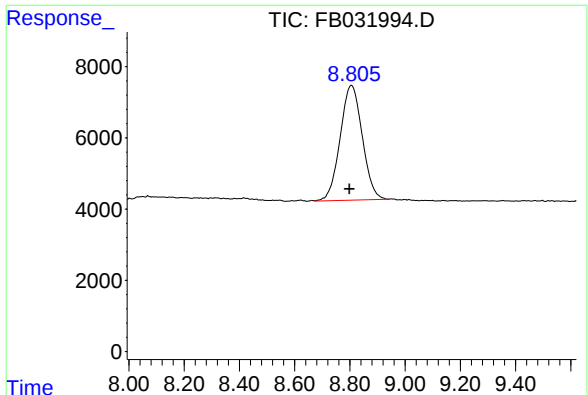

#5 AAA-TFT


R.T.: 8.806 min
Delta R.T.: 0.008 min
Response: 179153
Conc: 11.61 ng/ml

Instrument :
FID_B
ClientSampleId :
FB-06272025

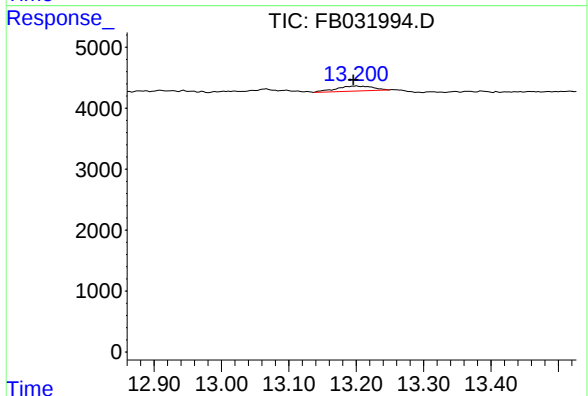


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: 0.006 min
Response: 3039
Conc: 0.09 ng/ml

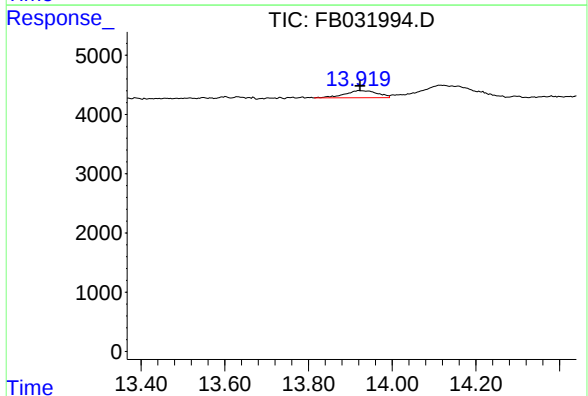

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: -0.002 min
Response: 6514
Conc: 0.21 ng/ml

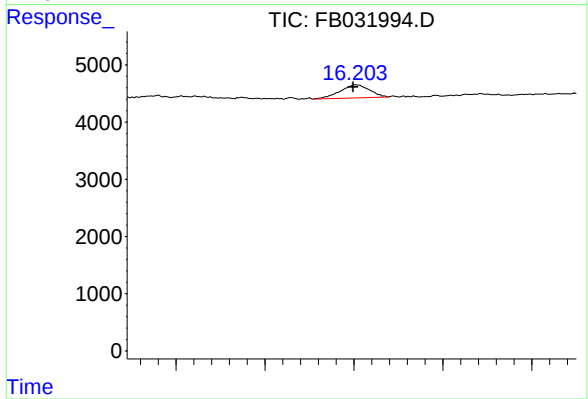

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min
Delta R.T.: 0.006 min
Response: 10479
Conc: 0.40 ng/ml