

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070125\
 Data File : FB031993.D
 Signal(s) : FID2B.CH
 Acq On : 1 Jul 2025 14:42
 Operator : YP/AJ
 Sample : BSF0701W1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0701W1

Integration File: Calibration.e
 Quant Time: Jul 01 14:31:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
 Quant Title :
 QLast Update : Mon Jun 23 13:56:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.806	321635	20.848 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.719	620402	24.386 ng/ml
2) t	2,2,4-Trimethylpentane	7.435	803912	29.810 ng/ml
3) t	n-Heptane	7.765	243172	9.746 ng/ml
4) t	Benzene	7.904	344966	10.146 ng/ml
6) t	Toluene	10.634	980272	27.414 ng/ml
7) t	Ethylbenzene	13.070	291208	9.222 ng/ml
8) t	m-Xylene	13.203	609246	18.575 ng/ml
9) t	O-Xylene	13.930	579107	18.658 ng/ml
10) t	1,2,4-Trimethylbenzene	16.205	489941	18.530 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070125\
Data File : FB031993.D
Signal(s) : FID2B.CH
Acq On : 1 Jul 2025 14:42
Operator : YP/AJ
Sample : BSF0701W1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0701W1

Integration File: Calibration.e
Quant Time: Jul 01 14:31:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

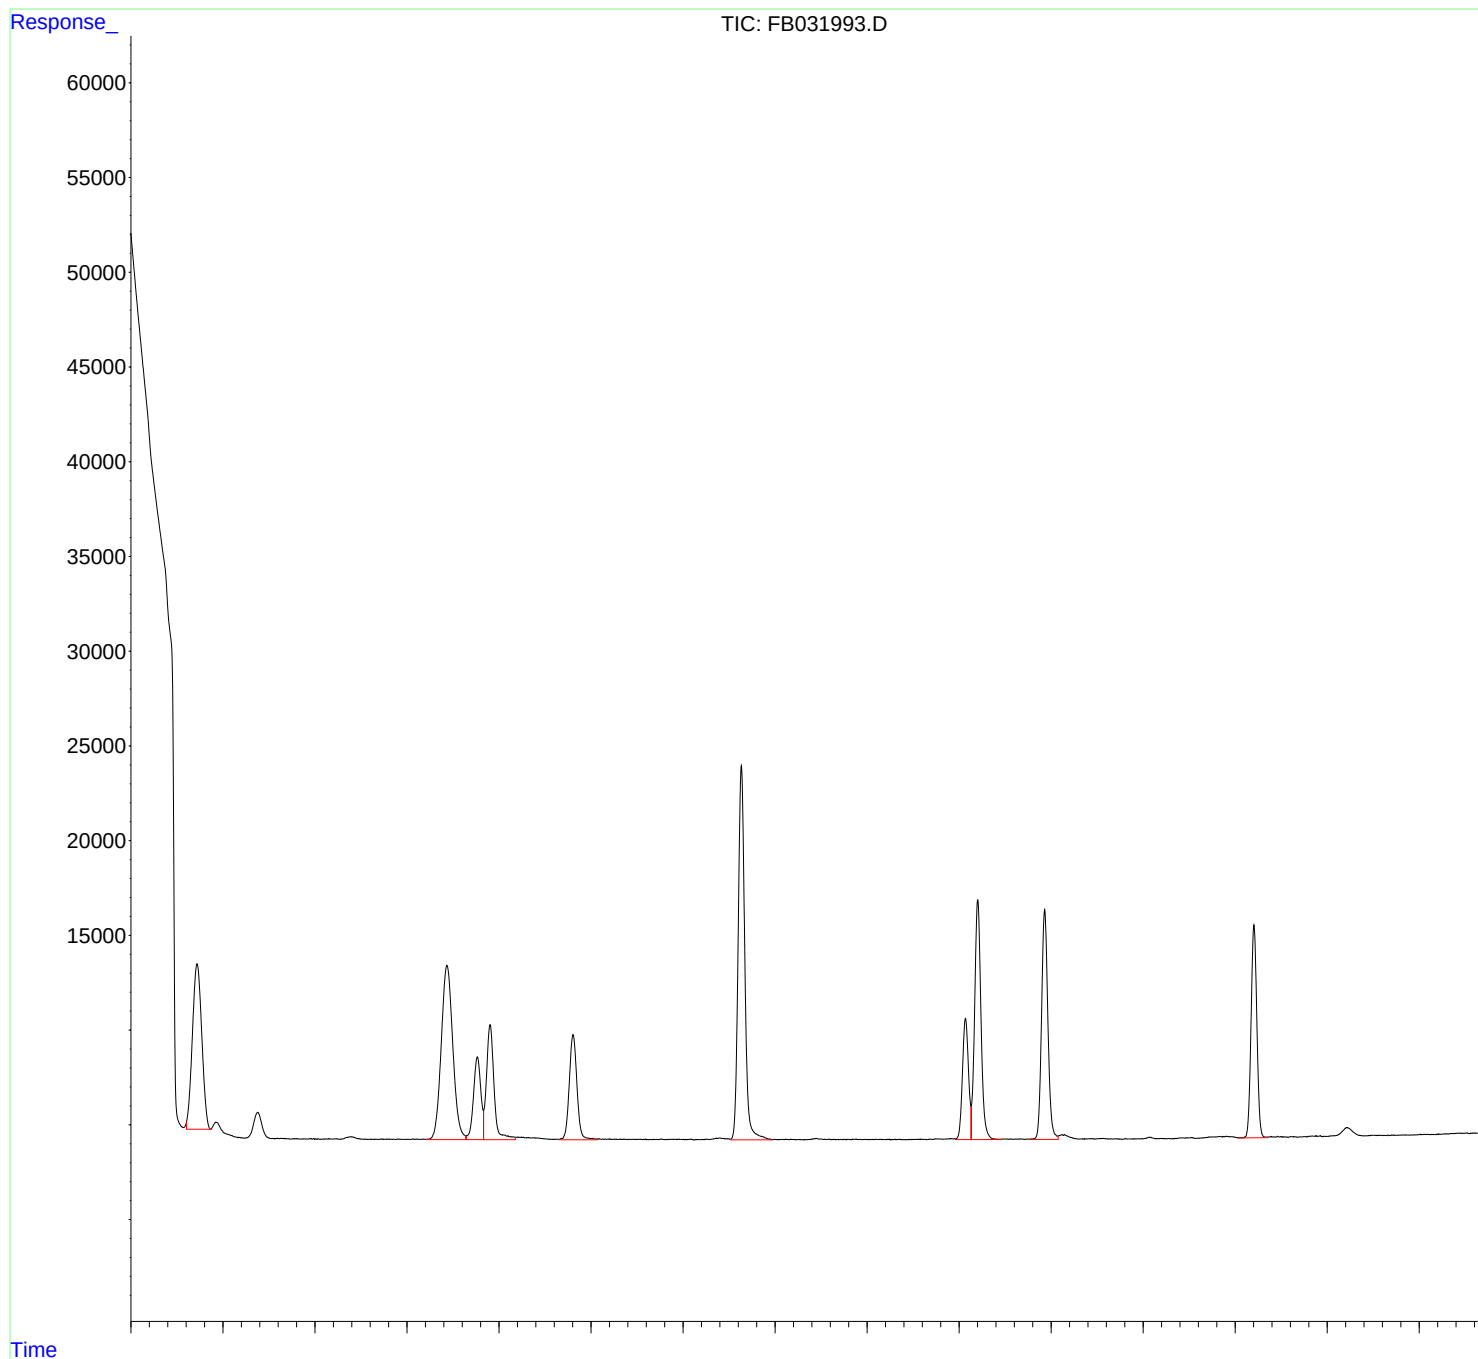


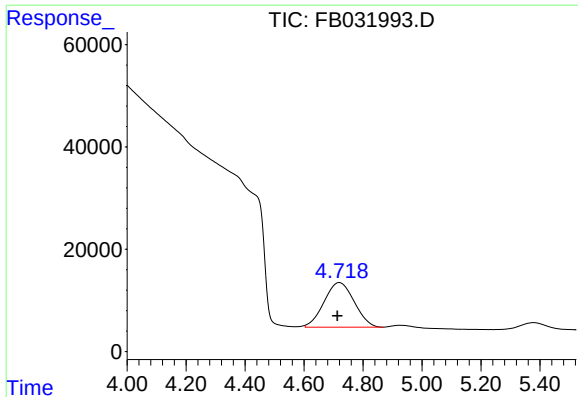

#1 2-Methylpentane


R.T.: 4.719 min
Delta R.T.: 0.006 min
Response: 620402
Conc: 24.39 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701W1

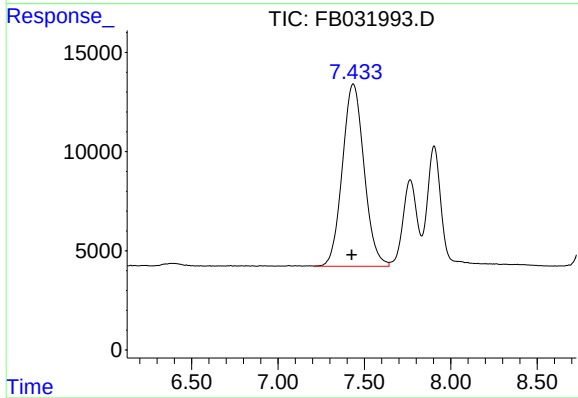


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: 0.009 min
Response: 803912
Conc: 29.81 ng/ml

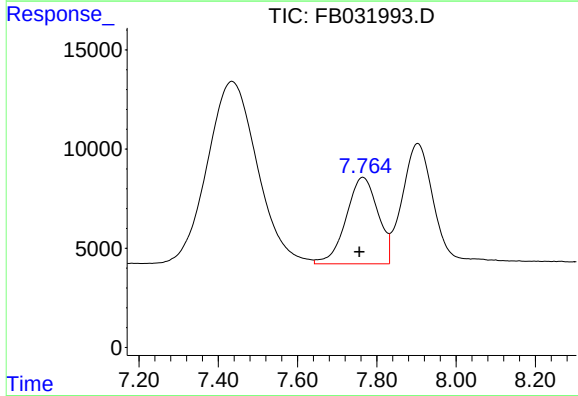


#3 n-Heptane

R.T.: 7.765 min
Delta R.T.: 0.009 min
Response: 243172
Conc: 9.75 ng/ml

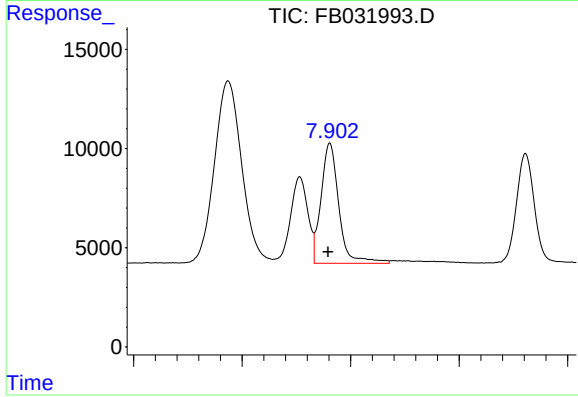

#4 Benzene


R.T.: 7.904 min
Delta R.T.: 0.008 min
Response: 344966
Conc: 10.15 ng/ml

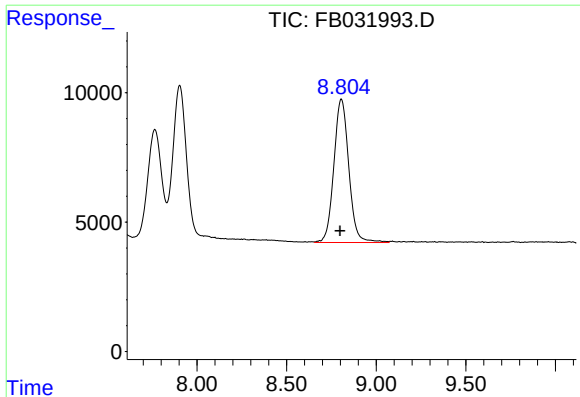

#5 AAA-TFT


R.T.: 8.806 min
Delta R.T.: 0.008 min
Response: 321635
Conc: 20.85 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701W1

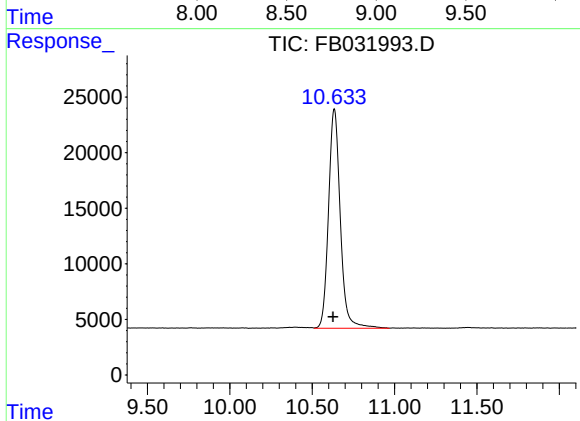


#6 Toluene

R.T.: 10.634 min
Delta R.T.: 0.008 min
Response: 980272
Conc: 27.41 ng/ml

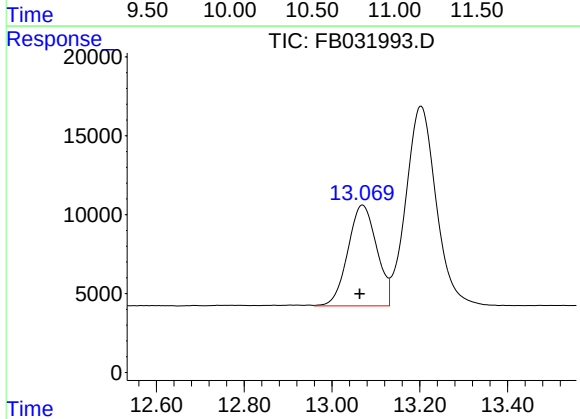


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.007 min
Response: 291208
Conc: 9.22 ng/ml

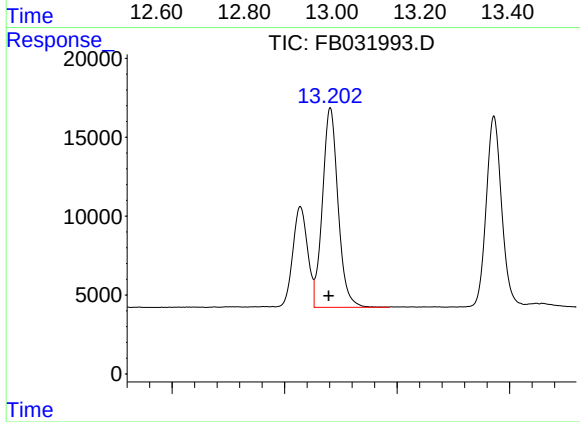

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: 0.008 min
Response: 609246
Conc: 18.57 ng/ml

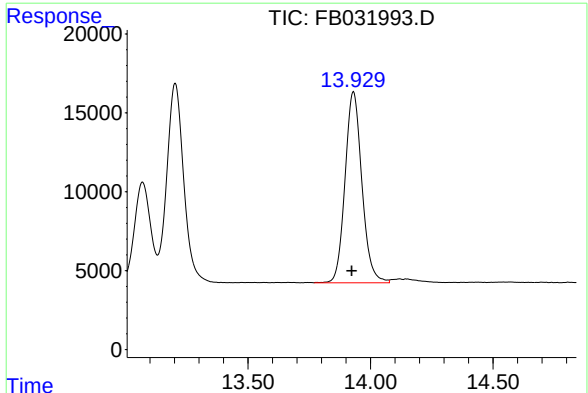

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: 0.008 min
Response: 579107
Conc: 18.66 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701W1

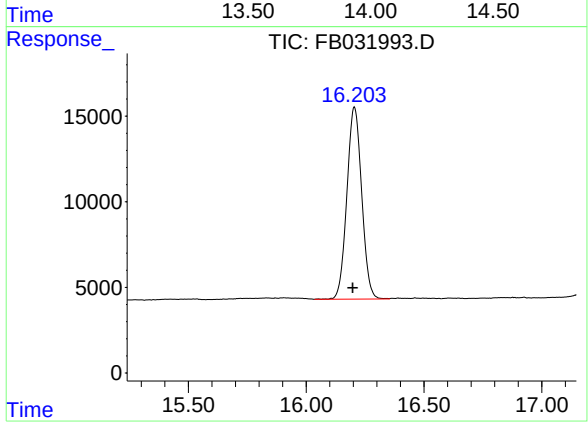

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: 0.007 min
Response: 489941
Conc: 18.53 ng/ml