

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070219\
 Data File : FB021617.D
 Signal(s) : FID2B.CH
 Acq On : 2 Jul 2019 11:48
 Operator : MJ/SJ
 Sample : BSF0702S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 02 13:34:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.989	284028	20.542 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.861	999006	29.264 ng/ml
2) t	2,2,4-Trimethylpentane	7.609	946610	30.632 ng/ml
3) t	n-Heptane	7.948	297726	10.172 ng/ml
4) t	Benzene	8.083	347271	10.346 ng/ml
6) t	Toluene	10.830	714762	31.291 ng/ml
7) t	Ethylbenzene	13.275	245124	10.355 ng/ml
8) t	m-Xylene	13.408	524872	20.708 ng/ml
9) t	O-Xylene	14.137	546349	20.832 ng/ml
10) t	1,2,4-Trimethylbenzene	16.417	557783	21.230 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070219\
Data File : FB021617.D
Signal(s) : FID2B.CH
Acq On : 2 Jul 2019 11:48
Operator : MJ/SJ
Sample : BSF0702S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 02 13:34:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

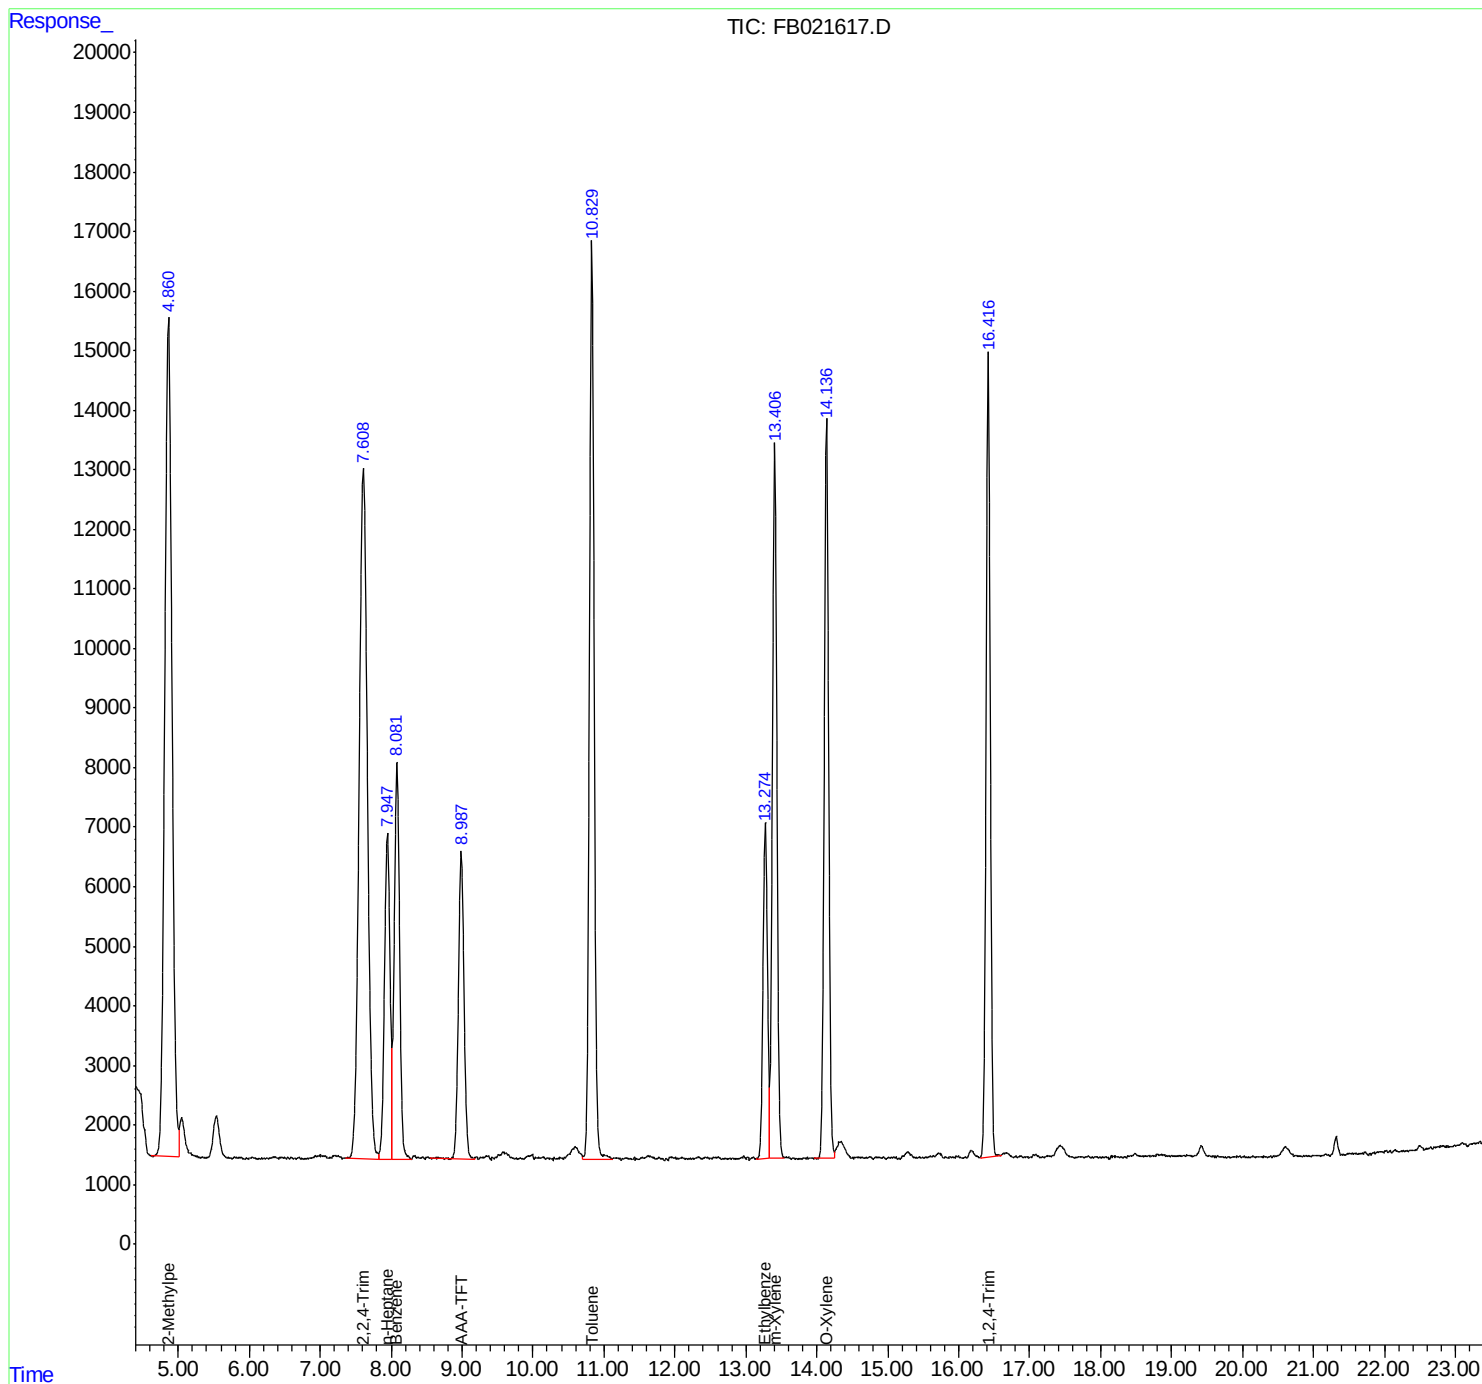

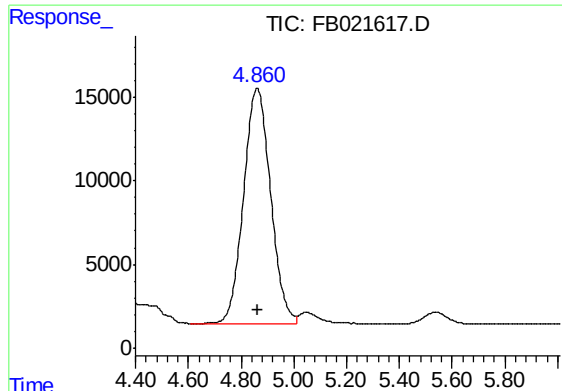


#1 2-Methylpentane

R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 999006
Conc: 29.26 ng/ml

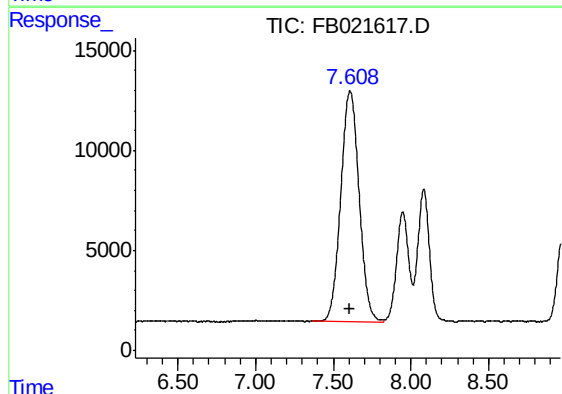


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: 0.001 min
Response: 946610
Conc: 30.63 ng/ml

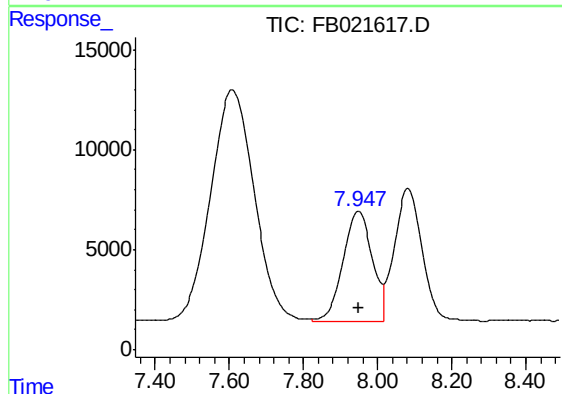


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: 0.000 min
Response: 297726
Conc: 10.17 ng/ml

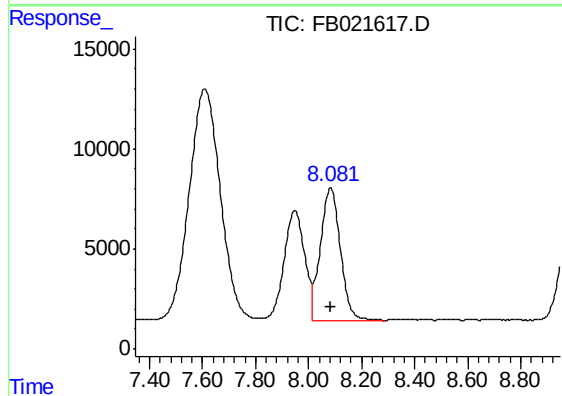


#4 Benzene

R.T.: 8.083 min
Delta R.T.: 0.000 min
Response: 347271
Conc: 10.35 ng/ml

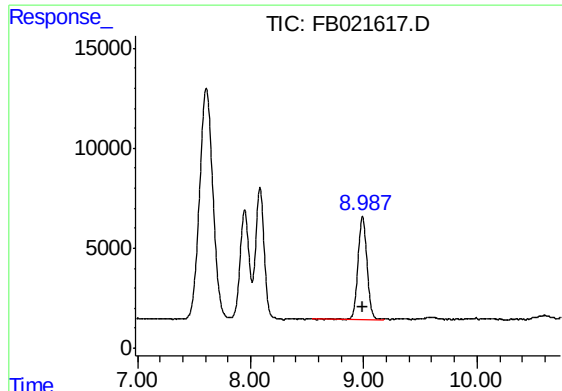


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 284028
Conc: 20.54 ng/ml

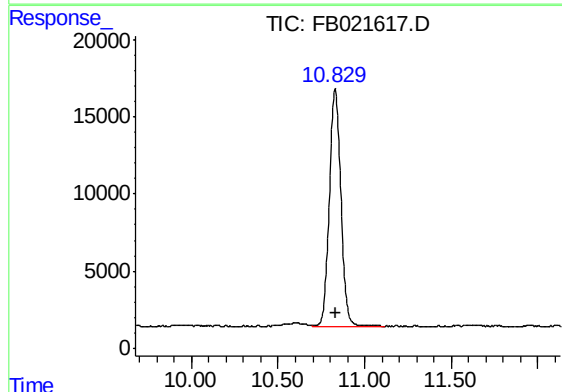


#6 Toluene

R.T.: 10.830 min
Delta R.T.: 0.000 min
Response: 714762
Conc: 31.29 ng/ml

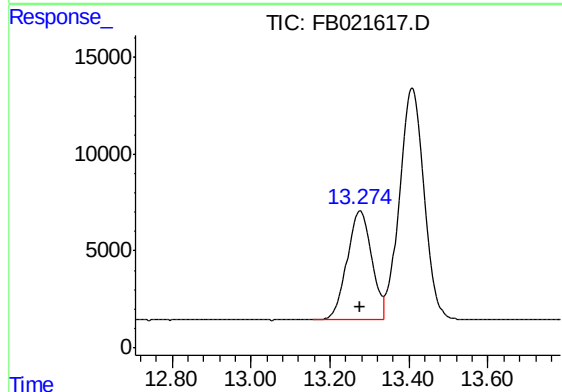


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: 0.000 min
Response: 245124
Conc: 10.35 ng/ml

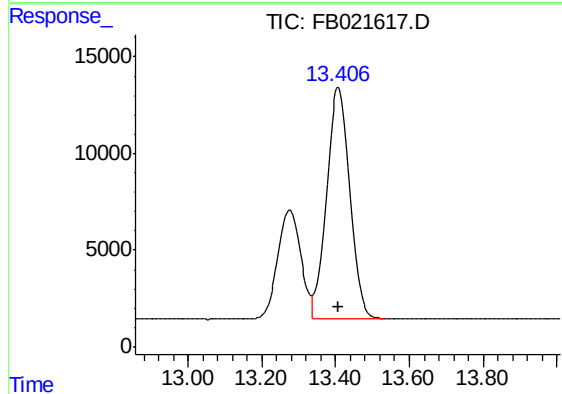


#8 m-Xylene

R.T.: 13.408 min
Delta R.T.: 0.000 min
Response: 524872
Conc: 20.71 ng/ml

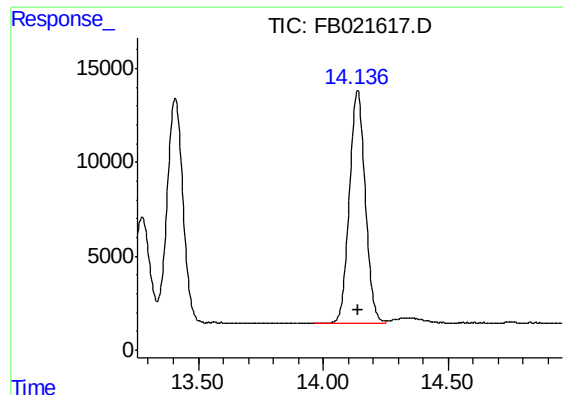

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: 0.000 min
Response: 546349
Conc: 20.83 ng/ml

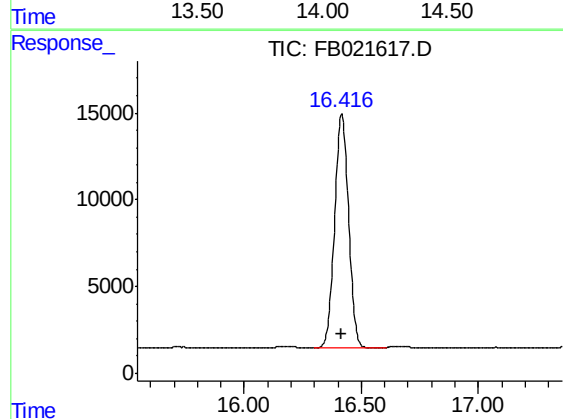

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: 0.000 min
Response: 557783
Conc: 21.23 ng/ml