

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070220\
 Data File : FB024532.D
 Signal(s) : FID2B.CH
 Acq On : 2 Jul 2020 12:01
 Operator : DD/AJ
 Sample : BSF0702S1
 Misc : 5.02gm/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 03 01:09:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	510664	21.107 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	942660	29.492 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1017505	30.352 ng/ml
3) t n-Heptane	7.758	334936	9.904 ng/ml
4) t Benzene	7.893	407523	10.081 ng/ml
6) t Toluene	10.631	1170551	29.786 ng/ml
7) t Ethylbenzene	13.070	360882	10.284 ng/ml
8) t m-Xylene	13.203	705439	20.599 ng/ml
9) t O-Xylene	13.931	690633	20.600 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	570423	20.544 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070220\
Data File : FB024532.D
Signal(s) : FID2B.CH
Acq On : 2 Jul 2020 12:01
Operator : DD/AJ
Sample : BSF0702S1
Misc : 5.02gm/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 03 01:09:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

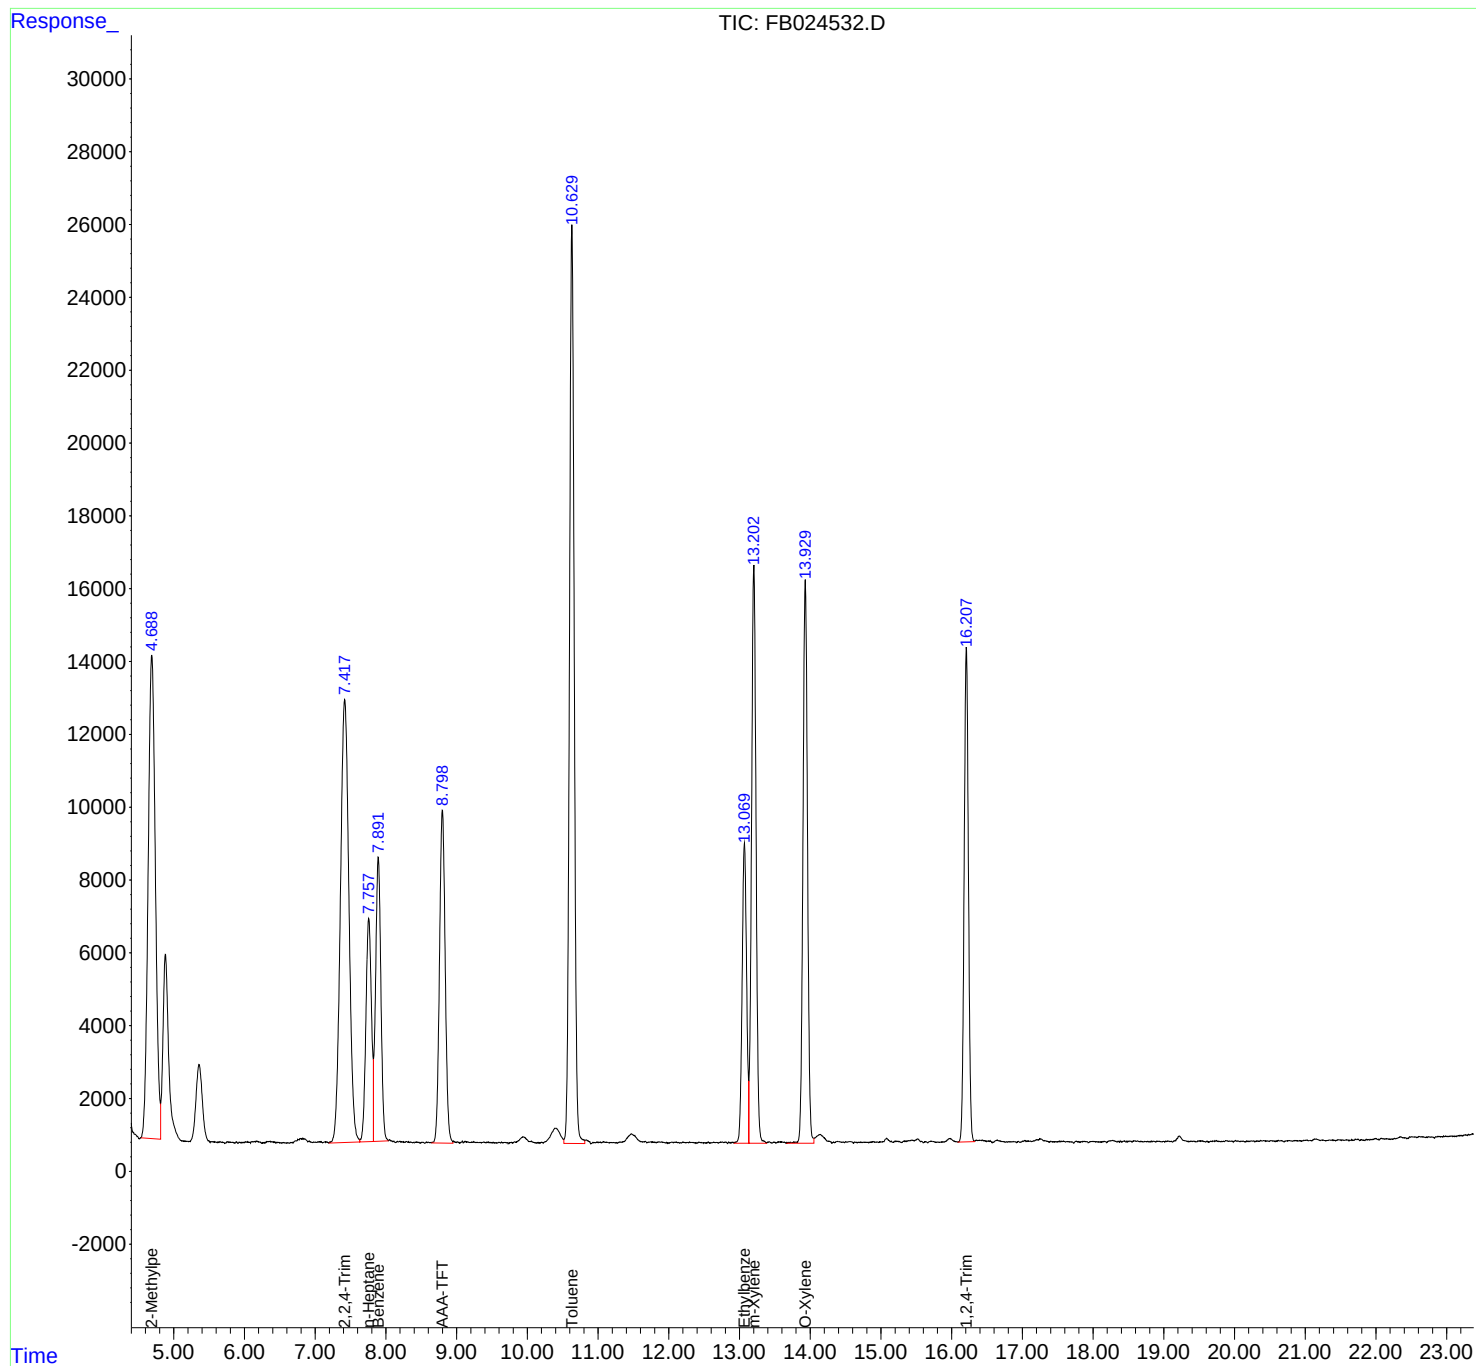

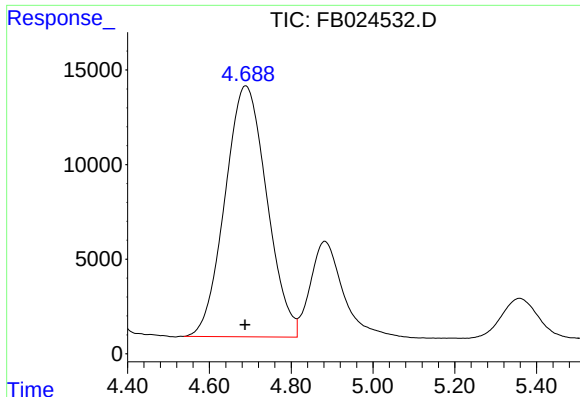


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.002 min
Response: 942660
Conc: 29.49 ng/ml

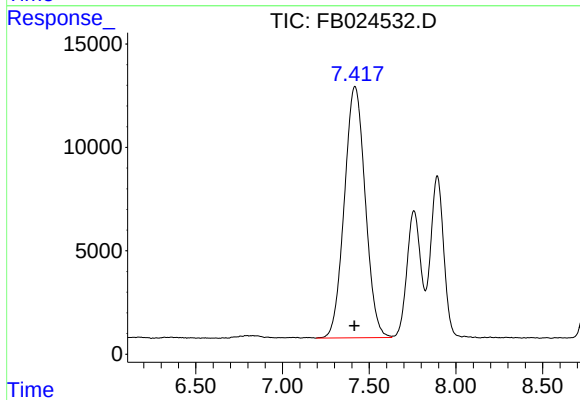


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.002 min
Response: 1017505
Conc: 30.35 ng/ml

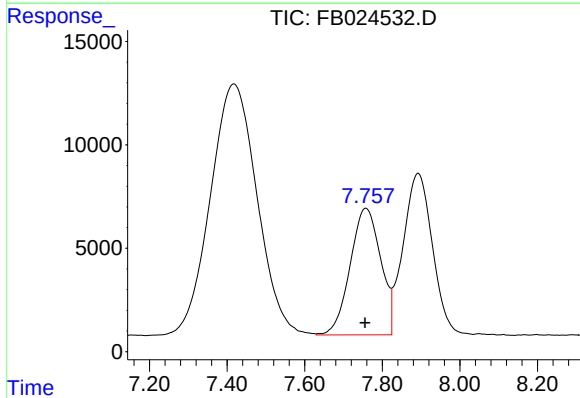


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.003 min
Response: 334936
Conc: 9.90 ng/ml

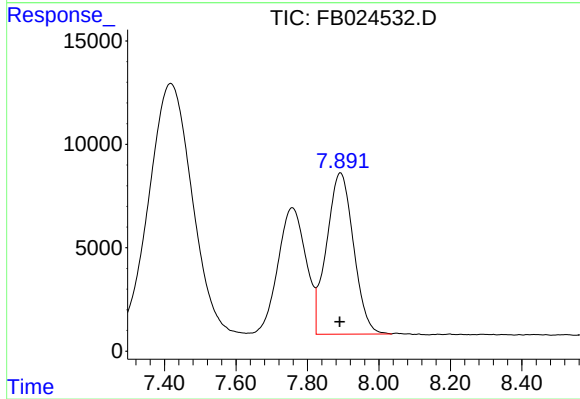


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.003 min
Response: 407523
Conc: 10.08 ng/ml

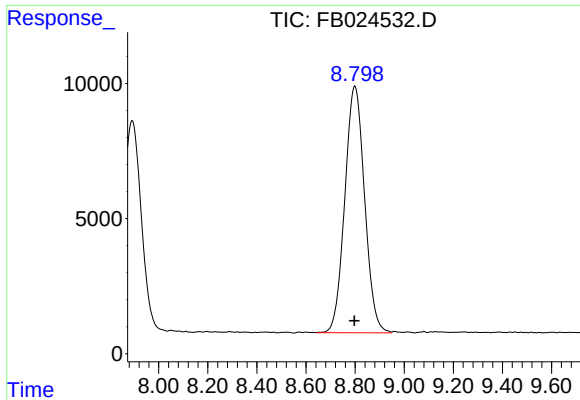


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.002 min
Response: 510664
Conc: 21.11 ng/ml

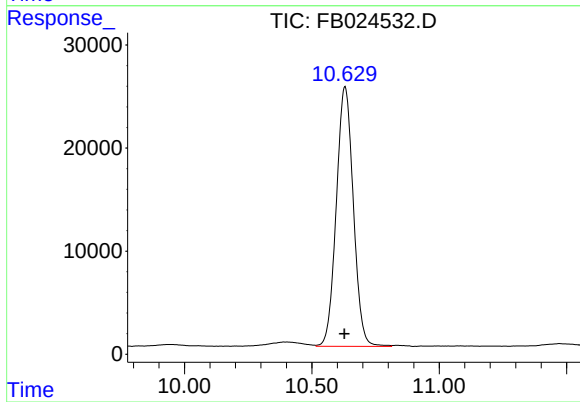


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.002 min
Response: 1170551
Conc: 29.79 ng/ml

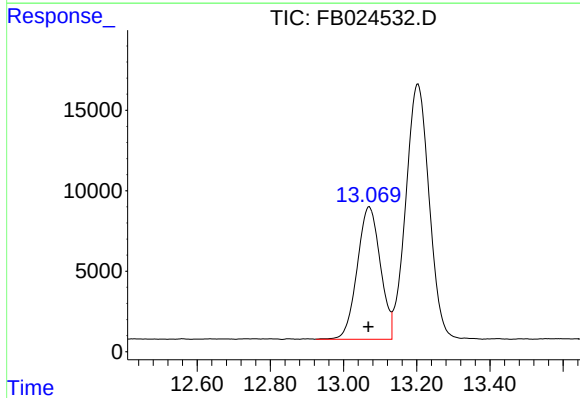


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.003 min
Response: 360882
Conc: 10.28 ng/ml

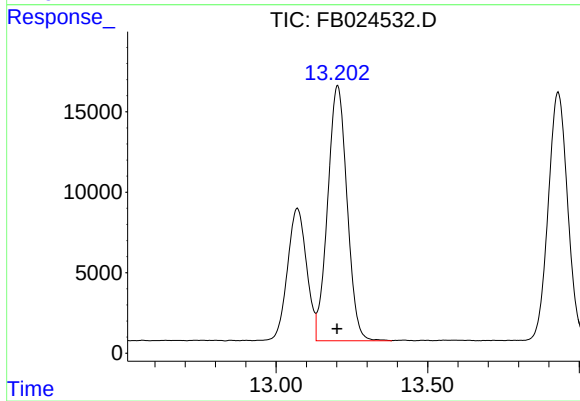


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.002 min
Response: 705439
Conc: 20.60 ng/ml

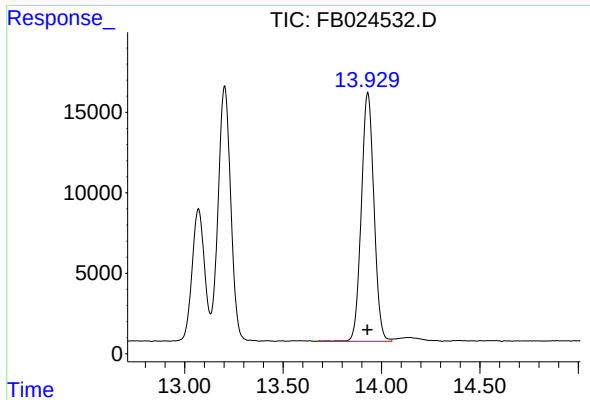

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.002 min
Response: 690633
Conc: 20.60 ng/ml

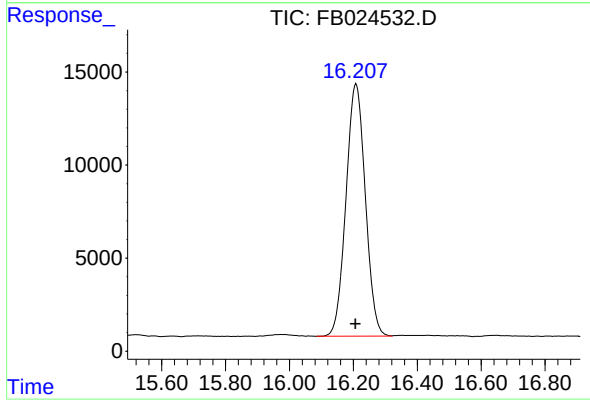

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.002 min
Response: 570423
Conc: 20.54 ng/ml