

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070319\
 Data File : FB021631.D
 Signal(s) : FID2B.CH
 Acq On : 3 Jul 2019 13:30
 Operator : MJ/SJ
 Sample : BSF0703S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 03 22:25:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.989	277679	20.083 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.862	941126	27.569 ng/ml
2) t 2,2,4-Trimethylpentane	7.609	894202	28.936 ng/ml
3) t n-Heptane	7.948	278989	9.532 ng/ml
4) t Benzene	8.083	328614	9.791 ng/ml
6) t Toluene	10.830	682202	29.865 ng/ml
7) t Ethylbenzene	13.275	234251	9.895 ng/ml
8) t m-Xylene	13.408	501114	19.771 ng/ml
9) t O-Xylene	14.137	520706	19.854 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	528639	20.120 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070319\
Data File : FB021631.D
Signal(s) : FID2B.CH
Acq On : 3 Jul 2019 13:30
Operator : MJ/SJ
Sample : BSF0703S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 03 22:25:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

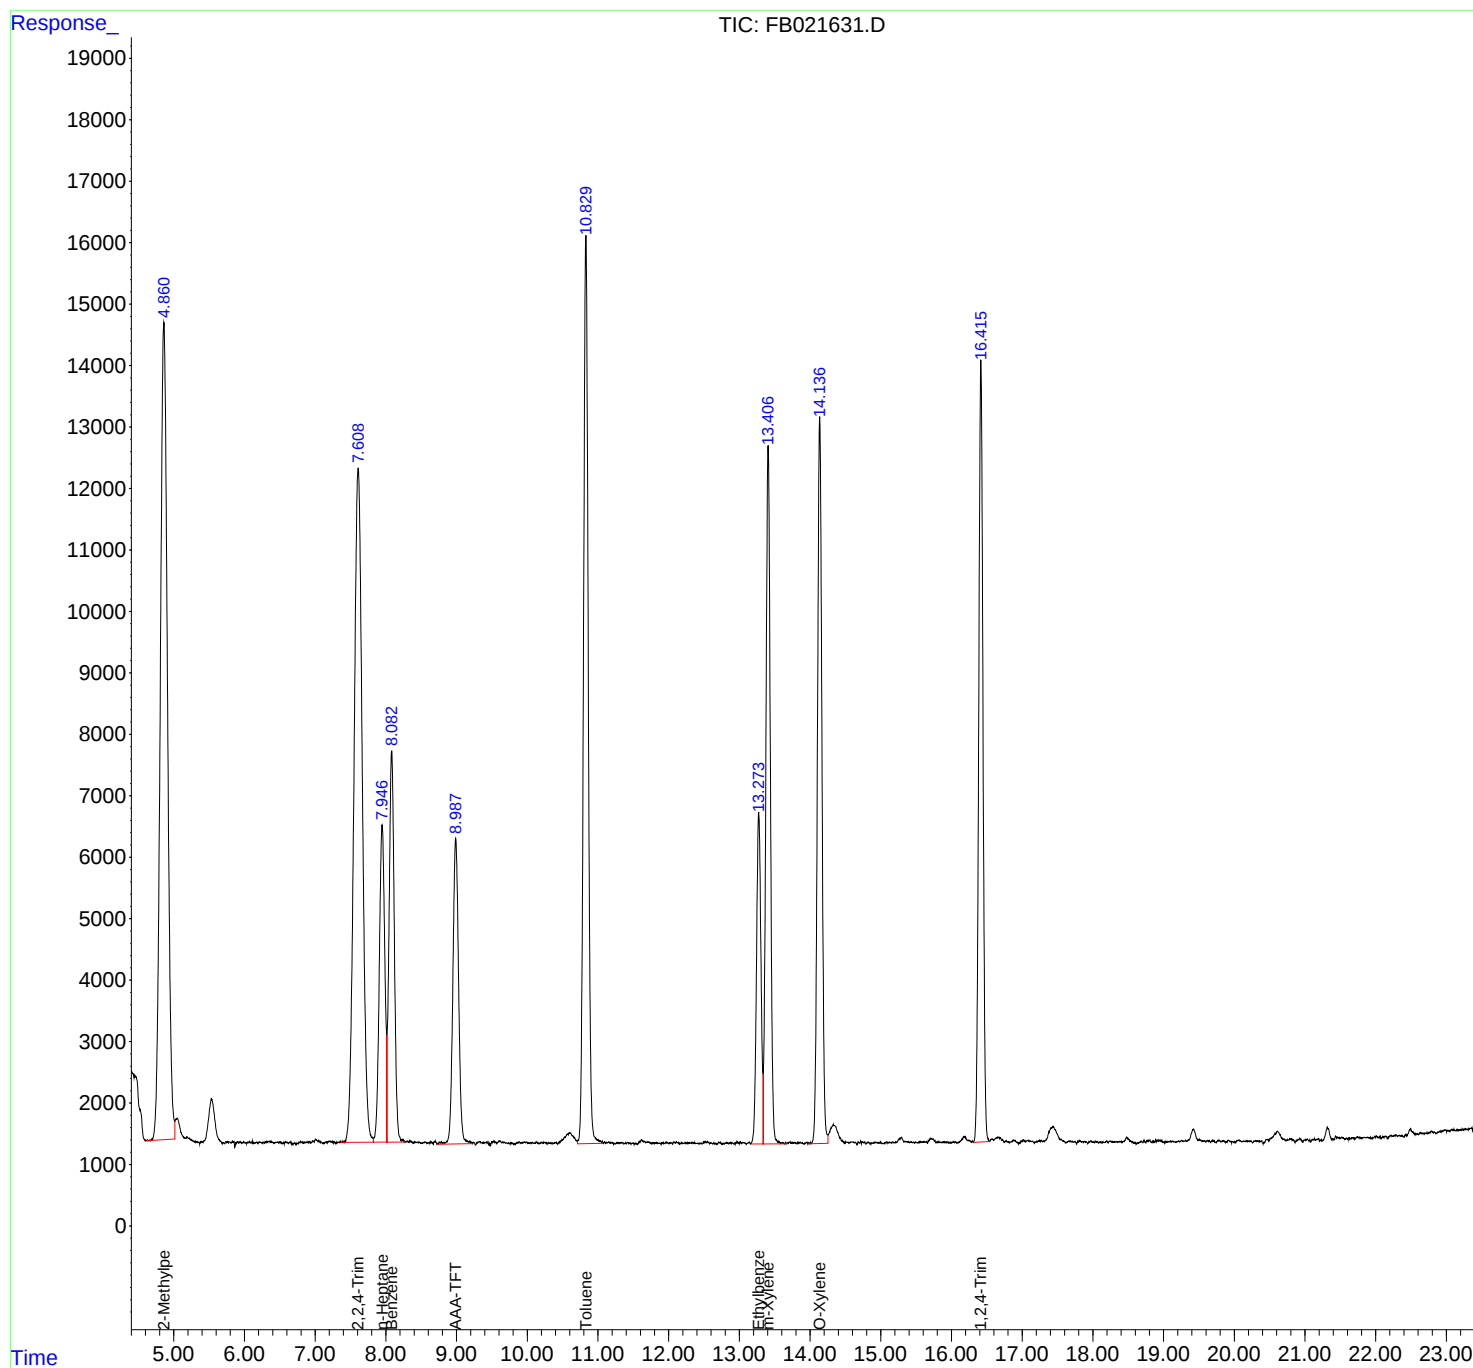

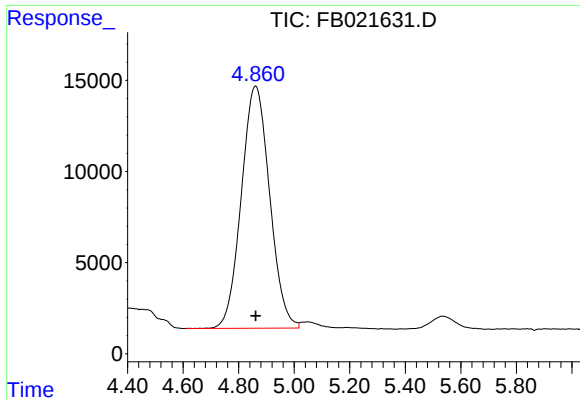


#1 2-Methylpentane

R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 941126
Conc: 27.57 ng/ml

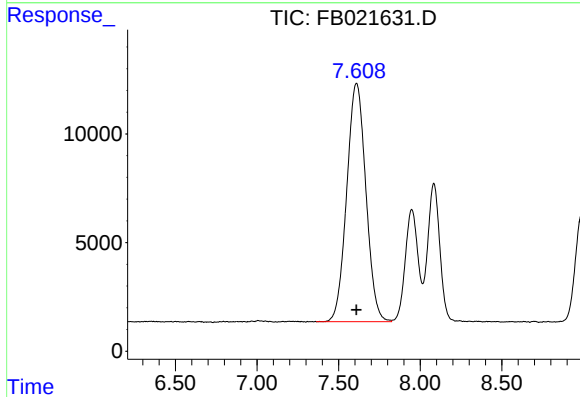


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: 0.002 min
Response: 894202
Conc: 28.94 ng/ml

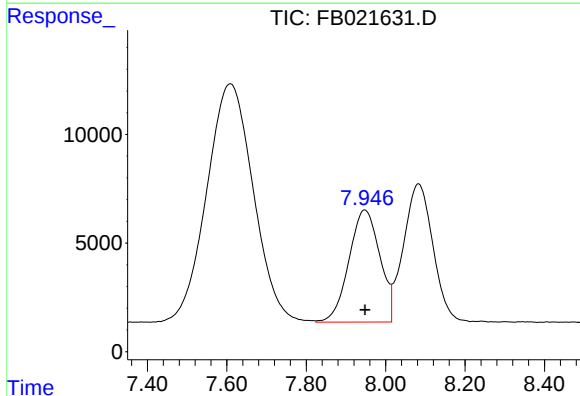


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: 0.000 min
Response: 278989
Conc: 9.53 ng/ml

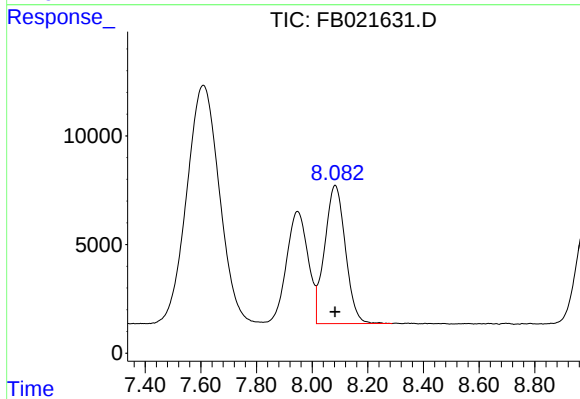


#4 Benzene

R.T.: 8.083 min
Delta R.T.: 0.001 min
Response: 328614
Conc: 9.79 ng/ml

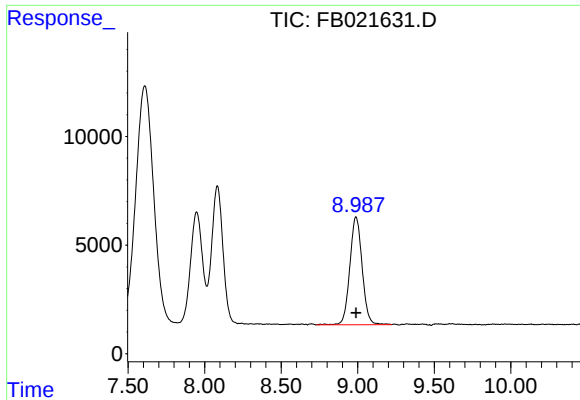


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 277679
Conc: 20.08 ng/ml

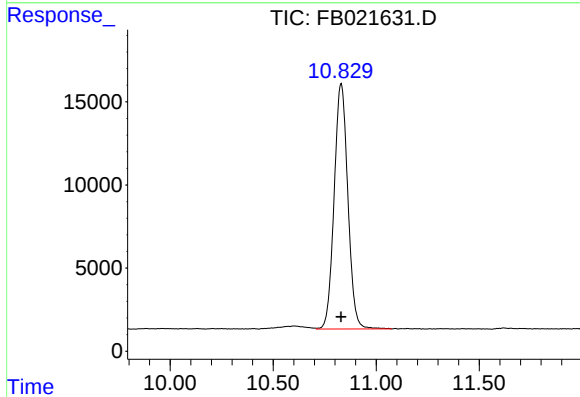


#6 Toluene

R.T.: 10.830 min
Delta R.T.: 0.000 min
Response: 682202
Conc: 29.87 ng/ml

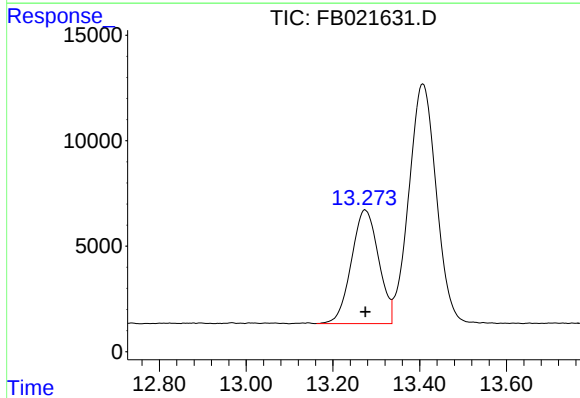


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: 0.000 min
Response: 234251
Conc: 9.90 ng/ml

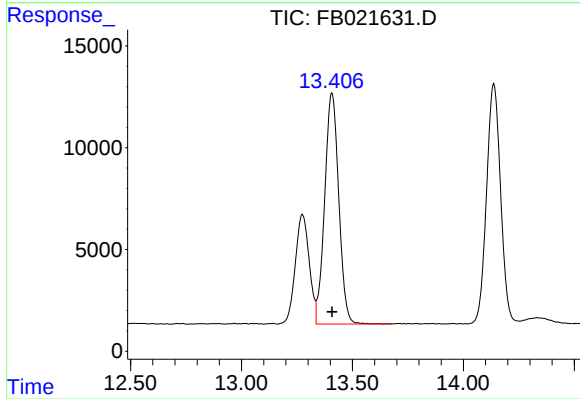


#8 m-Xylene

R.T.: 13.408 min
Delta R.T.: 0.000 min
Response: 501114
Conc: 19.77 ng/ml

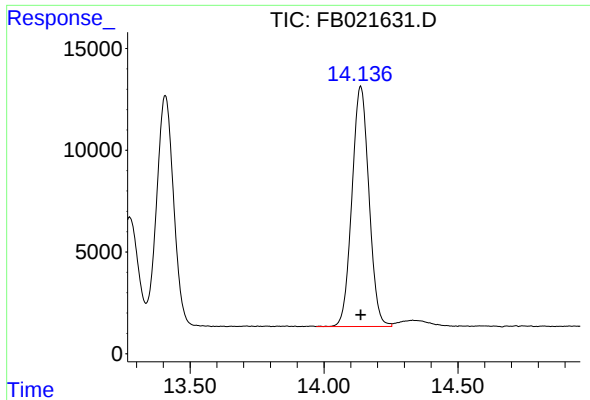

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: 0.000 min
Response: 520706
Conc: 19.85 ng/ml

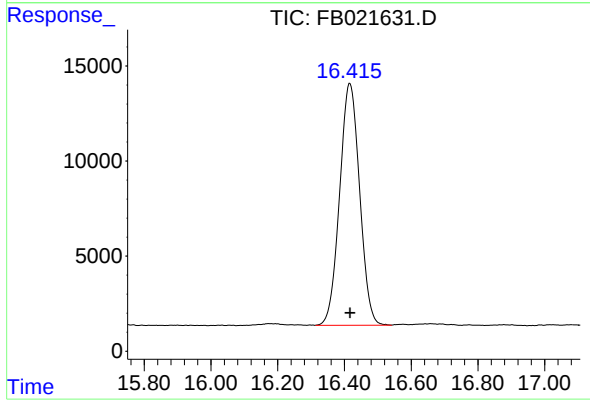

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: 0.000 min
Response: 528639
Conc: 20.12 ng/ml