

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070319\
 Data File : FB021634.D
 Signal(s) : FID2B.CH
 Acq On : 3 Jul 2019 15:57
 Operator : MJ/SJ
 Sample : K3618-01MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 03 22:26:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.990	269686	19.505 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.863	720140	21.095 ng/ml
2) t 2,2,4-Trimethylpentane	7.610	576344	18.650 ng/ml
3) t n-Heptane	7.949	184584	6.307 ng/ml
4) t Benzene	8.084	292552	8.716 ng/ml
6) t Toluene	10.831	598899	26.219 ng/ml
7) t Ethylbenzene	13.275	241153	10.187 ng/ml
8) t m-Xylene	13.409	446308	17.609 ng/ml
9) t O-Xylene	14.138	451688	17.222 ng/ml
10) t 1,2,4-Trimethylbenzene	16.418	421902	16.058 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070319\
Data File : FB021634.D
Signal(s) : FID2B.CH
Acq On : 3 Jul 2019 15:57
Operator : MJ/SJ
Sample : K3618-01MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 03 22:26:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

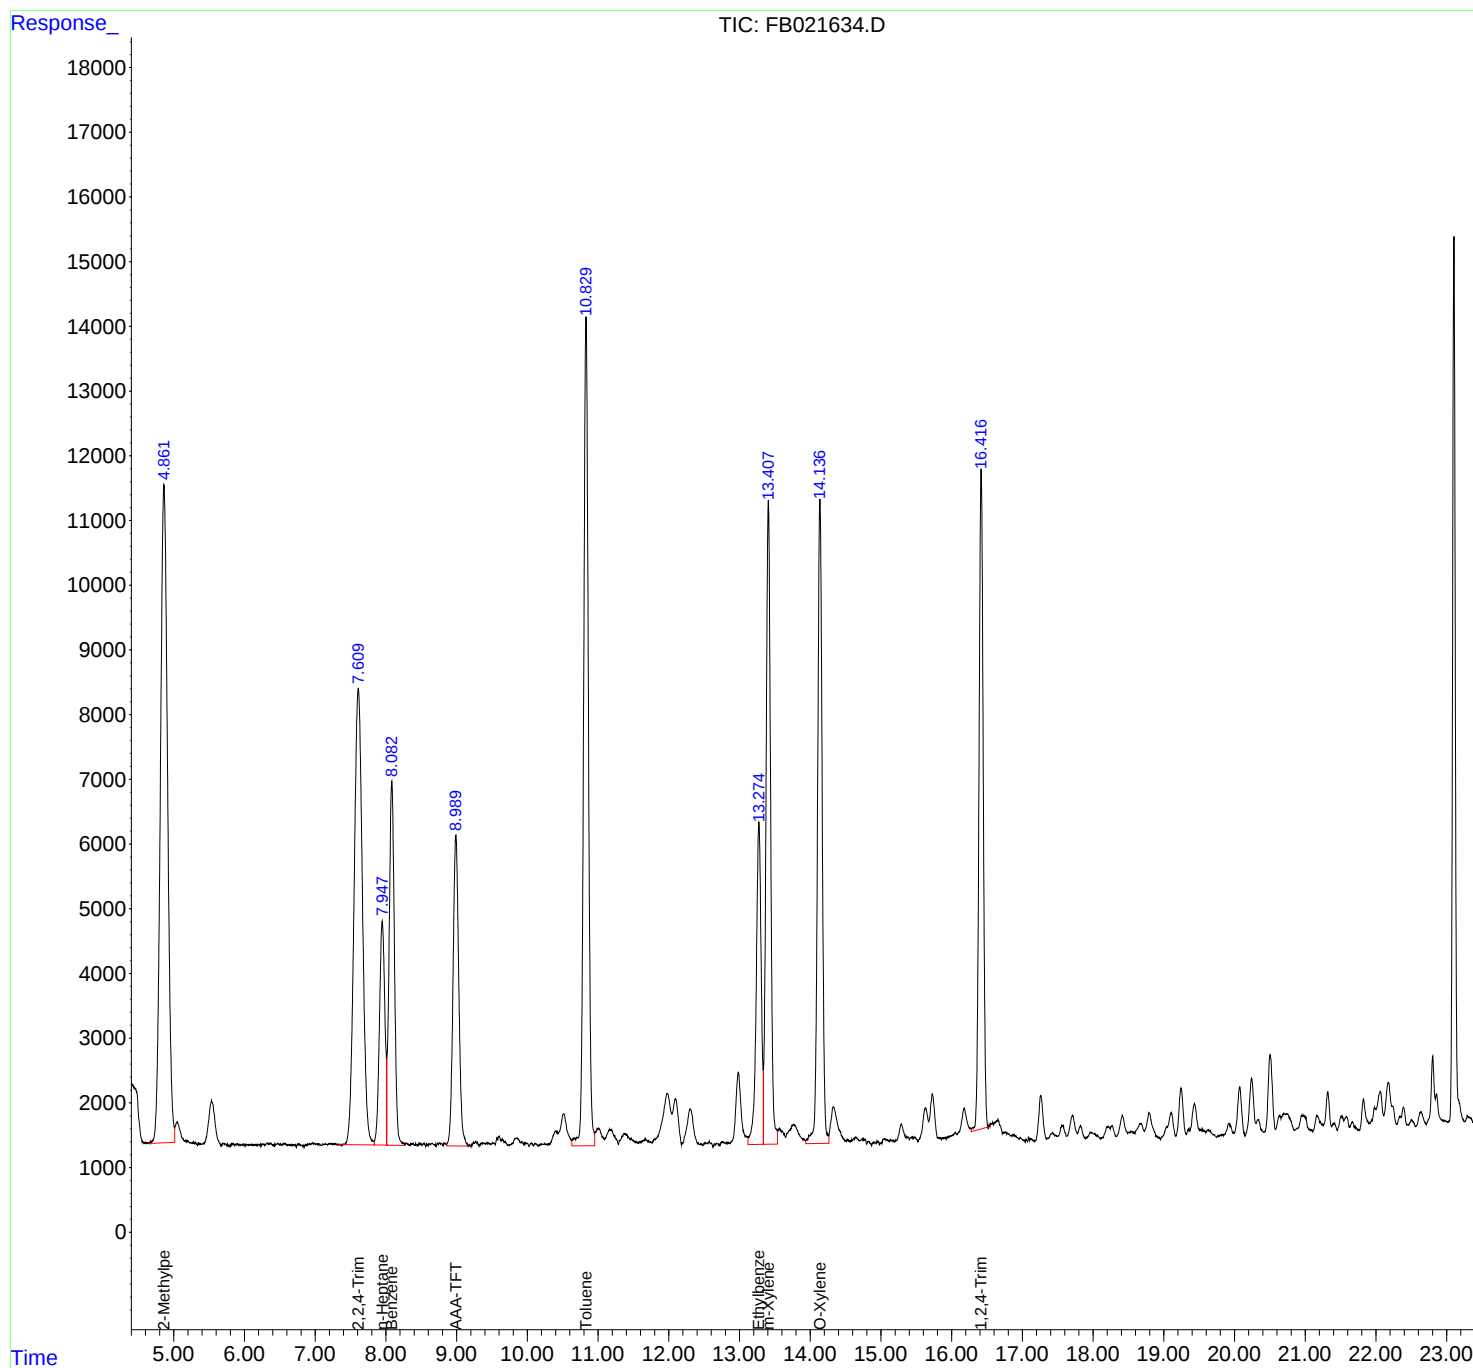

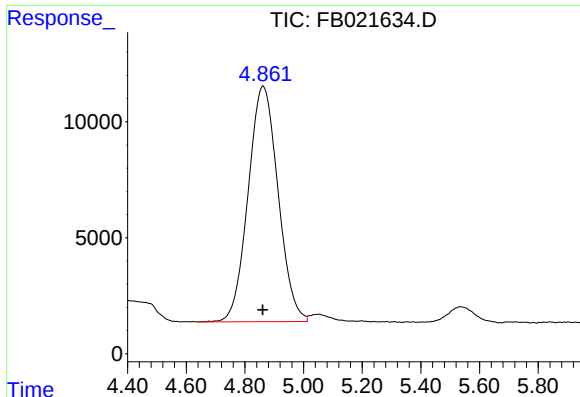


#1 2-Methylpentane

R.T.: 4.863 min
Delta R.T.: 0.002 min
Response: 720140
Conc: 21.10 ng/ml

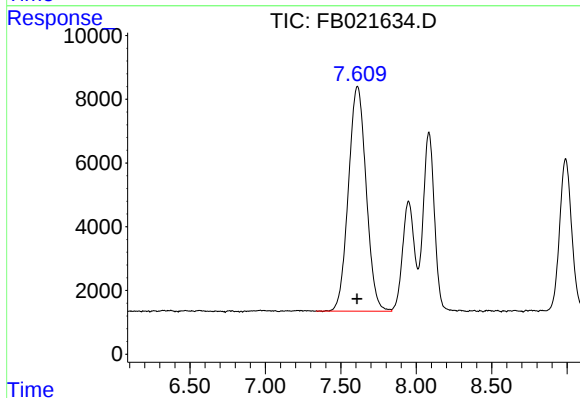


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: 0.003 min
Response: 576344
Conc: 18.65 ng/ml

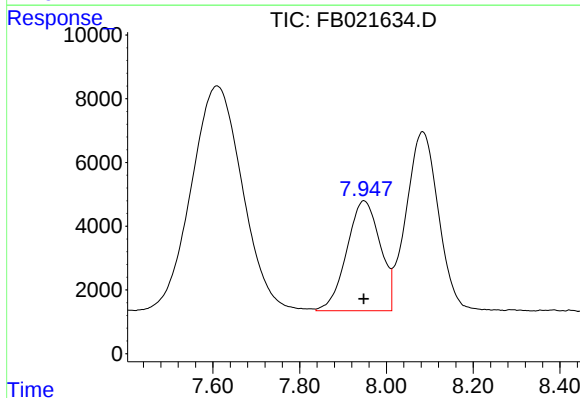


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: 0.001 min
Response: 184584
Conc: 6.31 ng/ml

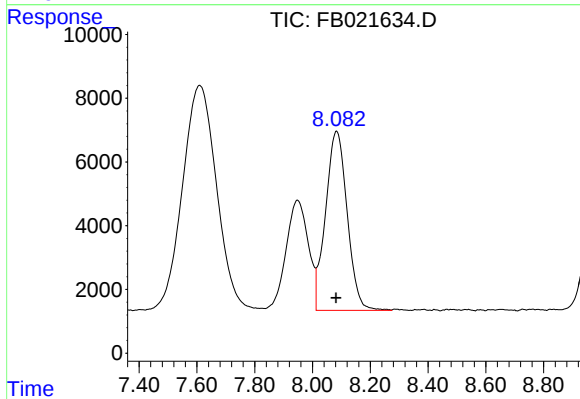


#4 Benzene

R.T.: 8.084 min
Delta R.T.: 0.002 min
Response: 292552
Conc: 8.72 ng/ml

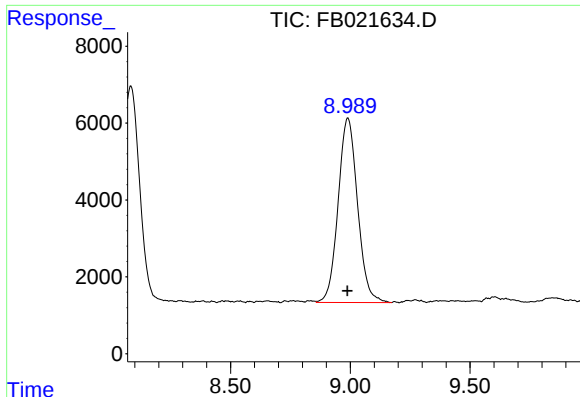


#5 AAA-TFT

R.T.: 8.990 min
Delta R.T.: 0.002 min
Response: 269686
Conc: 19.50 ng/ml

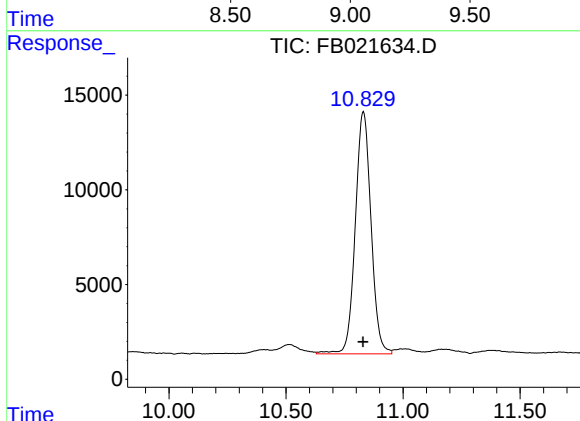


#6 Toluene

R.T.: 10.831 min
Delta R.T.: 0.001 min
Response: 598899
Conc: 26.22 ng/ml

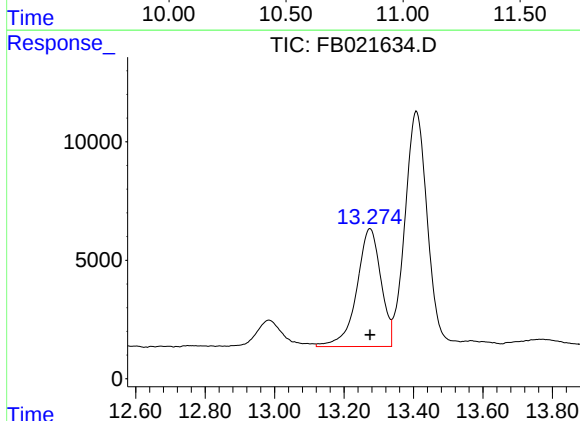


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: 0.000 min
Response: 241153
Conc: 10.19 ng/ml

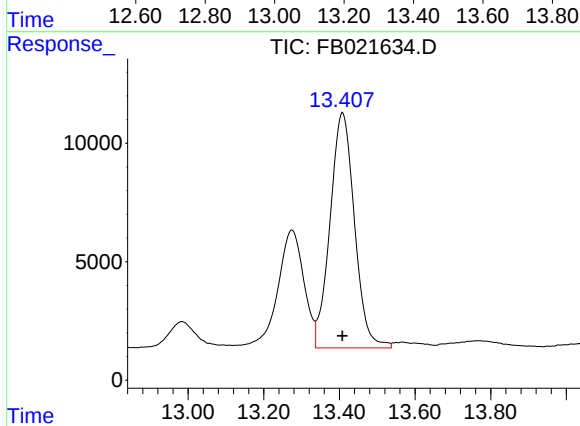


#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: 0.000 min
Response: 446308
Conc: 17.61 ng/ml

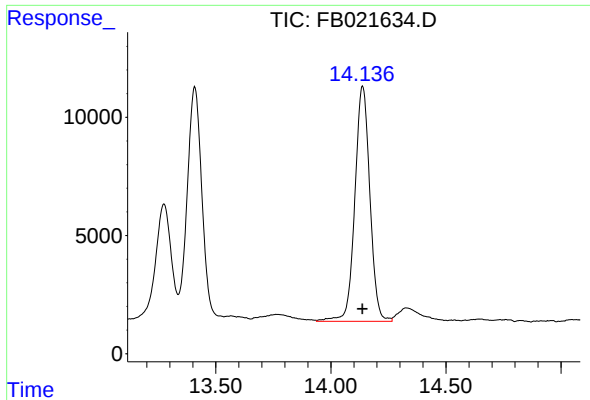

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: 0.000 min
Response: 451688
Conc: 17.22 ng/ml

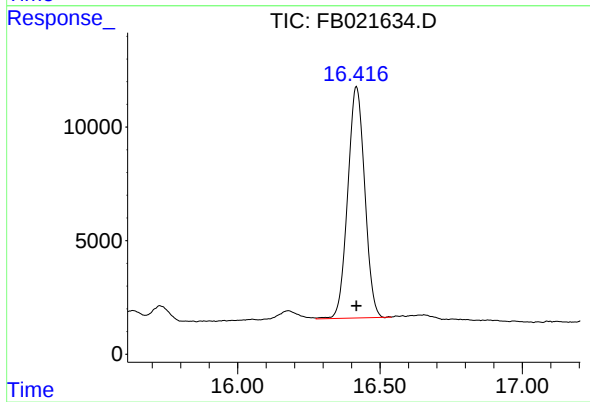

#10 1,2,4-Trimethylbenzene

R.T.: 16.418 min
Delta R.T.: 0.000 min
Response: 421902
Conc: 16.06 ng/ml