

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070522\
 Data File : FB027622.D
 Signal(s) : FID2B.CH
 Acq On : 5 Jul 2022 11:26
 Operator : AJ/MA
 Sample : BSF0705S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0705S1

Integration File: SAMPLE.e
 Quant Time: Jul 06 04:35:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	224056	19.975 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	531407	31.543 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	554325	31.570 ng/ml
3) t n-Heptane	7.752	189408	10.812 ng/ml
4) t Benzene	7.888	222899	10.930 ng/ml
6) t Toluene	10.621	632357	32.660 ng/ml
7) t Ethylbenzene	13.057	193746	10.699 ng/ml
8) t m-Xylene	13.189	383129	21.493 ng/ml
9) t O-Xylene	13.916	371005	21.352 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	361436	21.040 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070522\
Data File : FB027622.D
Signal(s) : FID2B.CH
Acq On : 5 Jul 2022 11:26
Operator : AJ/MA
Sample : BSF0705S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0705S1

Integration File: SAMPLE.e
Quant Time: Jul 06 04:35:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

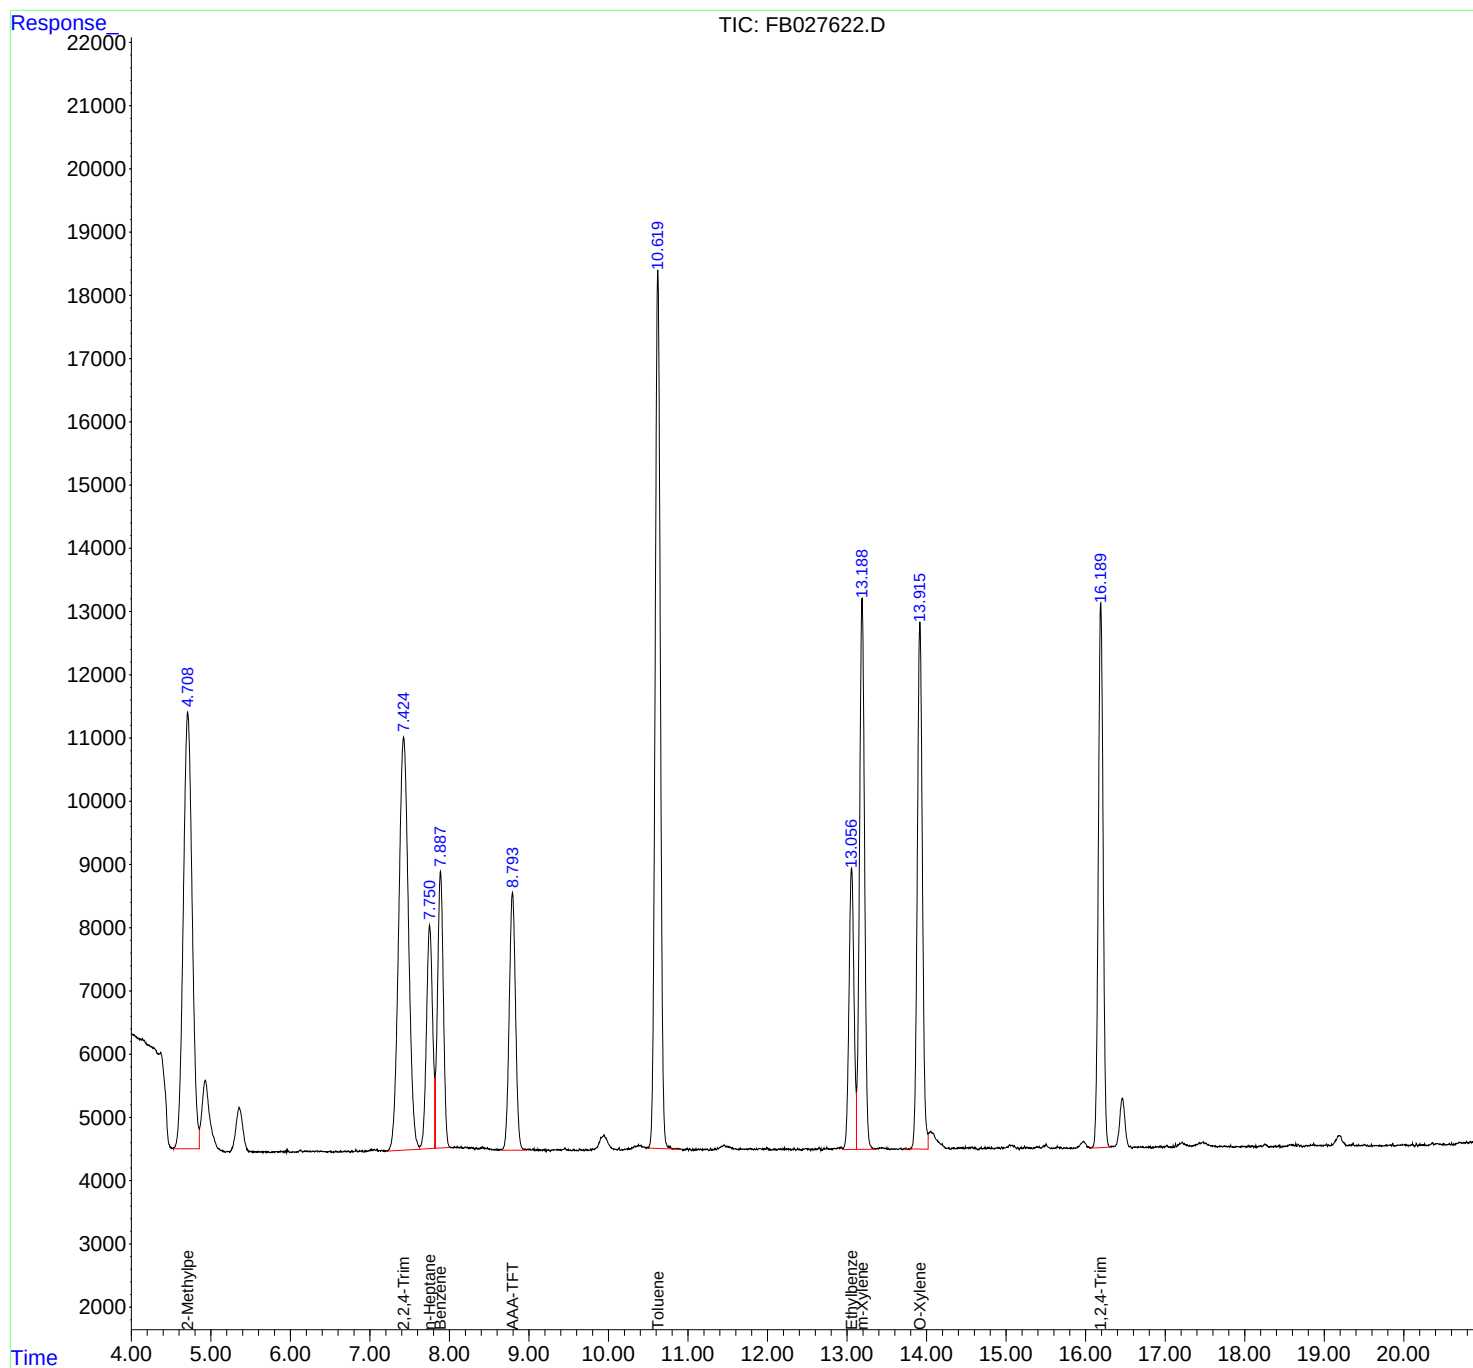


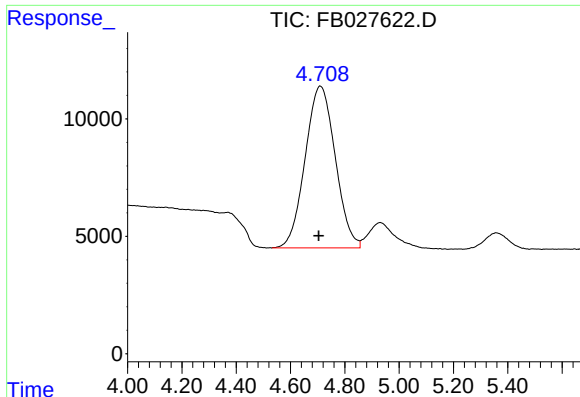

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.005 min
Response: 531407
Conc: 31.54 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0705S1

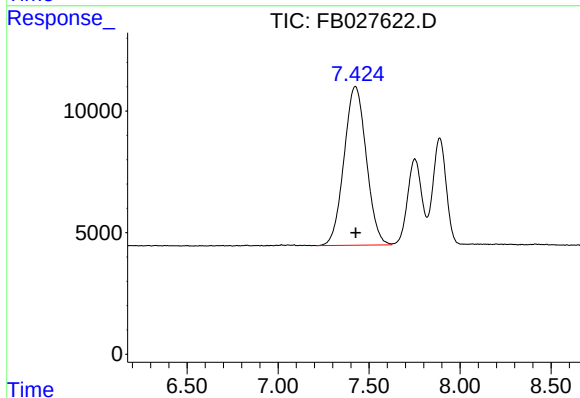


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: -0.001 min
Response: 554325
Conc: 31.57 ng/ml

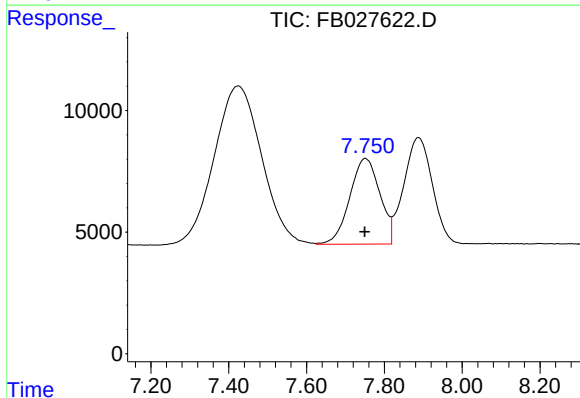


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.002 min
Response: 189408
Conc: 10.81 ng/ml

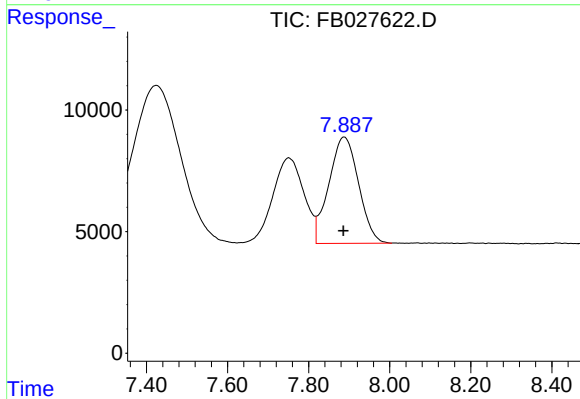

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.003 min
Response: 222899
Conc: 10.93 ng/ml

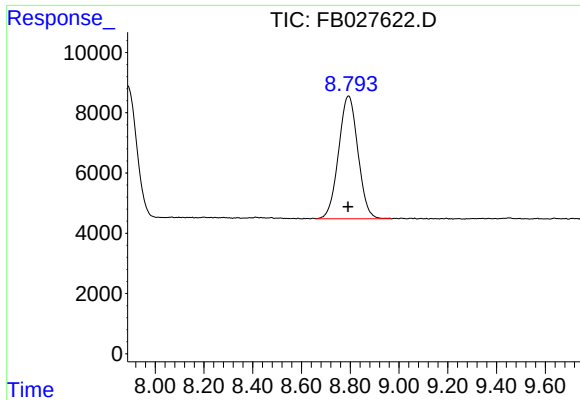

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.003 min
Response: 224056
Conc: 19.98 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0705S1

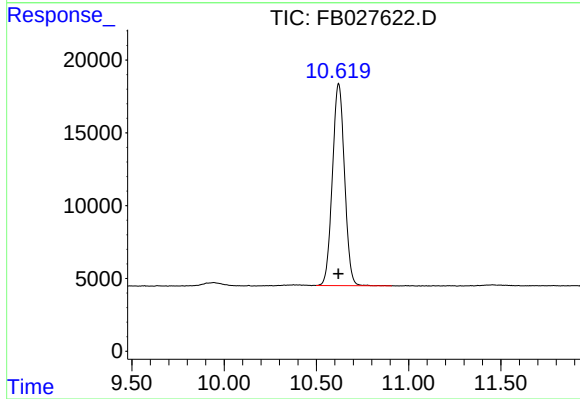


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.001 min
Response: 632357
Conc: 32.66 ng/ml

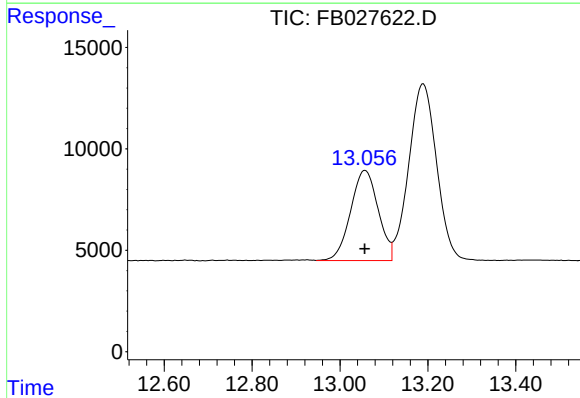


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.000 min
Response: 193746
Conc: 10.70 ng/ml

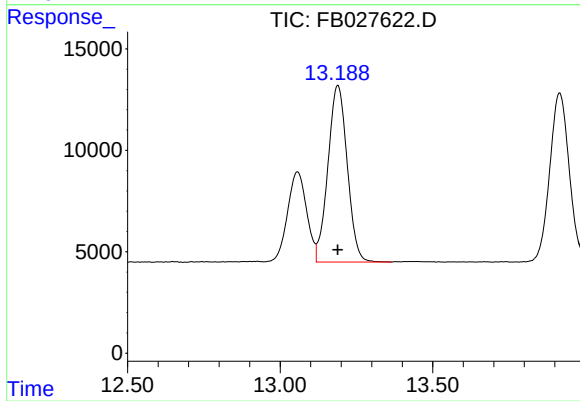

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 383129
Conc: 21.49 ng/ml

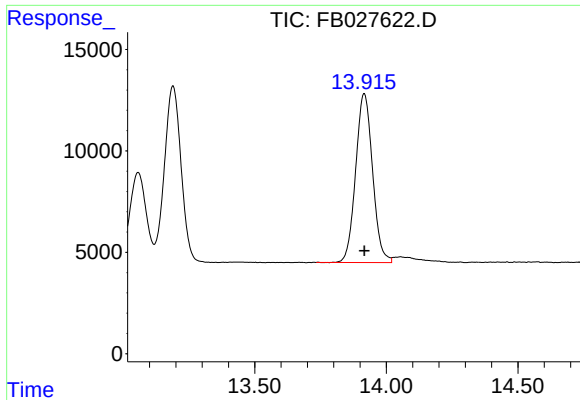

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 371005
Conc: 21.35 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0705S1

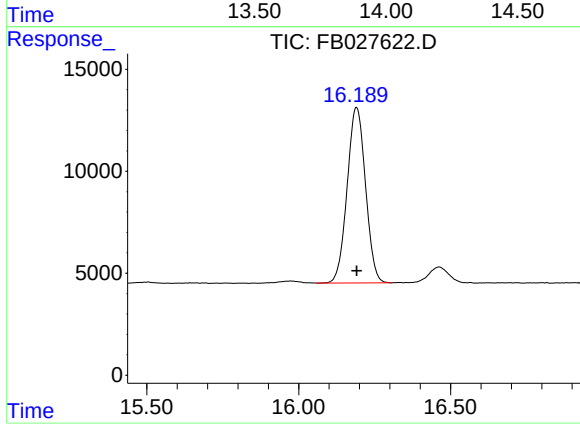

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 361436
Conc: 21.04 ng/ml