

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070522\
 Data File : FB027628.D
 Signal(s) : FID2B.CH
 Acq On : 5 Jul 2022 15:28
 Operator : AJ/MA
 Sample : BSF0705S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0705S2

Integration File: SAMPLE.e
 Quant Time: Jul 06 04:35:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	226982	20.236 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	467642	27.758 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	497933	28.359 ng/ml
3) t n-Heptane	7.755	167272	9.548 ng/ml
4) t Benzene	7.891	192909	9.460 ng/ml
6) t Toluene	10.625	558786	28.860 ng/ml
7) t Ethylbenzene	13.061	172748	9.539 ng/ml
8) t m-Xylene	13.194	341376	19.150 ng/ml
9) t O-Xylene	13.921	339205	19.521 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	323080	18.807 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070522\
Data File : FB027628.D
Signal(s) : FID2B.CH
Acq On : 5 Jul 2022 15:28
Operator : AJ/MA
Sample : BSF0705S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0705S2

Integration File: SAMPLE.e
Quant Time: Jul 06 04:35:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

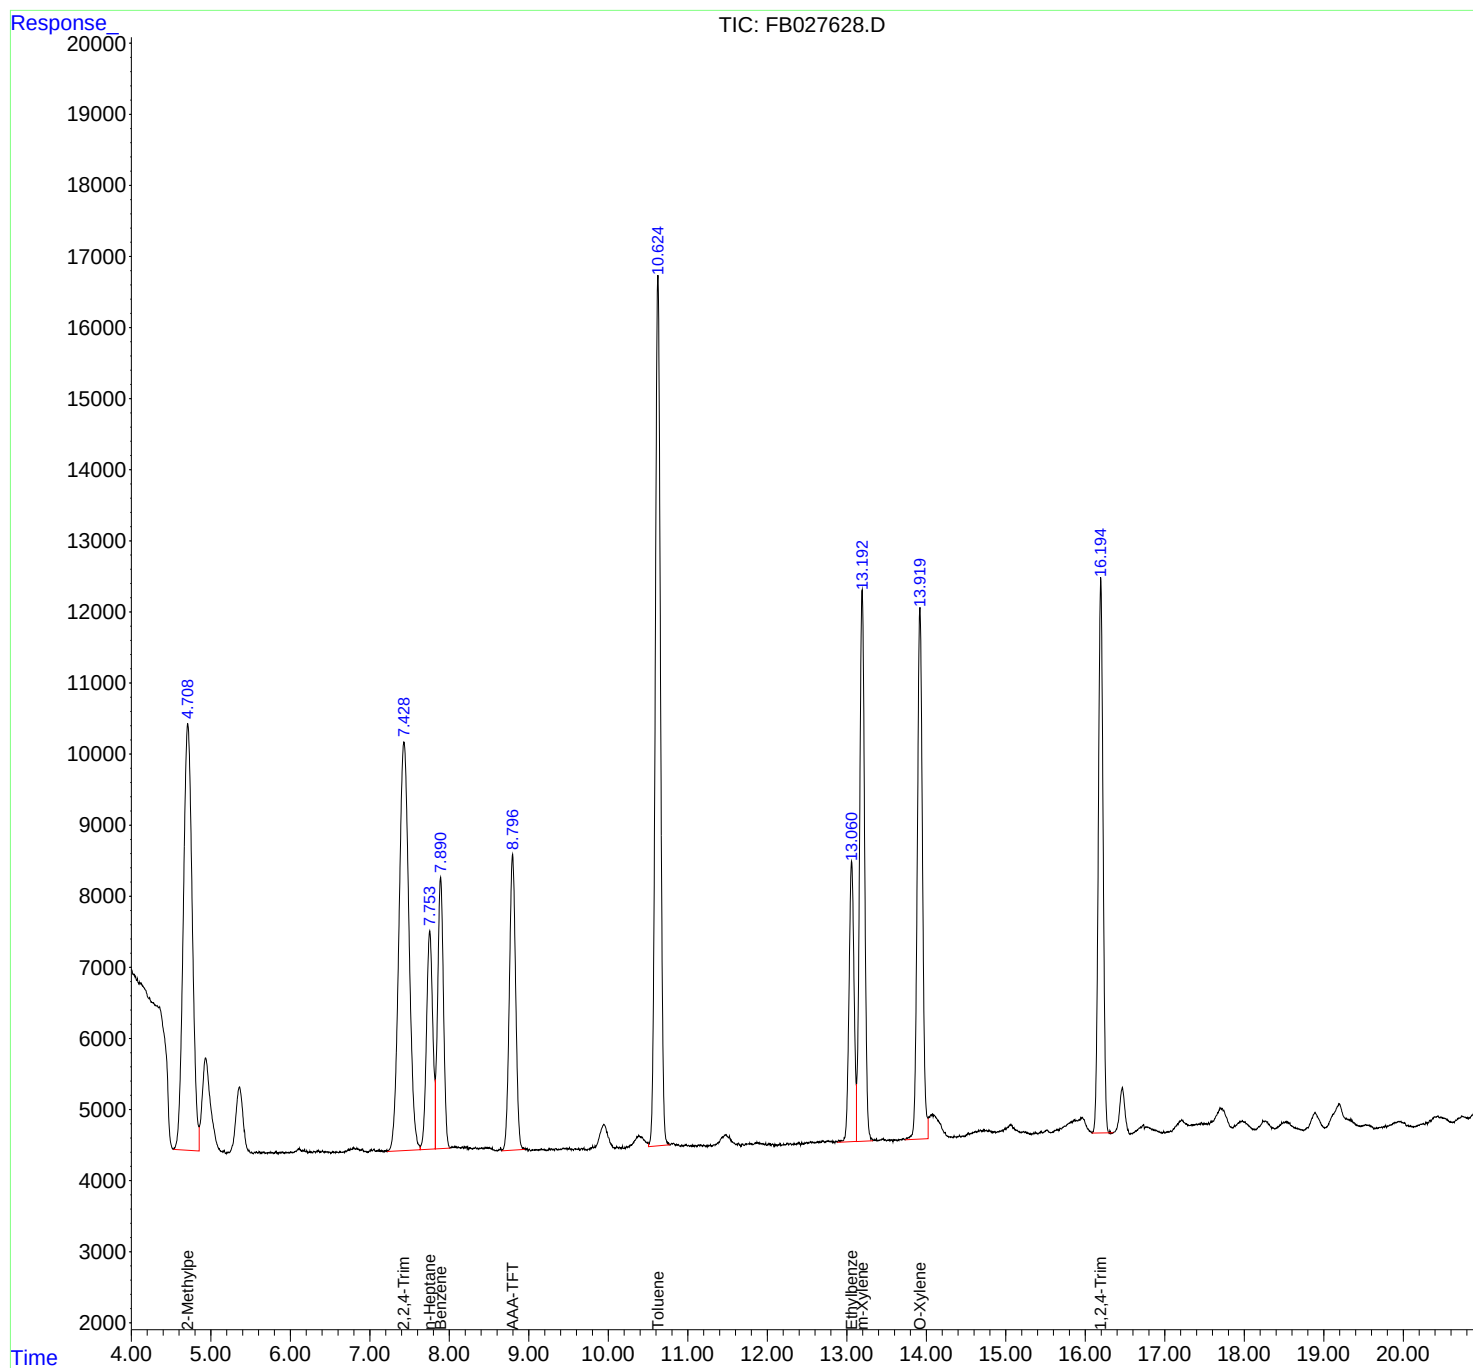


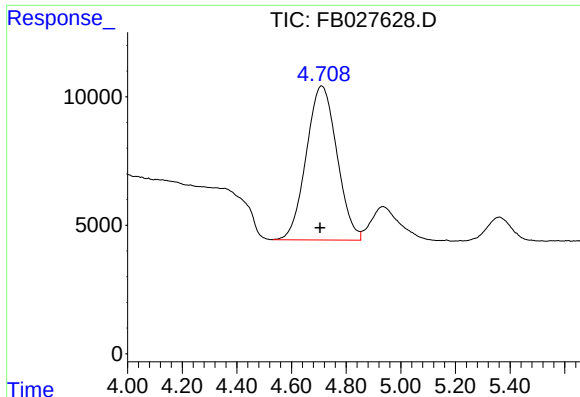

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.006 min
Response: 467642
Conc: 27.76 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0705S2

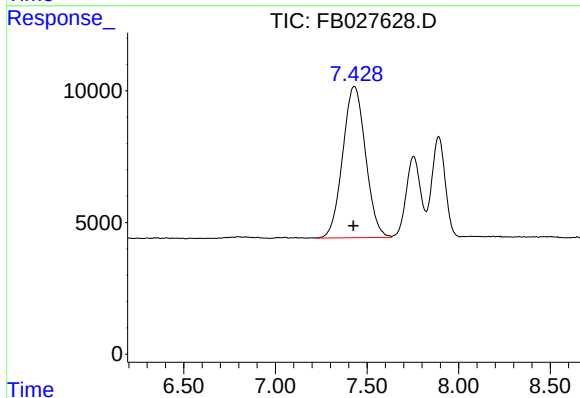


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: 0.004 min
Response: 497933
Conc: 28.36 ng/ml

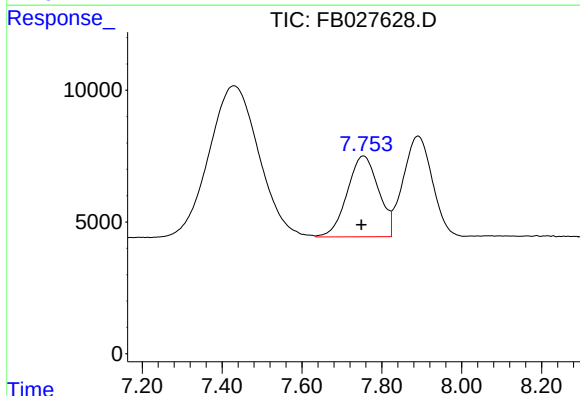


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.005 min
Response: 167272
Conc: 9.55 ng/ml

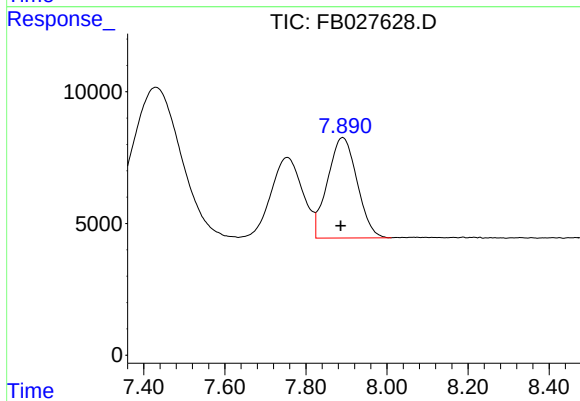

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.005 min
Response: 192909
Conc: 9.46 ng/ml

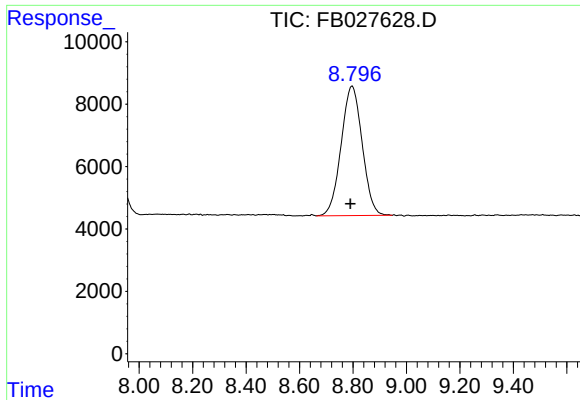

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.006 min
Response: 226982
Conc: 20.24 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0705S2

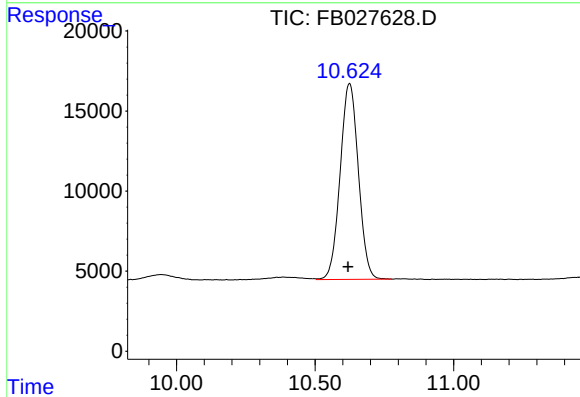


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.006 min
Response: 558786
Conc: 28.86 ng/ml

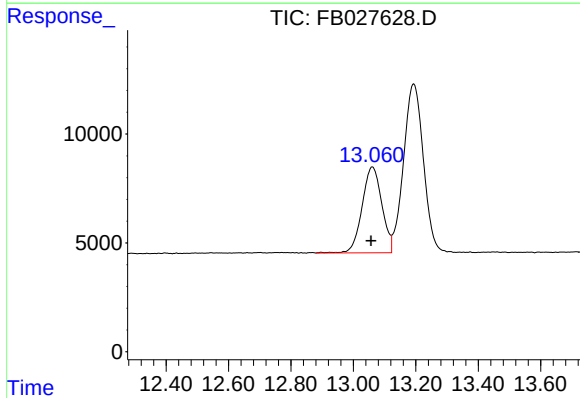


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: 0.005 min
Response: 172748
Conc: 9.54 ng/ml

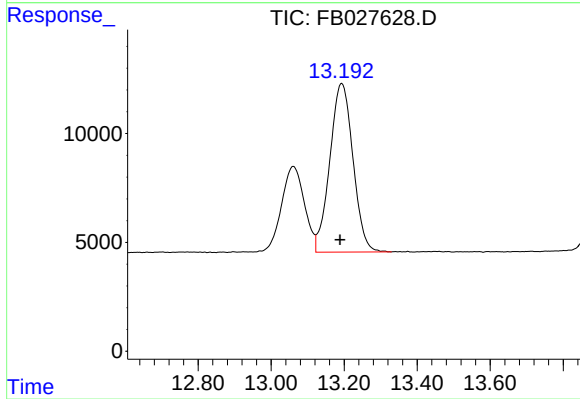

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: 0.005 min
Response: 341376
Conc: 19.15 ng/ml

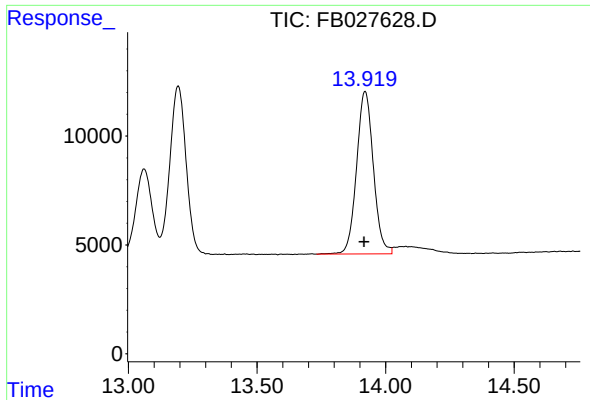

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.005 min
Response: 339205
Conc: 19.52 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0705S2

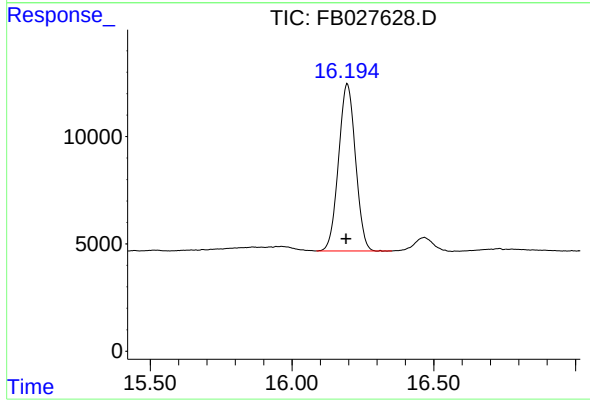

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.004 min
Response: 323080
Conc: 18.81 ng/ml