

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070523\
 Data File : FB030128.D
 Signal(s) : FID2B.CH
 Acq On : 5 Jul 2023 15:26
 Operator : YP/AJ
 Sample : 03509-19
 Misc : 2.80G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jul 06 02:41:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
 Quant Title :
 QLast Update : Mon Jun 26 14:31:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	248204	18.887 ng/ml
Target Compounds			
6) t Toluene	10.616	5673	0.239 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070523\
Data File : FB030128.D
Signal(s) : FID2B.CH
Acq On : 5 Jul 2023 15:26
Operator : YP/AJ
Sample : 03509-19
Misc : 2.80G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 06 02:41:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
Quant Title :
QLast Update : Mon Jun 26 14:31:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

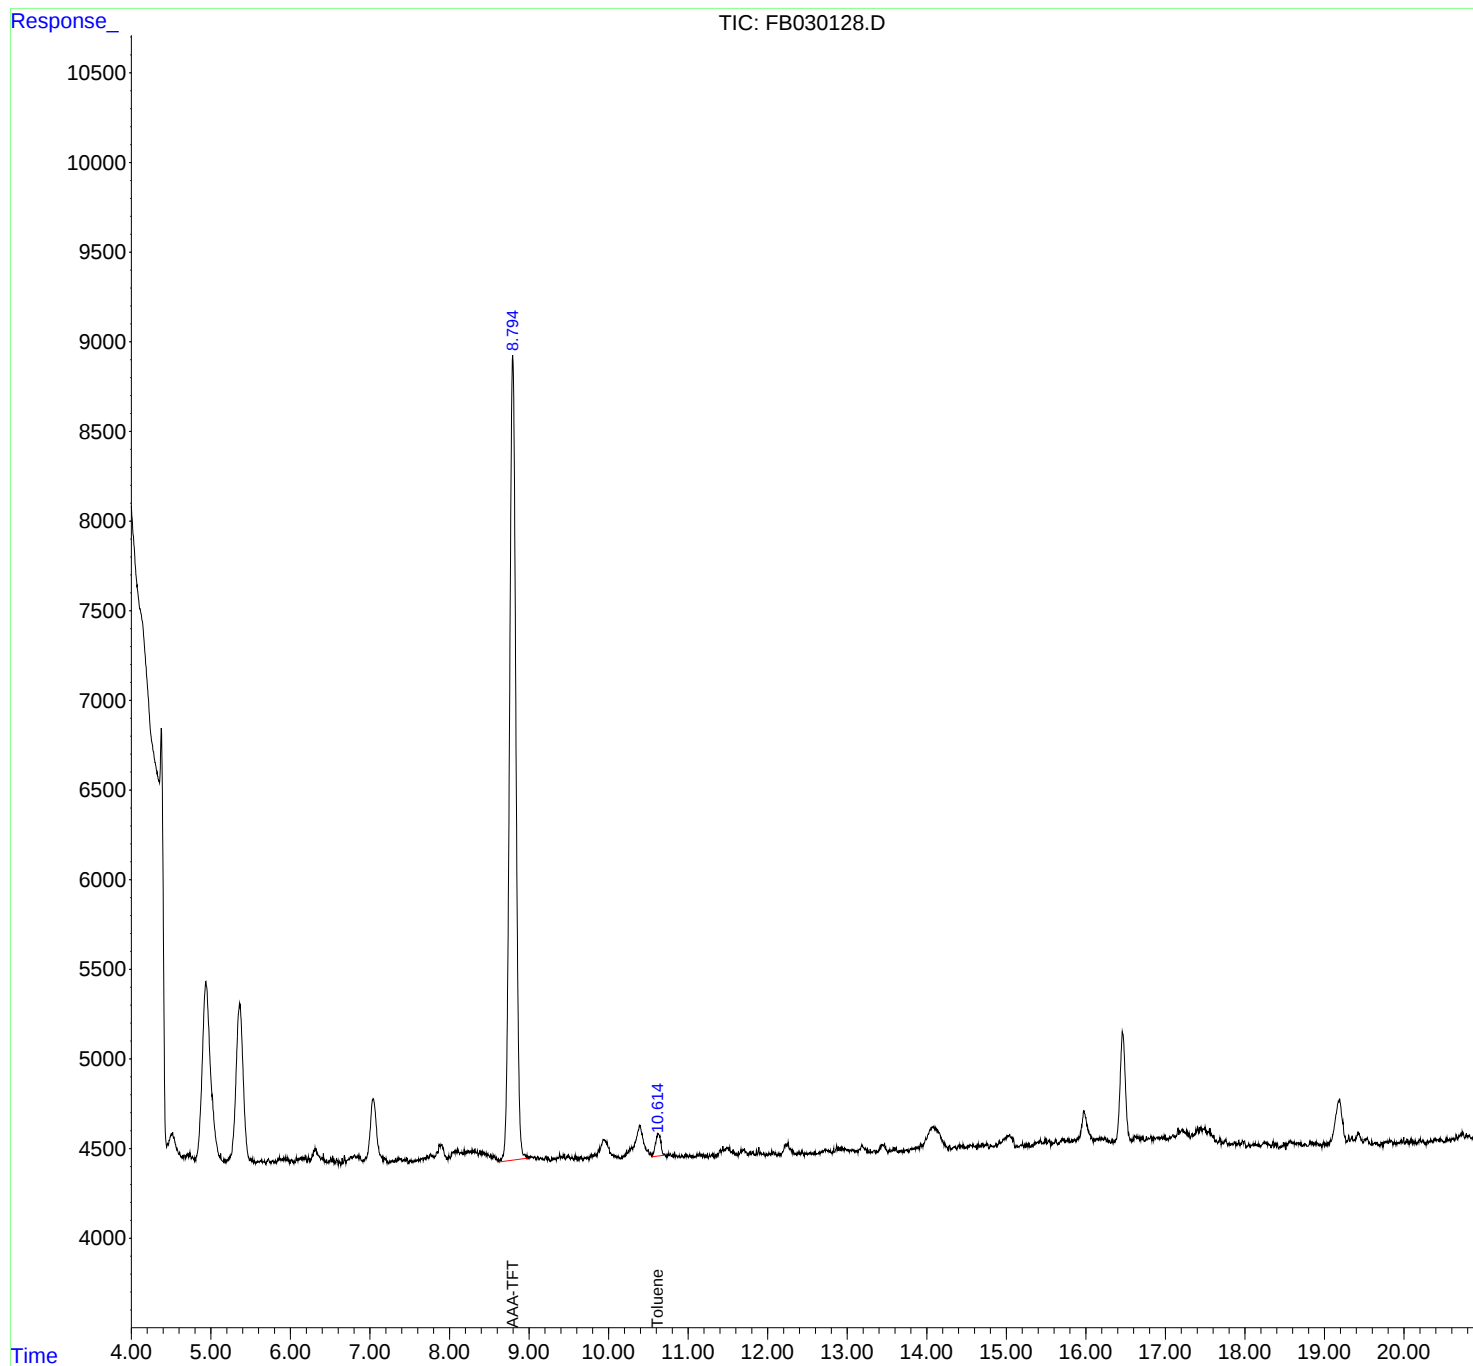


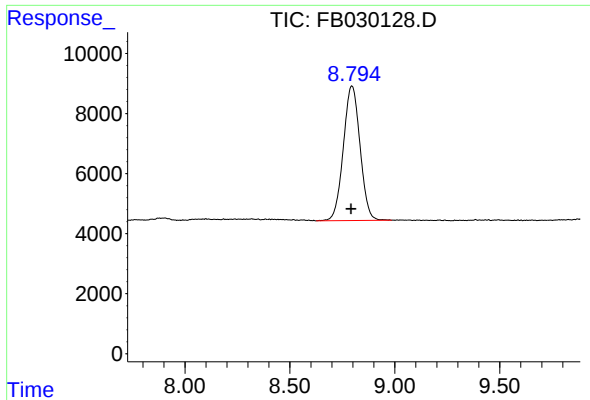

#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: 0.004 min
Response: 248204
Conc: 18.89 ng/ml

Instrument :
FID_B
ClientSampleId :

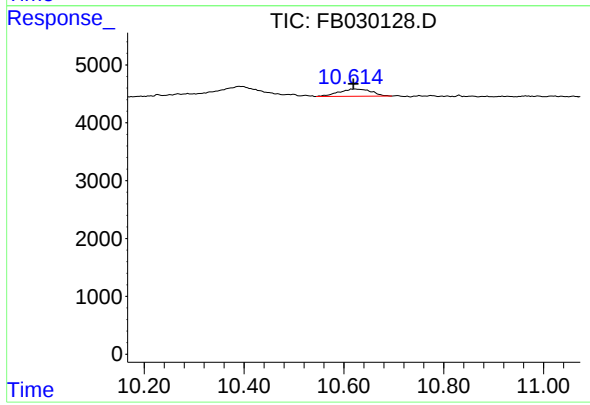

#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.003 min
Response: 5673
Conc: 0.24 ng/ml