

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070523\
Data File : FB030132.D
Signal(s) : FID2B.CH
Acq On : 5 Jul 2023 18:42
Operator : YP/AJ
Sample : 03510-04
Misc : 2.29G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 06 02:42:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
Quant Title :
QLast Update : Mon Jun 26 14:31:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	224086	17.052 ng/ml
Target Compounds			
8) t m-Xylene	13.194	2906	0.128 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070523\
Data File : FB030132.D
Signal(s) : FID2B.CH
Acq On : 5 Jul 2023 18:42
Operator : YP/AJ
Sample : 03510-04
Misc : 2.29G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 06 02:42:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
Quant Title :
QLast Update : Mon Jun 26 14:31:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

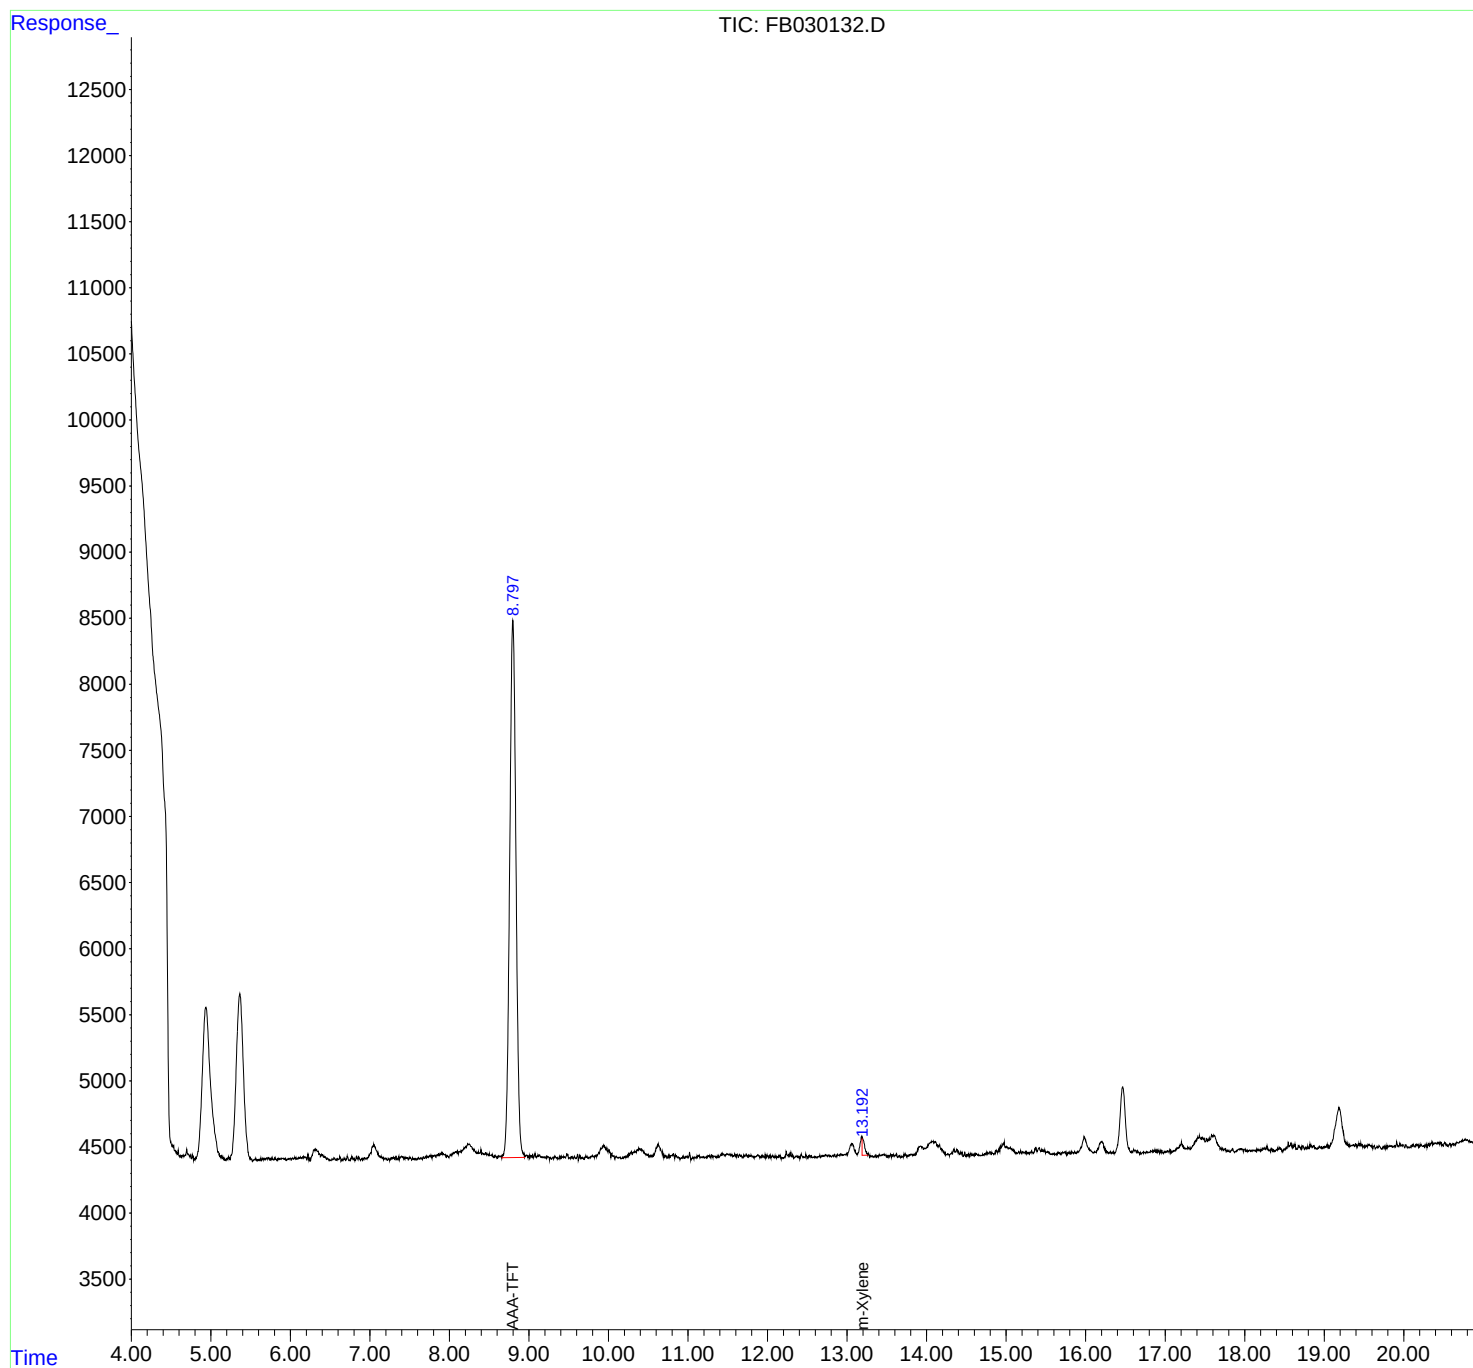


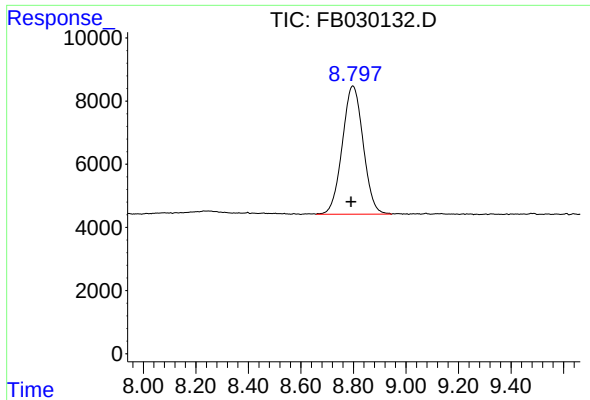

#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.007 min
Response: 224086
Conc: 17.05 ng/ml

Instrument :
FID_B
ClientSampleId :

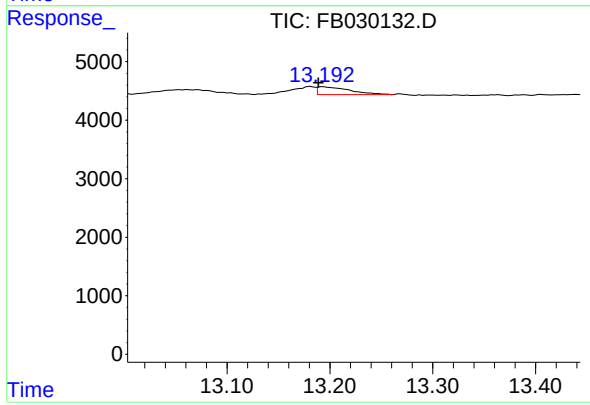

#8 m-Xylene

R.T.: 13.194 min
Delta R.T.: 0.005 min
Response: 2906
Conc: 0.13 ng/ml