

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB070523\  
 Data File : FB030124.D  
 Signal(s) : FID2B.CH  
 Acq On : 5 Jul 2023 12:46  
 Operator : YP/AJ  
 Sample : BSF0705S1  
 Misc : 5.00G/5.00 ML DI WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :  
 BSF0705S1

Integration File: Calibration.e  
 Quant Time: Jul 06 02:41:18 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB062623.M  
 Quant Title :  
 QLast Update : Mon Jun 26 14:31:24 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.793  | 229712   | 17.480 ng/ml |
| Target Compounds             |        |          |              |
| 1) t 2-Methylpentane         | 4.711  | 525358   | 27.946 ng/ml |
| 2) t 2,2,4-Trimethylpentane  | 7.420  | 590830   | 28.097 ng/ml |
| 3) t n-Heptane               | 7.750  | 202501   | 9.924 ng/ml  |
| 4) t Benzene                 | 7.887  | 235391   | 9.605 ng/ml  |
| 6) t Toluene                 | 10.621 | 685480   | 28.889 ng/ml |
| 7) t Ethylbenzene            | 13.057 | 215305   | 9.567 ng/ml  |
| 8) t m-Xylene                | 13.189 | 422245   | 18.567 ng/ml |
| 9) t O-Xylene                | 13.916 | 412224   | 18.182 ng/ml |
| 10) t 1,2,4-Trimethylbenzene | 16.191 | 397047   | 17.361 ng/ml |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB070523\  
Data File : FB030124.D  
Signal(s) : FID2B.CH  
Acq On : 5 Jul 2023 12:46  
Operator : YP/AJ  
Sample : BSF0705S1  
Misc : 5.00G/5.00 ML DI WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
BSF0705S1

Integration File: Calibration.e  
Quant Time: Jul 06 02:41:18 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB062623.M  
Quant Title :  
QLast Update : Mon Jun 26 14:31:24 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

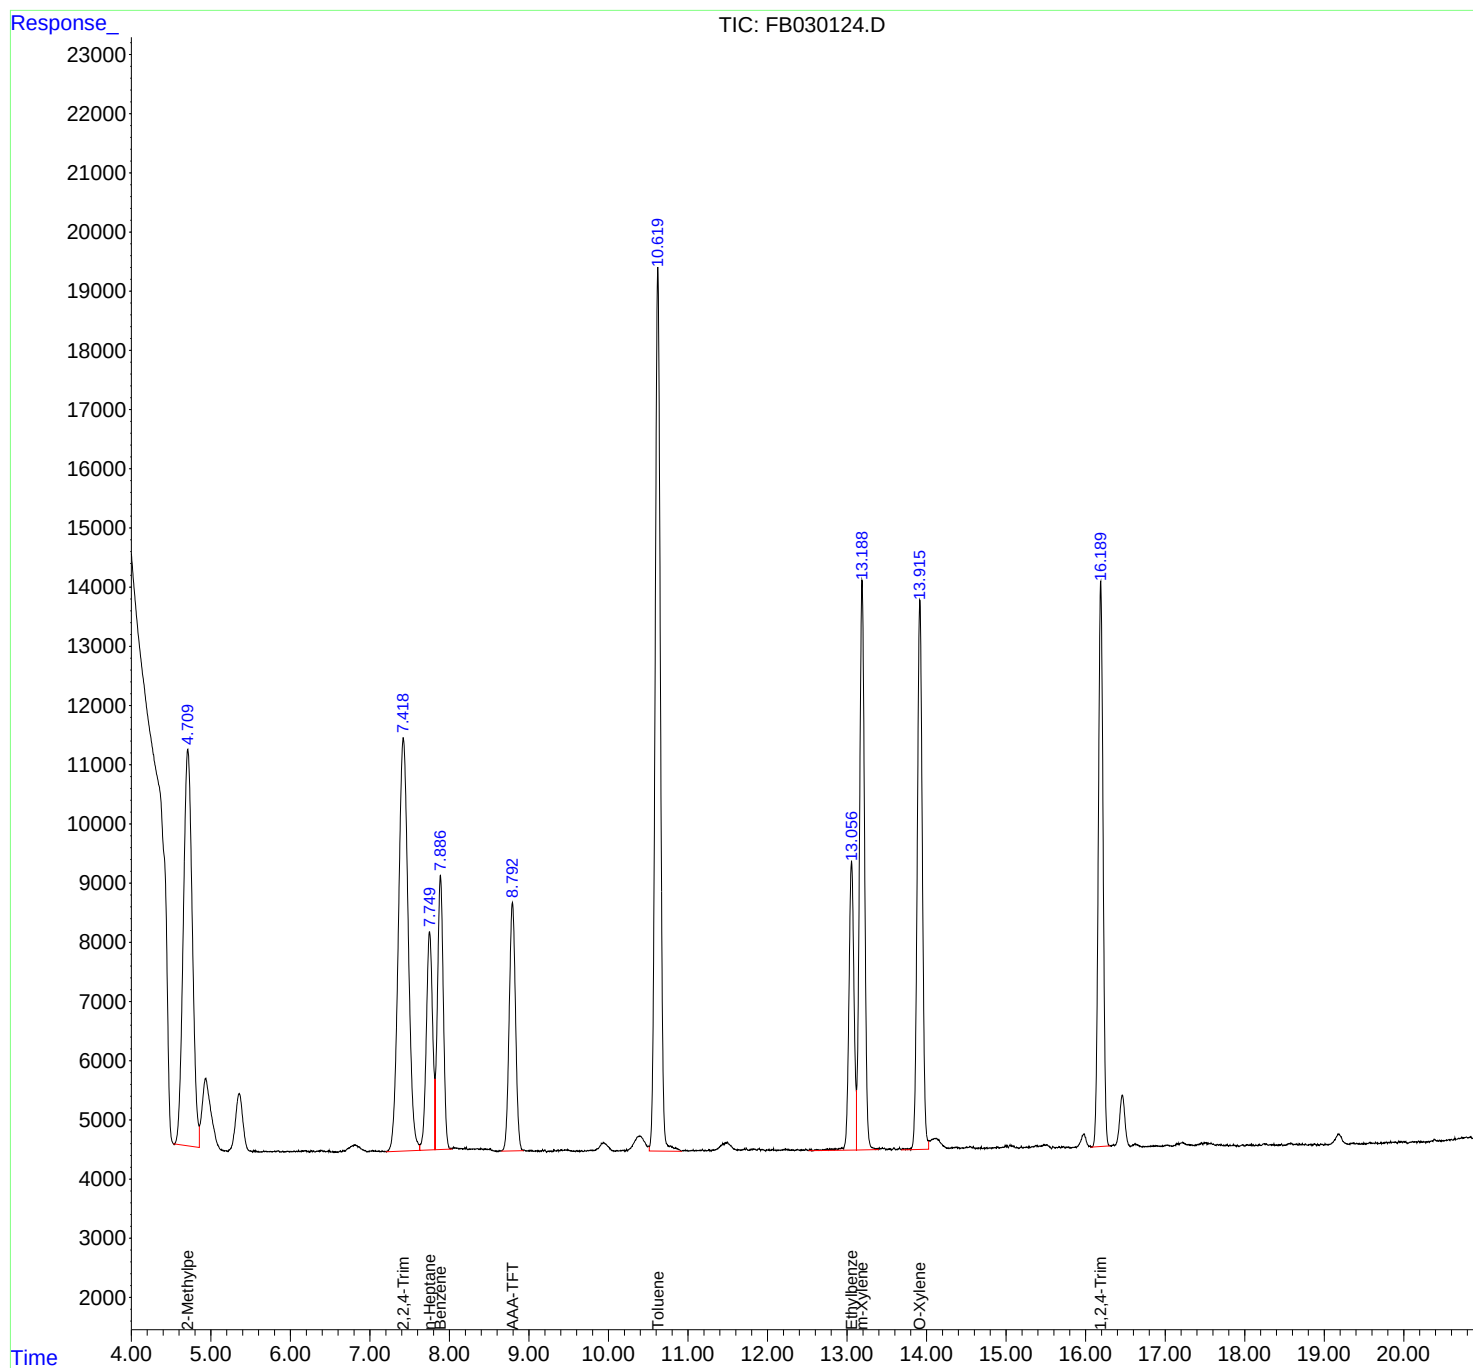


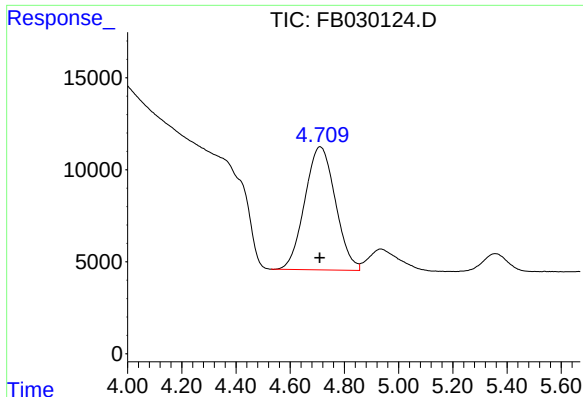

#1 2-Methylpentane


R.T.: 4.711 min  
Delta R.T.: 0.002 min  
Response: 525358  
Conc: 27.95 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF0705S1

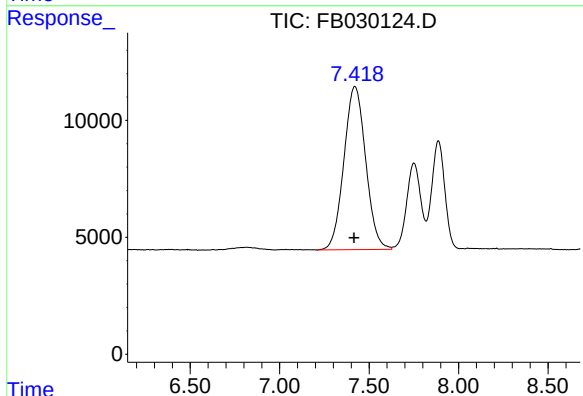


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min  
Delta R.T.: 0.004 min  
Response: 590830  
Conc: 28.10 ng/ml

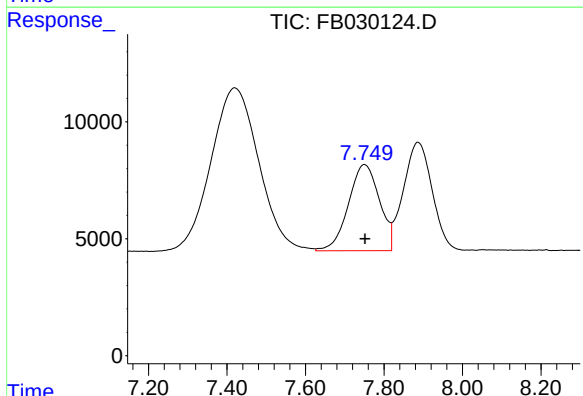


#3 n-Heptane

R.T.: 7.750 min  
Delta R.T.: 0.000 min  
Response: 202501  
Conc: 9.92 ng/ml

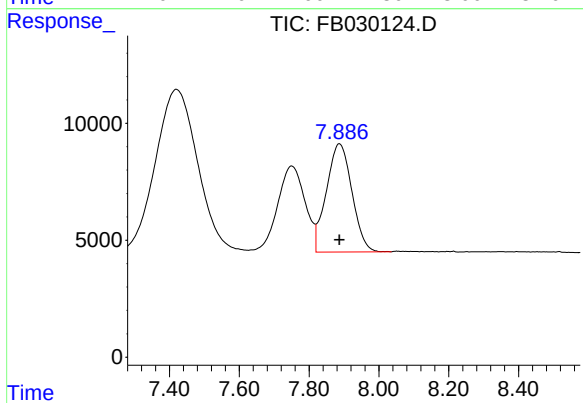

#4 Benzene


R.T.: 7.887 min  
Delta R.T.: 0.000 min  
Response: 235391  
Conc: 9.61 ng/ml

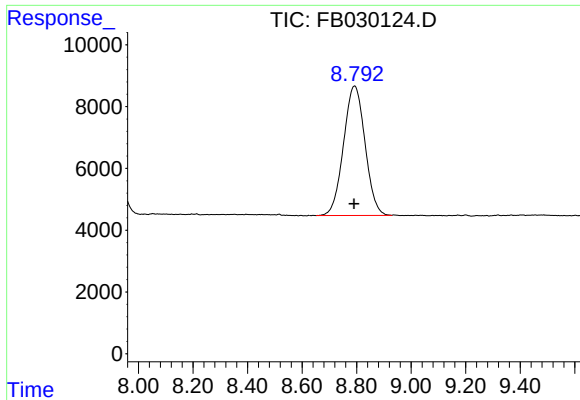

#5 AAA-TFT


R.T.: 8.793 min  
Delta R.T.: 0.002 min  
Response: 229712  
Conc: 17.48 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF0705S1

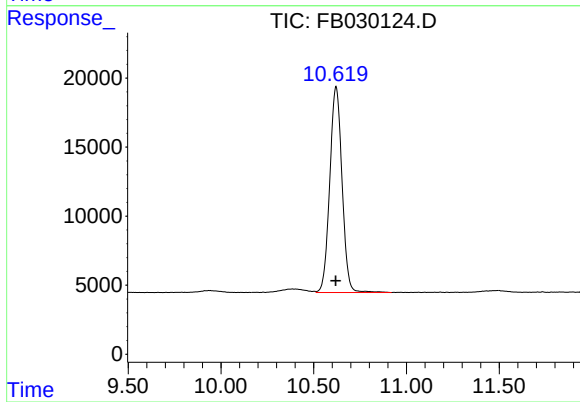


#6 Toluene

R.T.: 10.621 min  
Delta R.T.: 0.001 min  
Response: 685480  
Conc: 28.89 ng/ml

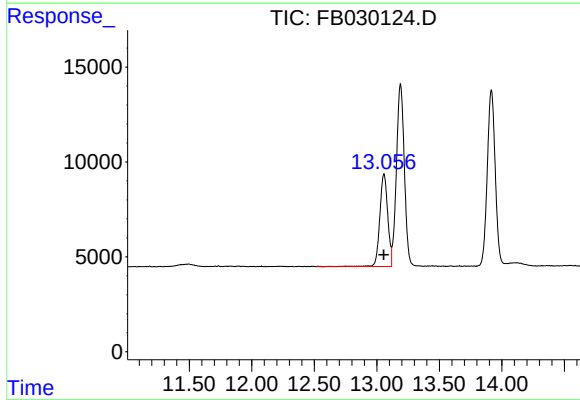


#7 Ethylbenzene

R.T.: 13.057 min  
Delta R.T.: 0.000 min  
Response: 215305  
Conc: 9.57 ng/ml

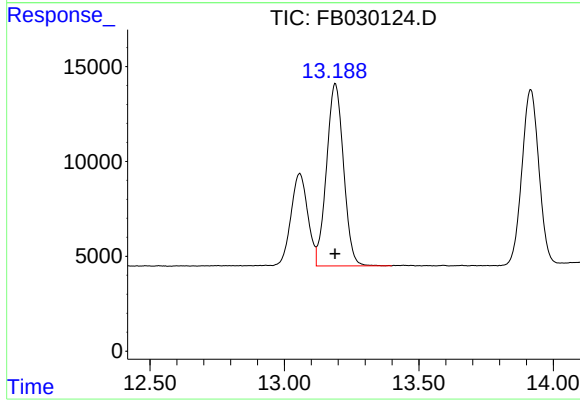

#8 m-Xylene


R.T.: 13.189 min  
Delta R.T.: 0.000 min  
Response: 422245  
Conc: 18.57 ng/ml

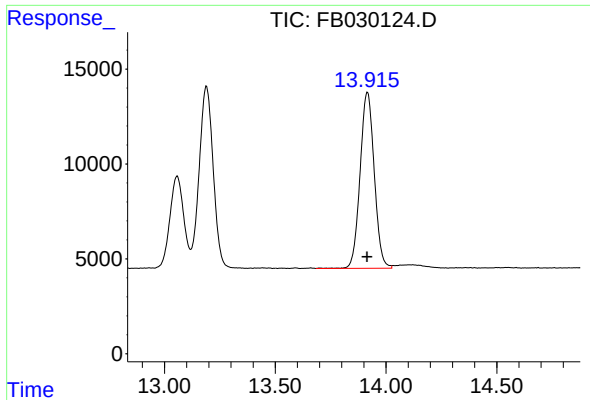

#9 O-Xylene

R.T.: 13.916 min  
Delta R.T.: 0.001 min  
Response: 412224  
Conc: 18.18 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
BSF0705S1

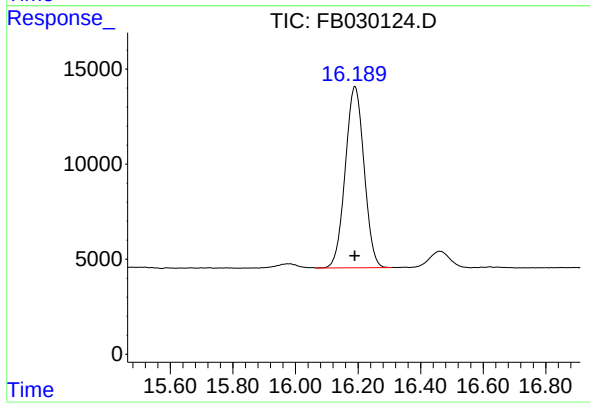

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min  
Delta R.T.: 0.000 min  
Response: 397047  
Conc: 17.36 ng/ml