

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070623\
 Data File : FB030141.D
 Signal(s) : FID2B.CH
 Acq On : 6 Jul 2023 10:15
 Operator : YP/AJ
 Sample : BSF0706S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0706S1

Integration File: Calibration.e
 Quant Time: Jul 07 02:52:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
 Quant Title :
 QLast Update : Mon Jun 26 14:31:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	329272	25.056 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	556522	29.604 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	619274	29.450 ng/ml
3) t n-Heptane	7.752	218143	10.691 ng/ml
4) t Benzene	7.888	247469	10.098 ng/ml
6) t Toluene	10.621	710505	29.943 ng/ml
7) t Ethylbenzene	13.057	221207	9.829 ng/ml
8) t m-Xylene	13.189	442156	19.443 ng/ml
9) t O-Xylene	13.916	427434	18.853 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	406079	17.756 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070623\
Data File : FB030141.D
Signal(s) : FID2B.CH
Acq On : 6 Jul 2023 10:15
Operator : YP/AJ
Sample : BSF0706S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0706S1

Integration File: Calibration.e
Quant Time: Jul 07 02:52:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
Quant Title :
QLast Update : Mon Jun 26 14:31:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

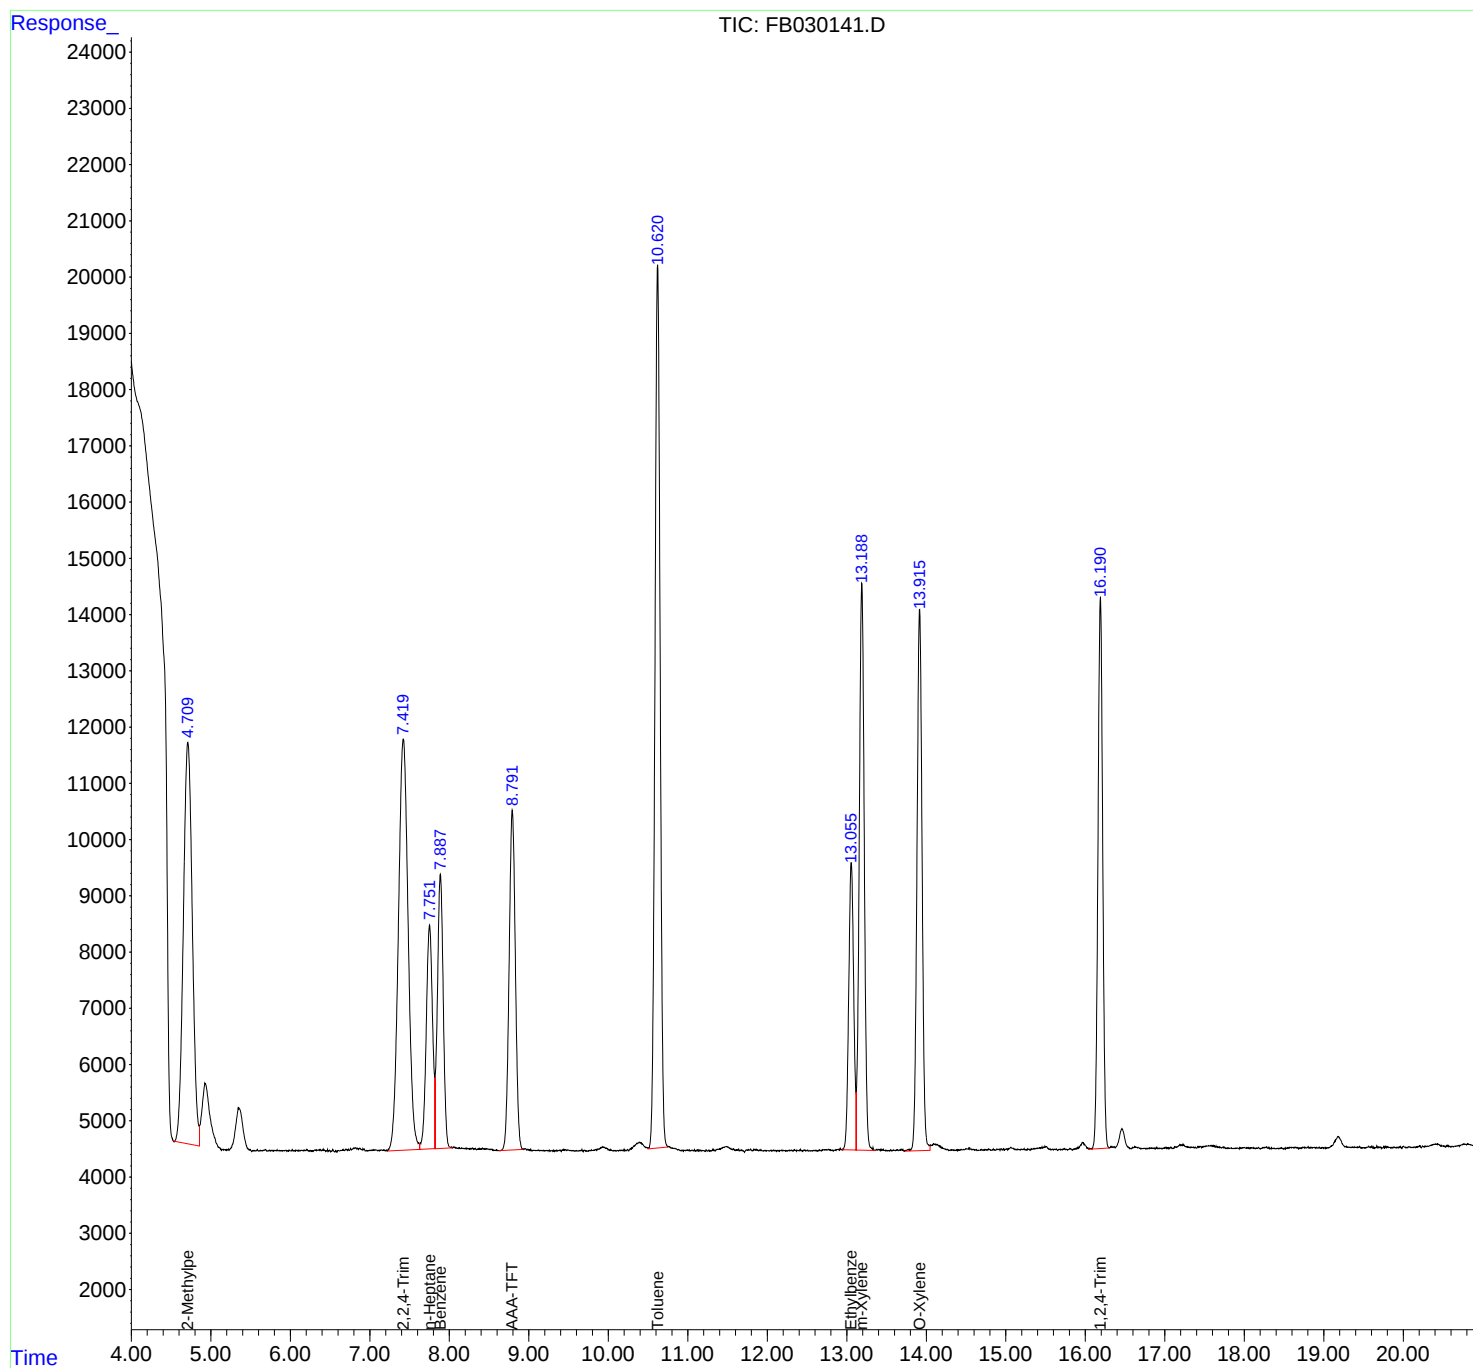


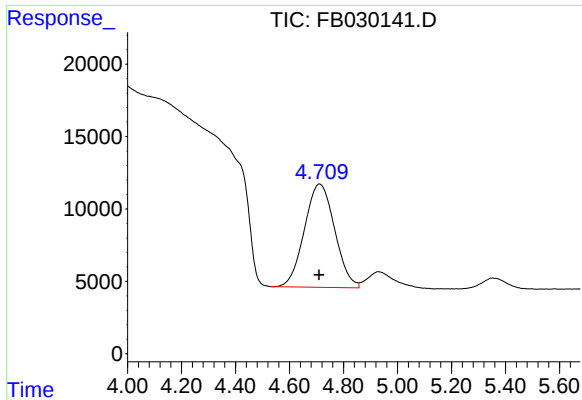

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.002 min
Response: 556522
Conc: 29.60 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0706S1

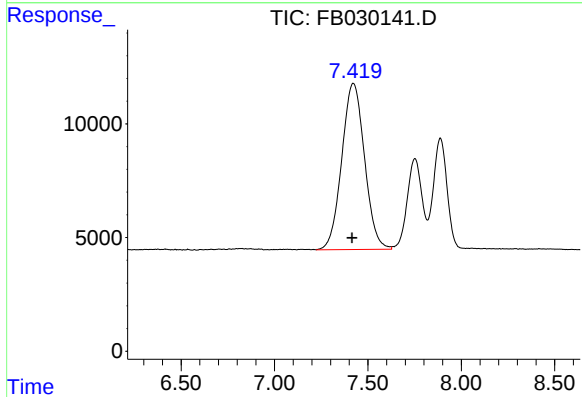


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: 0.006 min
Response: 619274
Conc: 29.45 ng/ml

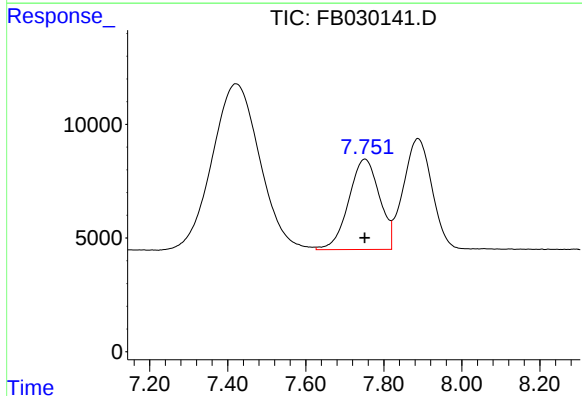


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 218143
Conc: 10.69 ng/ml

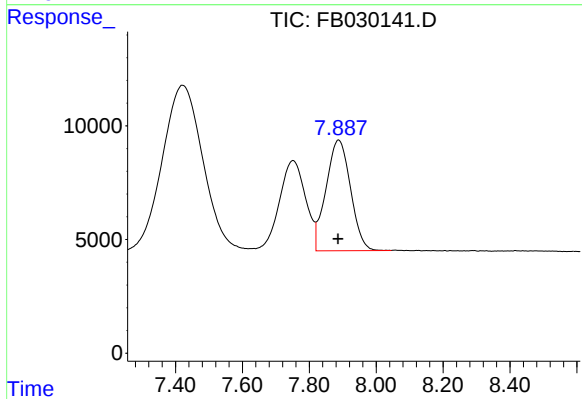

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.002 min
Response: 247469
Conc: 10.10 ng/ml

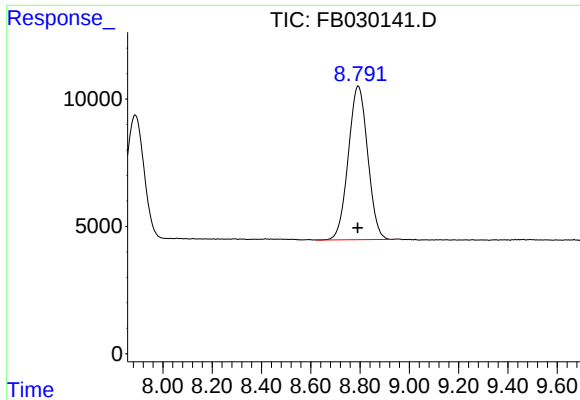

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 329272
Conc: 25.06 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0706S1

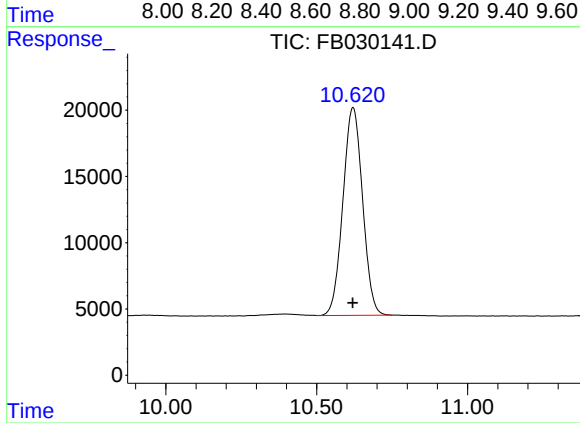


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.002 min
Response: 710505
Conc: 29.94 ng/ml

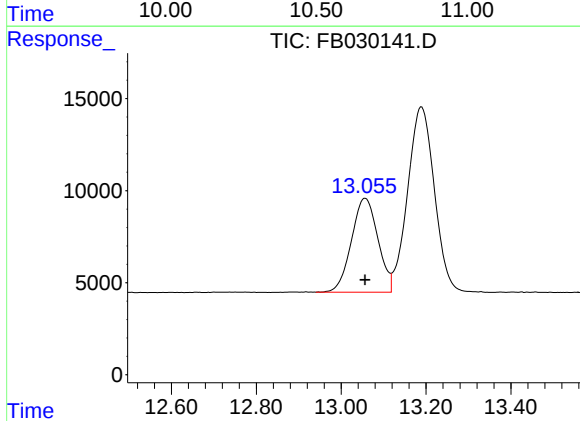


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.000 min
Response: 221207
Conc: 9.83 ng/ml

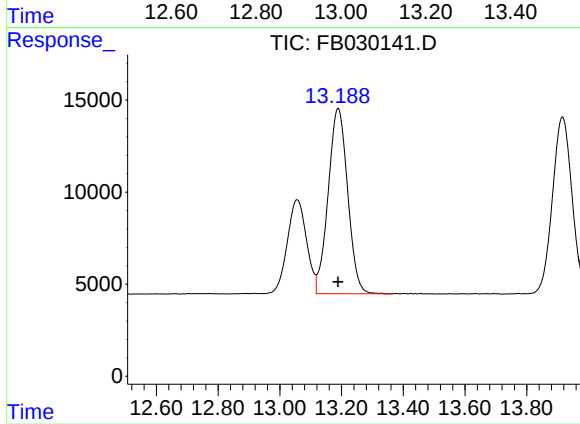

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 442156
Conc: 19.44 ng/ml

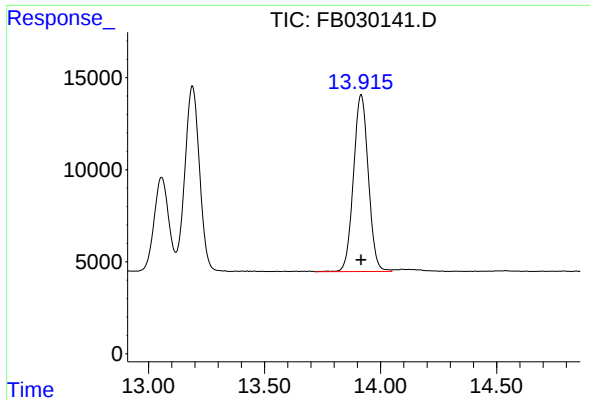

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.001 min
Response: 427434
Conc: 18.85 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0706S1

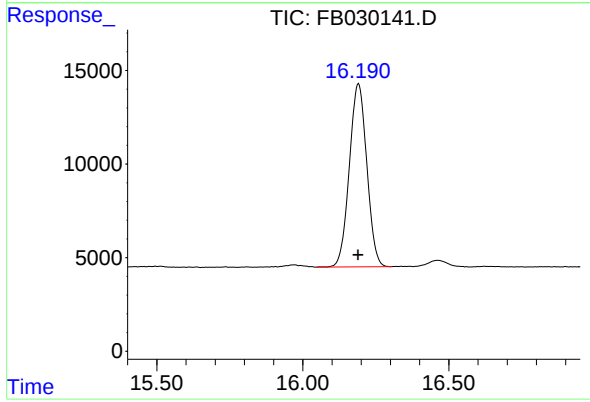

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 406079
Conc: 17.76 ng/ml