

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070623\
 Data File : FB030143.D
 Signal(s) : FID2B.CH
 Acq On : 6 Jul 2023 11:33
 Operator : YP/AJ
 Sample : BSF0706S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0706S2

Integration File: Calibration.e
 Quant Time: Jul 07 02:52:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
 Quant Title :
 QLast Update : Mon Jun 26 14:31:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	231085	17.585 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.714	567206	30.172 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	638681	30.373 ng/ml
3) t n-Heptane	7.752	220709	10.817 ng/ml
4) t Benzene	7.890	261814	10.684 ng/ml
6) t Toluene	10.622	773439	32.596 ng/ml
7) t Ethylbenzene	13.058	236525	10.510 ng/ml
8) t m-Xylene	13.190	471174	20.719 ng/ml
9) t O-Xylene	13.917	456405	20.131 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	432741	18.922 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070623\
Data File : FB030143.D
Signal(s) : FID2B.CH
Acq On : 6 Jul 2023 11:33
Operator : YP/AJ
Sample : BSF0706S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0706S2

Integration File: Calibration.e
Quant Time: Jul 07 02:52:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
Quant Title :
QLast Update : Mon Jun 26 14:31:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

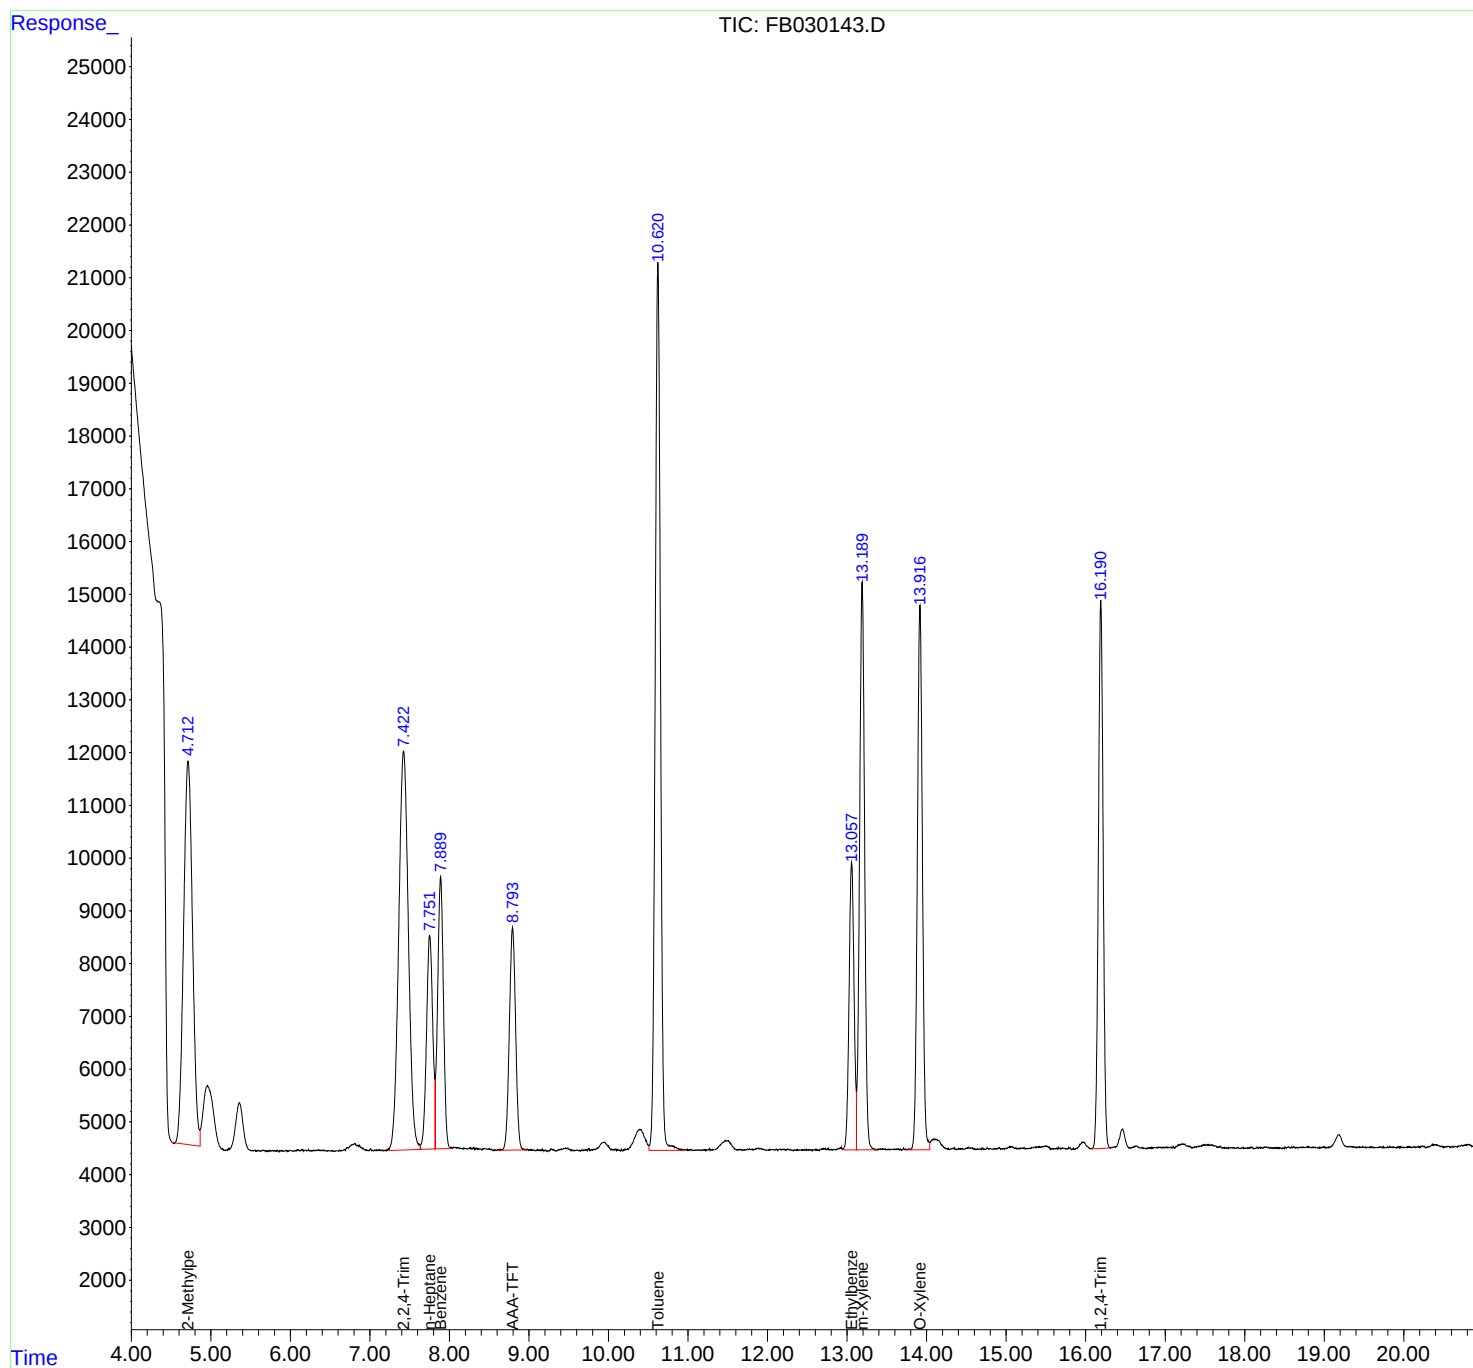


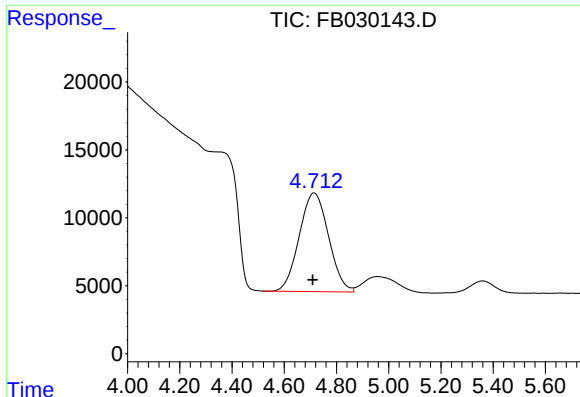

#1 2-Methylpentane


R.T.: 4.714 min
Delta R.T.: 0.005 min
Response: 567206
Conc: 30.17 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0706S2

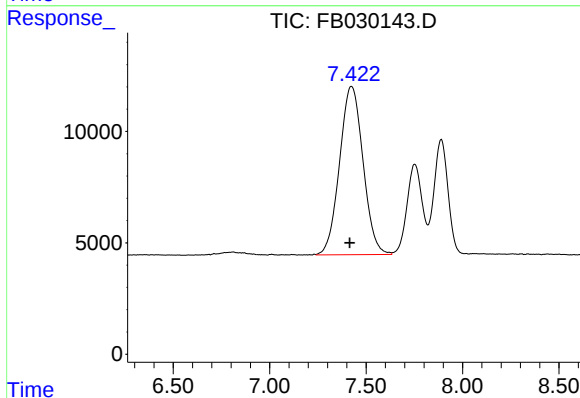


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: 0.008 min
Response: 638681
Conc: 30.37 ng/ml

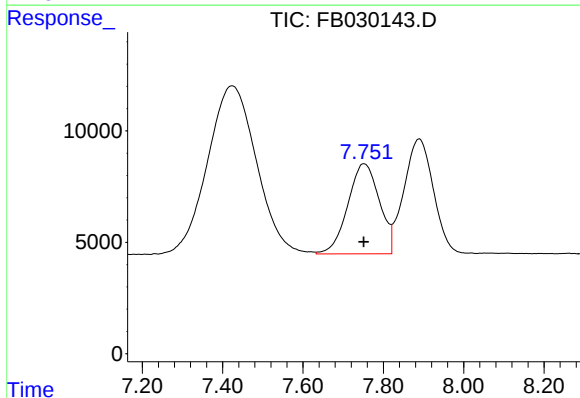


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 220709
Conc: 10.82 ng/ml

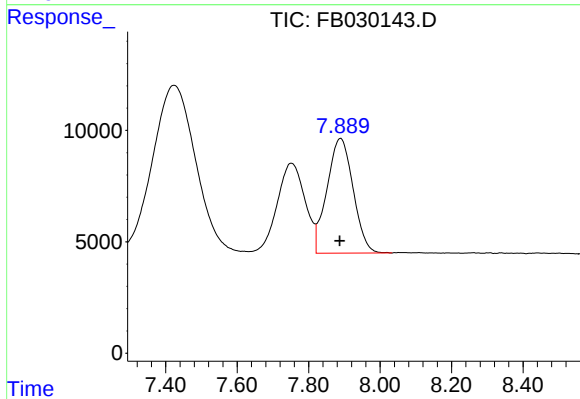

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.003 min
Response: 261814
Conc: 10.68 ng/ml

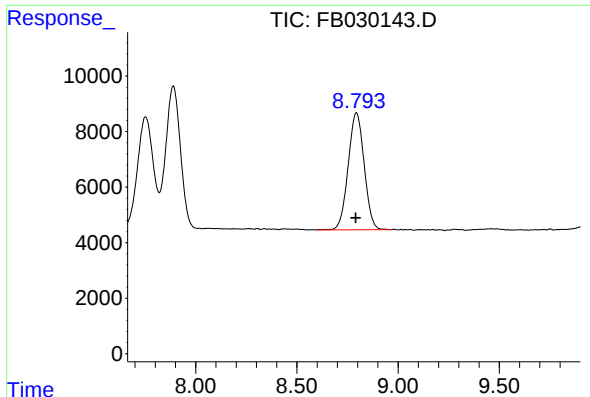

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.003 min
Response: 231085
Conc: 17.58 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0706S2

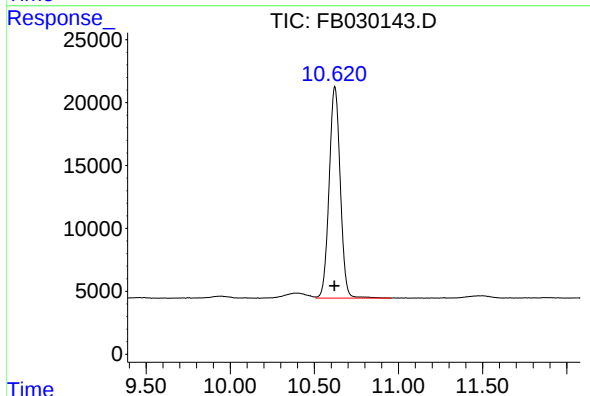


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.002 min
Response: 773439
Conc: 32.60 ng/ml

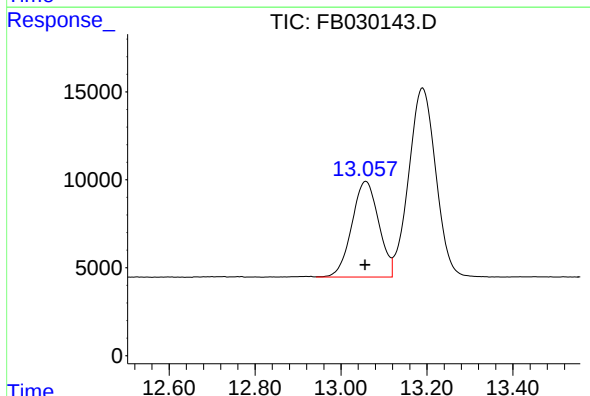


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.002 min
Response: 236525
Conc: 10.51 ng/ml

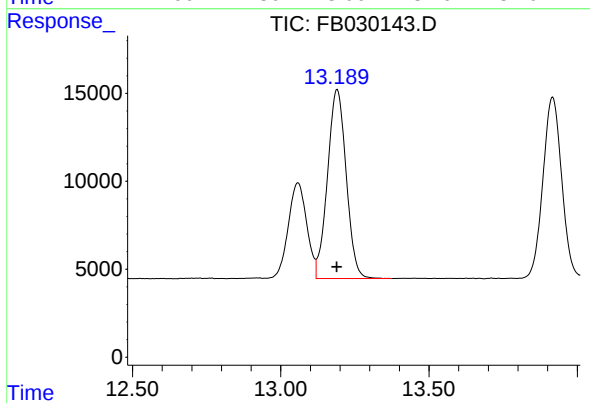

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.002 min
Response: 471174
Conc: 20.72 ng/ml

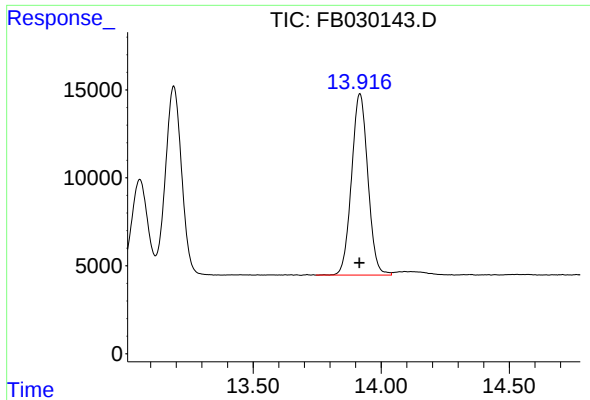

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.002 min
Response: 456405
Conc: 20.13 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0706S2

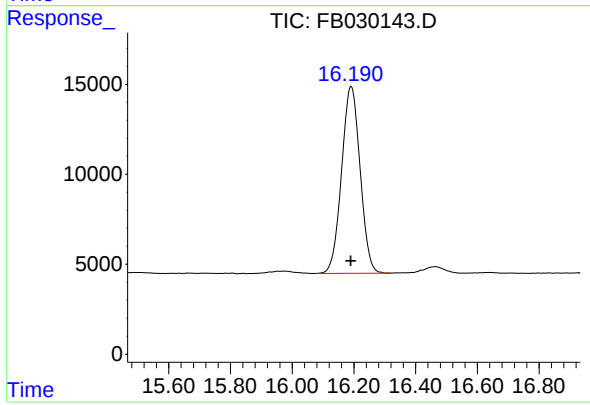

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.002 min
Response: 432741
Conc: 18.92 ng/ml