

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070720\
 Data File : FB024539.D
 Signal(s) : FID2B.CH
 Acq On : 7 Jul 2020 9:56
 Operator : DD/AJ
 Sample : BSF0707S1
 Misc : 5.00gm/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 08 00:58:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.796	499776	20.657 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.684	999495	31.270 ng/ml
2) t	2,2,4-Trimethylpentane	7.415	1097582	32.740 ng/ml
3) t	n-Heptane	7.755	359013	10.616 ng/ml
4) t	Benzene	7.889	424556	10.502 ng/ml
6) t	Toluene	10.628	1226661	31.214 ng/ml
7) t	Ethylbenzene	13.068	383769	10.936 ng/ml
8) t	m-Xylene	13.201	750318	21.910 ng/ml
9) t	O-Xylene	13.928	732817	21.858 ng/ml
10) t	1,2,4-Trimethylbenzene	16.206	621586	22.387 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070720\
Data File : FB024539.D
Signal(s) : FID2B.CH
Acq On : 7 Jul 2020 9:56
Operator : DD/AJ
Sample : BSF0707S1
Misc : 5.00gm/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 08 00:58:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

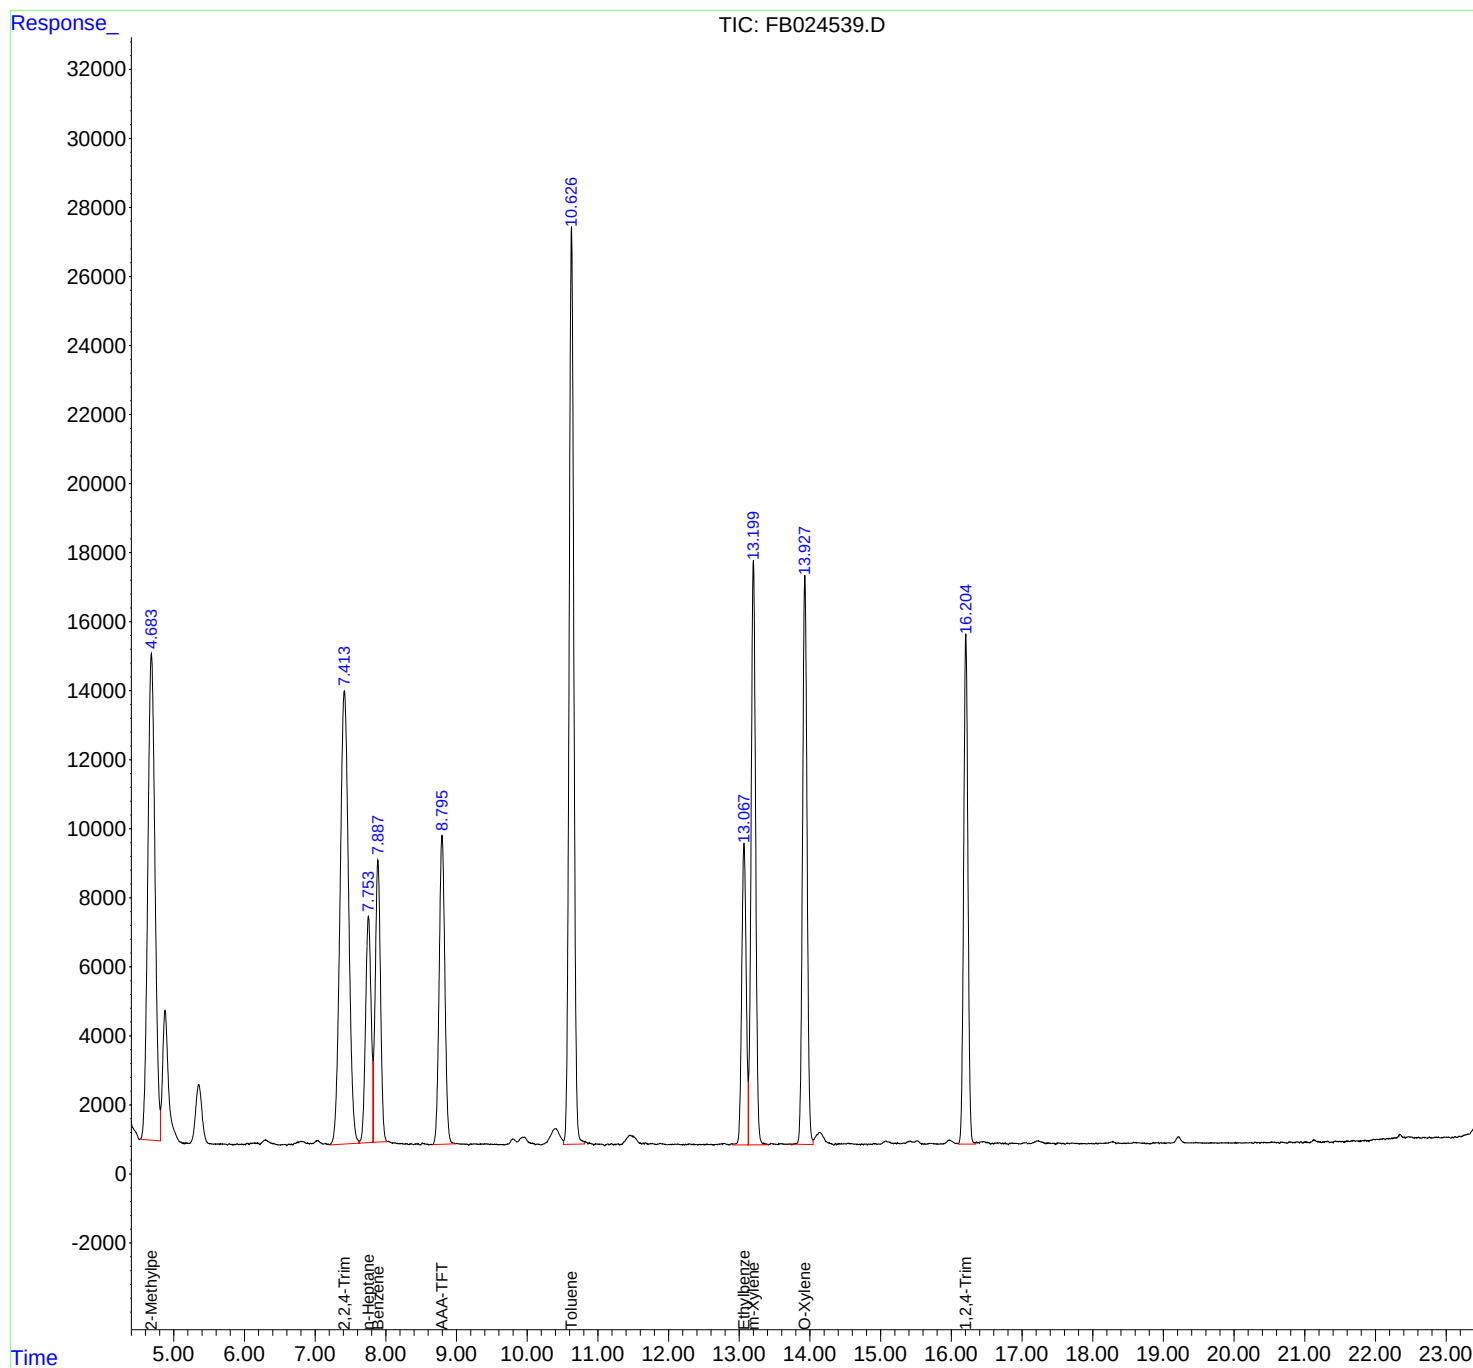

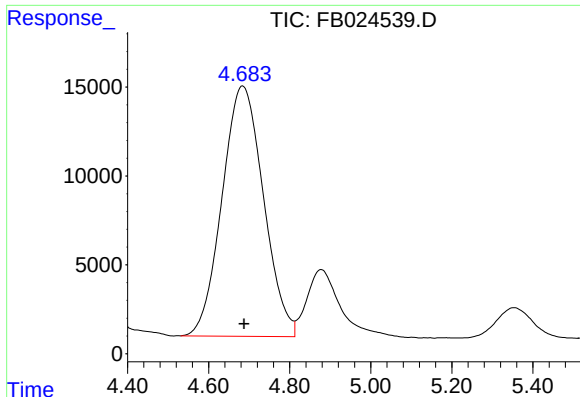


#1 2-Methylpentane

R.T.: 4.684 min
Delta R.T.: -0.003 min
Response: 999495
Conc: 31.27 ng/ml

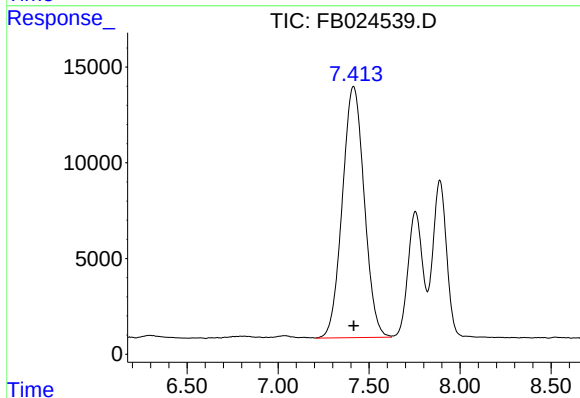


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.001 min
Response: 1097582
Conc: 32.74 ng/ml

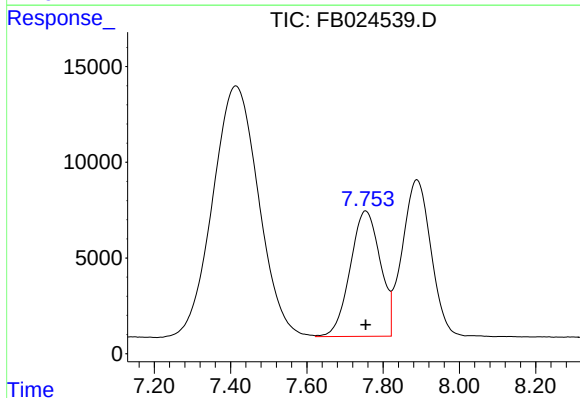


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 359013
Conc: 10.62 ng/ml

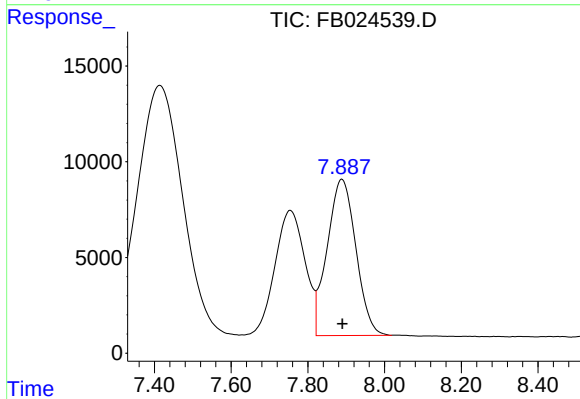


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.001 min
Response: 424556
Conc: 10.50 ng/ml

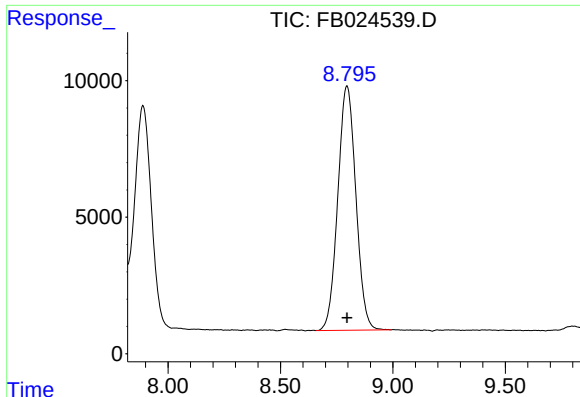


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: 0.000 min
Response: 499776
Conc: 20.66 ng/ml

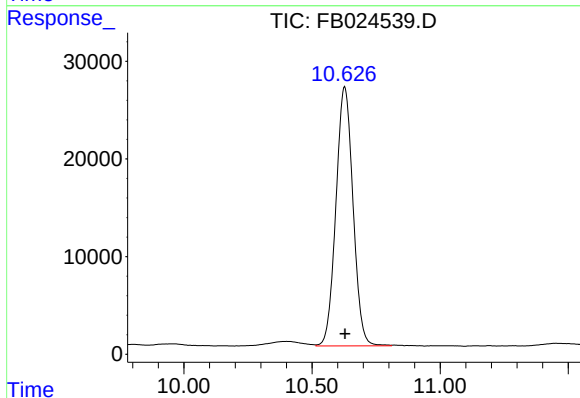


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.000 min
Response: 1226661
Conc: 31.21 ng/ml

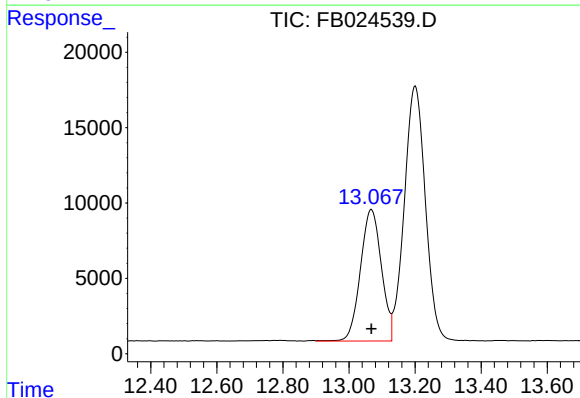


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: 0.000 min
Response: 383769
Conc: 10.94 ng/ml

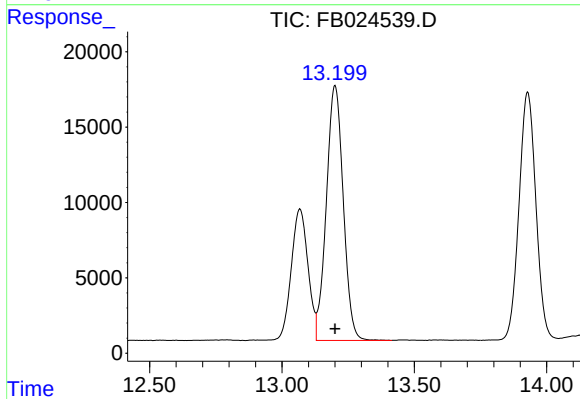


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: 0.000 min
Response: 750318
Conc: 21.91 ng/ml

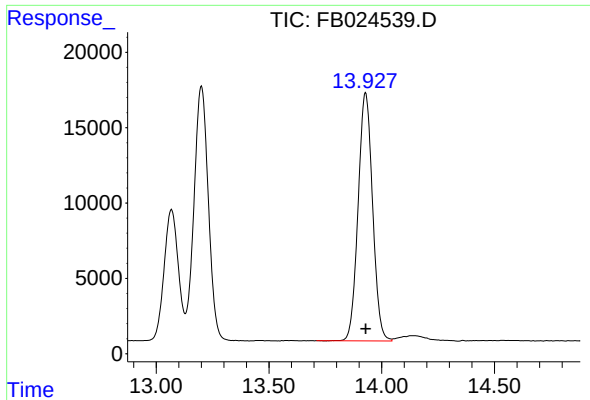

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: 0.000 min
Response: 732817
Conc: 21.86 ng/ml

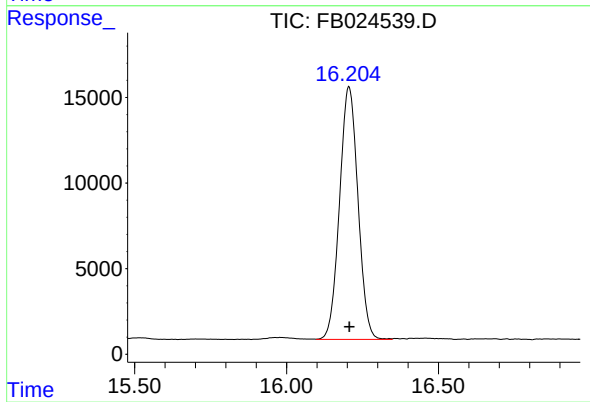

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.000 min
Response: 621586
Conc: 22.39 ng/ml