

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070722\
 Data File : FB027633.D
 Signal(s) : FID2B.CH
 Acq On : 7 Jul 2022 10:29
 Operator : AJ/MA
 Sample : BSF0707S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 08 03:30:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	248675	22.170 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	470473	27.926 ng/ml
2) t 2,2,4-Trimethylpentane	7.429	511414	29.127 ng/ml
3) t n-Heptane	7.753	163141	9.312 ng/ml
4) t Benzene	7.889	196315	9.627 ng/ml
6) t Toluene	10.622	565909	29.228 ng/ml
7) t Ethylbenzene	13.058	175428	9.687 ng/ml
8) t m-Xylene	13.191	351079	19.695 ng/ml
9) t O-Xylene	13.918	340990	19.624 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	341119	19.858 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070722\
Data File : FB027633.D
Signal(s) : FID2B.CH
Acq On : 7 Jul 2022 10:29
Operator : AJ/MA
Sample : BSF0707S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 08 03:30:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

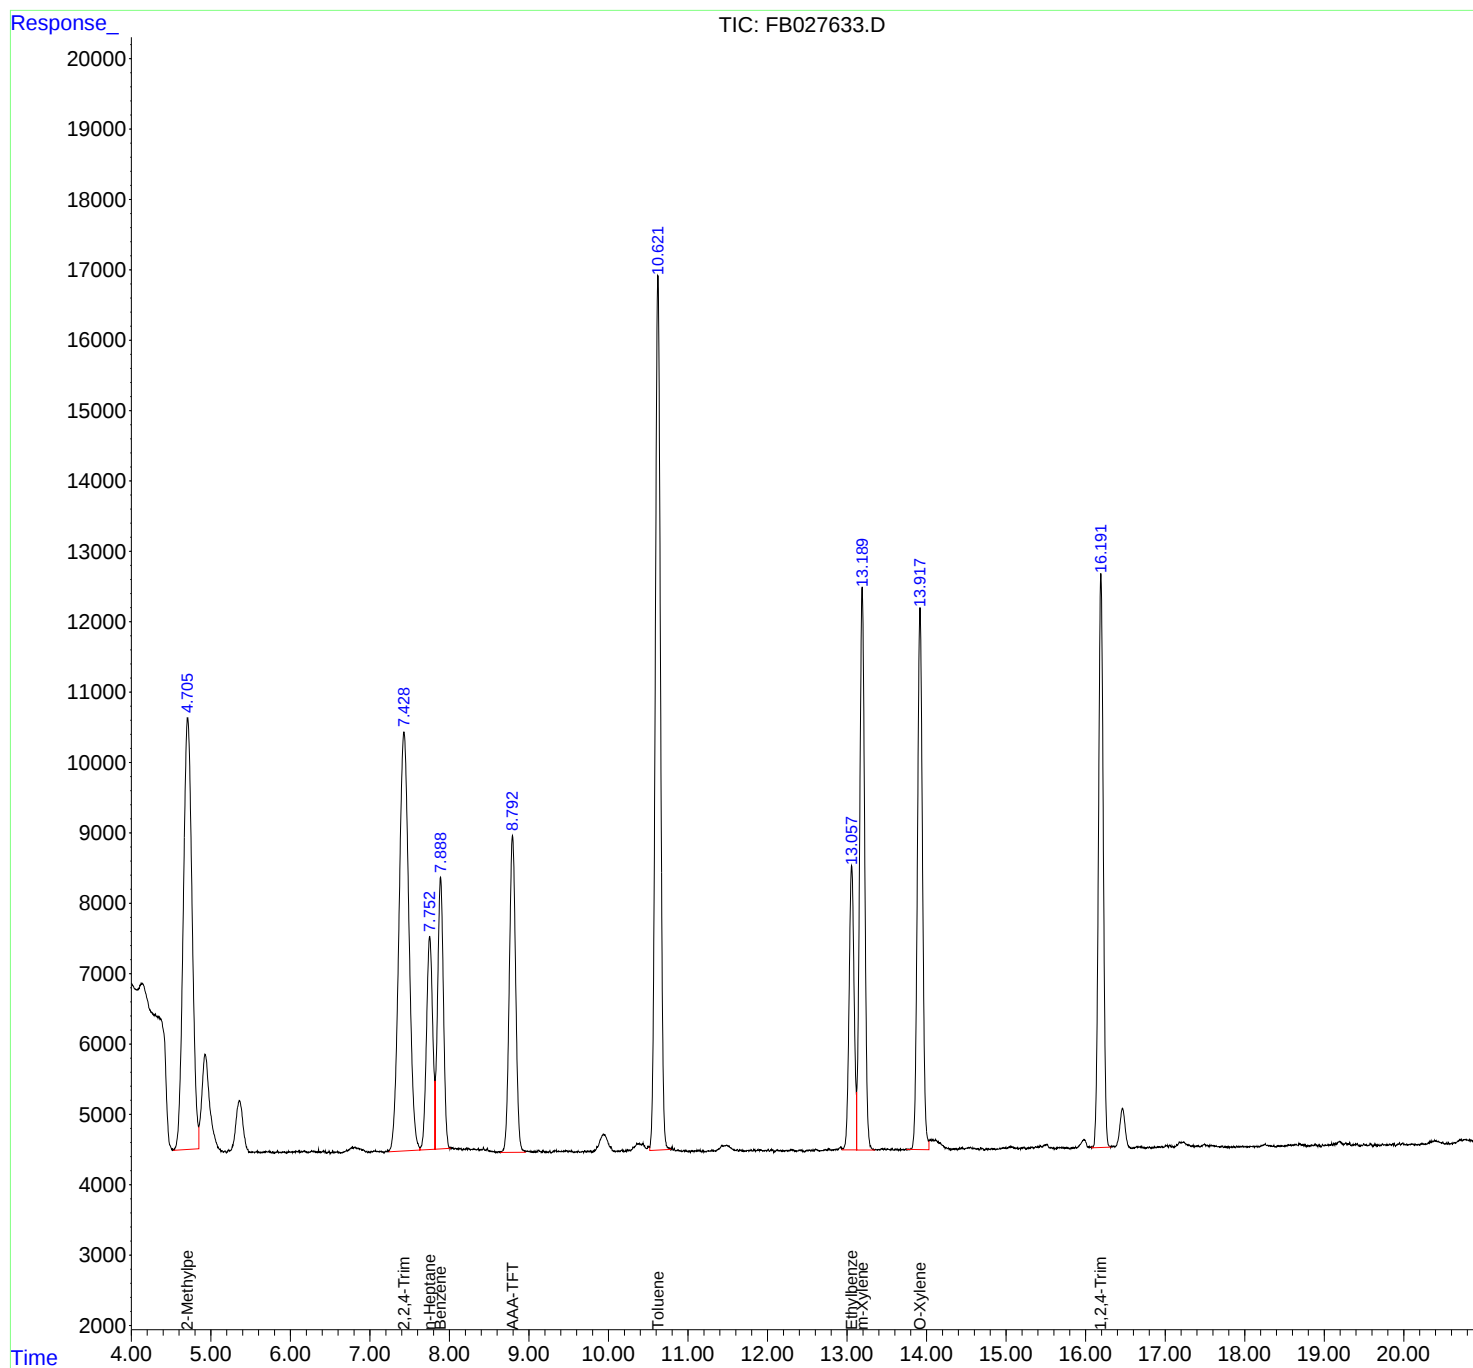

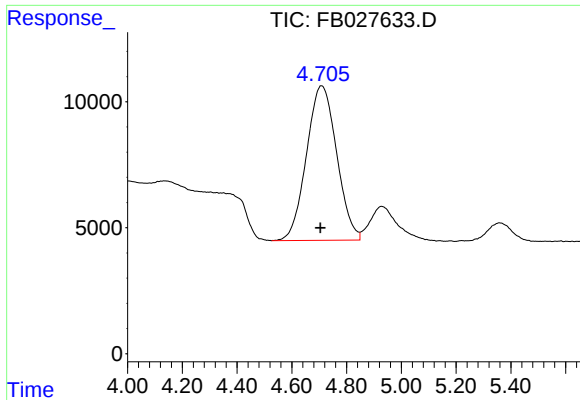


#1 2-Methylpentane

R.T.: 4.708 min
Delta R.T.: 0.004 min
Response: 470473
Conc: 27.93 ng/ml

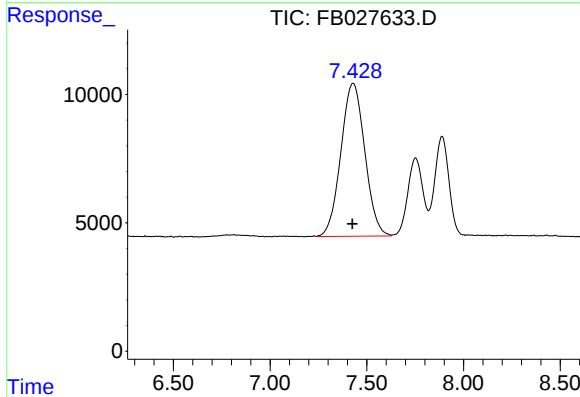


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min
Delta R.T.: 0.003 min
Response: 511414
Conc: 29.13 ng/ml

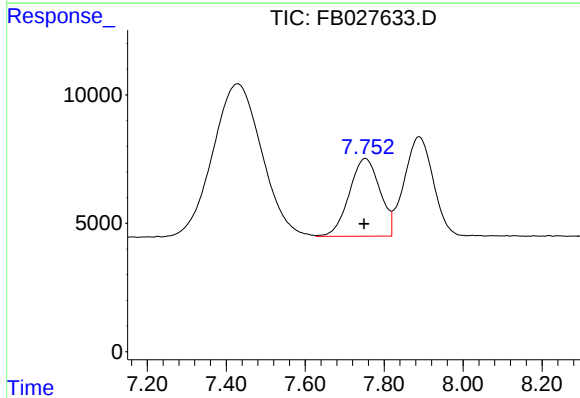


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.003 min
Response: 163141
Conc: 9.31 ng/ml

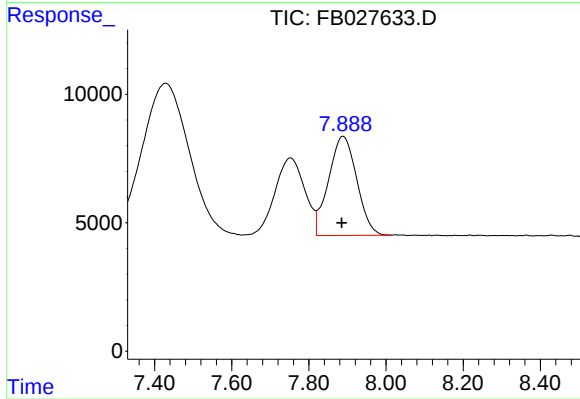


#4 Benzene

R.T.: 7.889 min
Delta R.T.: 0.003 min
Response: 196315
Conc: 9.63 ng/ml

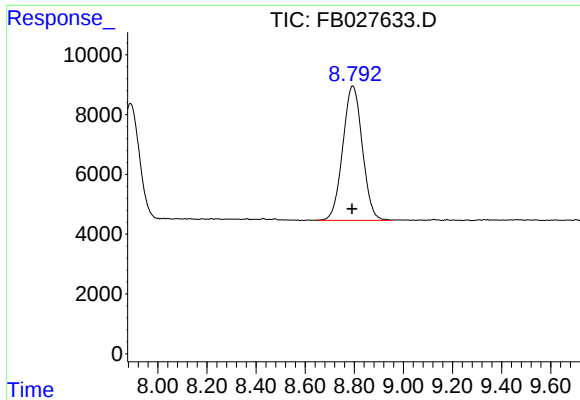


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: 0.003 min
Response: 248675
Conc: 22.17 ng/ml

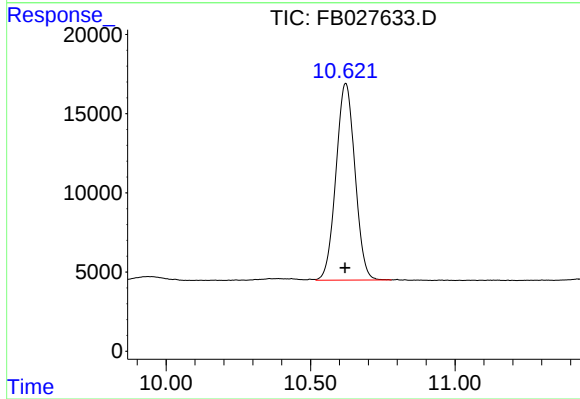


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.003 min
Response: 565909
Conc: 29.23 ng/ml

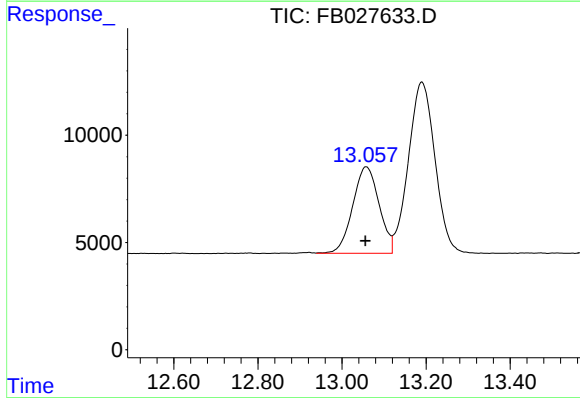


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.002 min
Response: 175428
Conc: 9.69 ng/ml

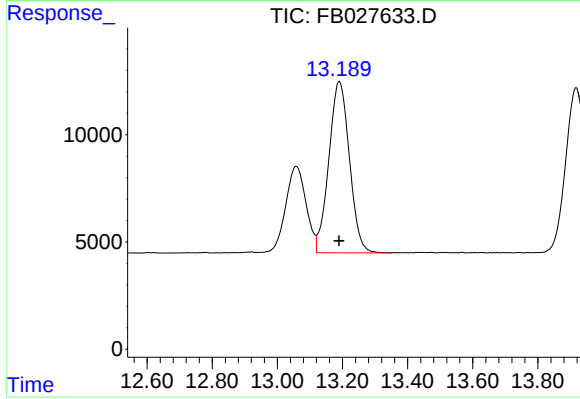

#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.001 min
Response: 351079
Conc: 19.69 ng/ml

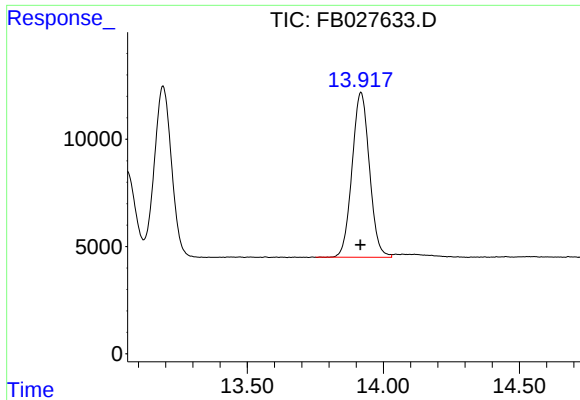


#9 O-Xylene

R.T.: 13.918 min

Delta R.T.: 0.002 min

Response: 340990

Conc: 19.62 ng/ml

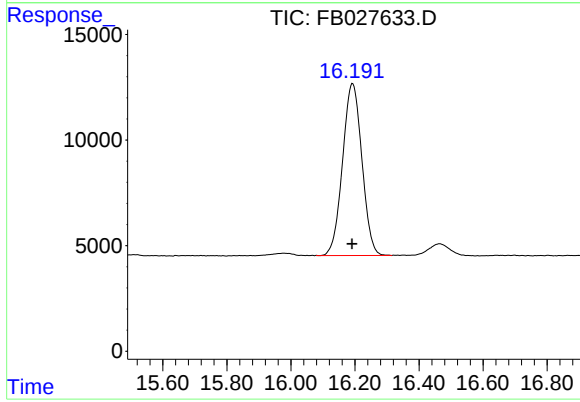

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min

Delta R.T.: 0.001 min

Response: 341119

Conc: 19.86 ng/ml