

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070722\
 Data File : FB027635.D
 Signal(s) : FID2B.CH
 Acq On : 7 Jul 2022 13:09
 Operator : AJ/MA
 Sample : N3581-01MS
 Misc : 4.87G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 08 03:30:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	218831	19.509 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	481712	28.593 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	494362	28.155 ng/ml
3) t n-Heptane	7.755	165987	9.475 ng/ml
4) t Benzene	7.892	192407	9.435 ng/ml
6) t Toluene	10.624	562806	29.067 ng/ml
7) t Ethylbenzene	13.060	175793	9.707 ng/ml
8) t m-Xylene	13.193	349601	19.612 ng/ml
9) t O-Xylene	13.920	336489	19.365 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	334958	19.499 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070722\
Data File : FB027635.D
Signal(s) : FID2B.CH
Acq On : 7 Jul 2022 13:09
Operator : AJ/MA
Sample : N3581-01MS
Misc : 4.87G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 08 03:30:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

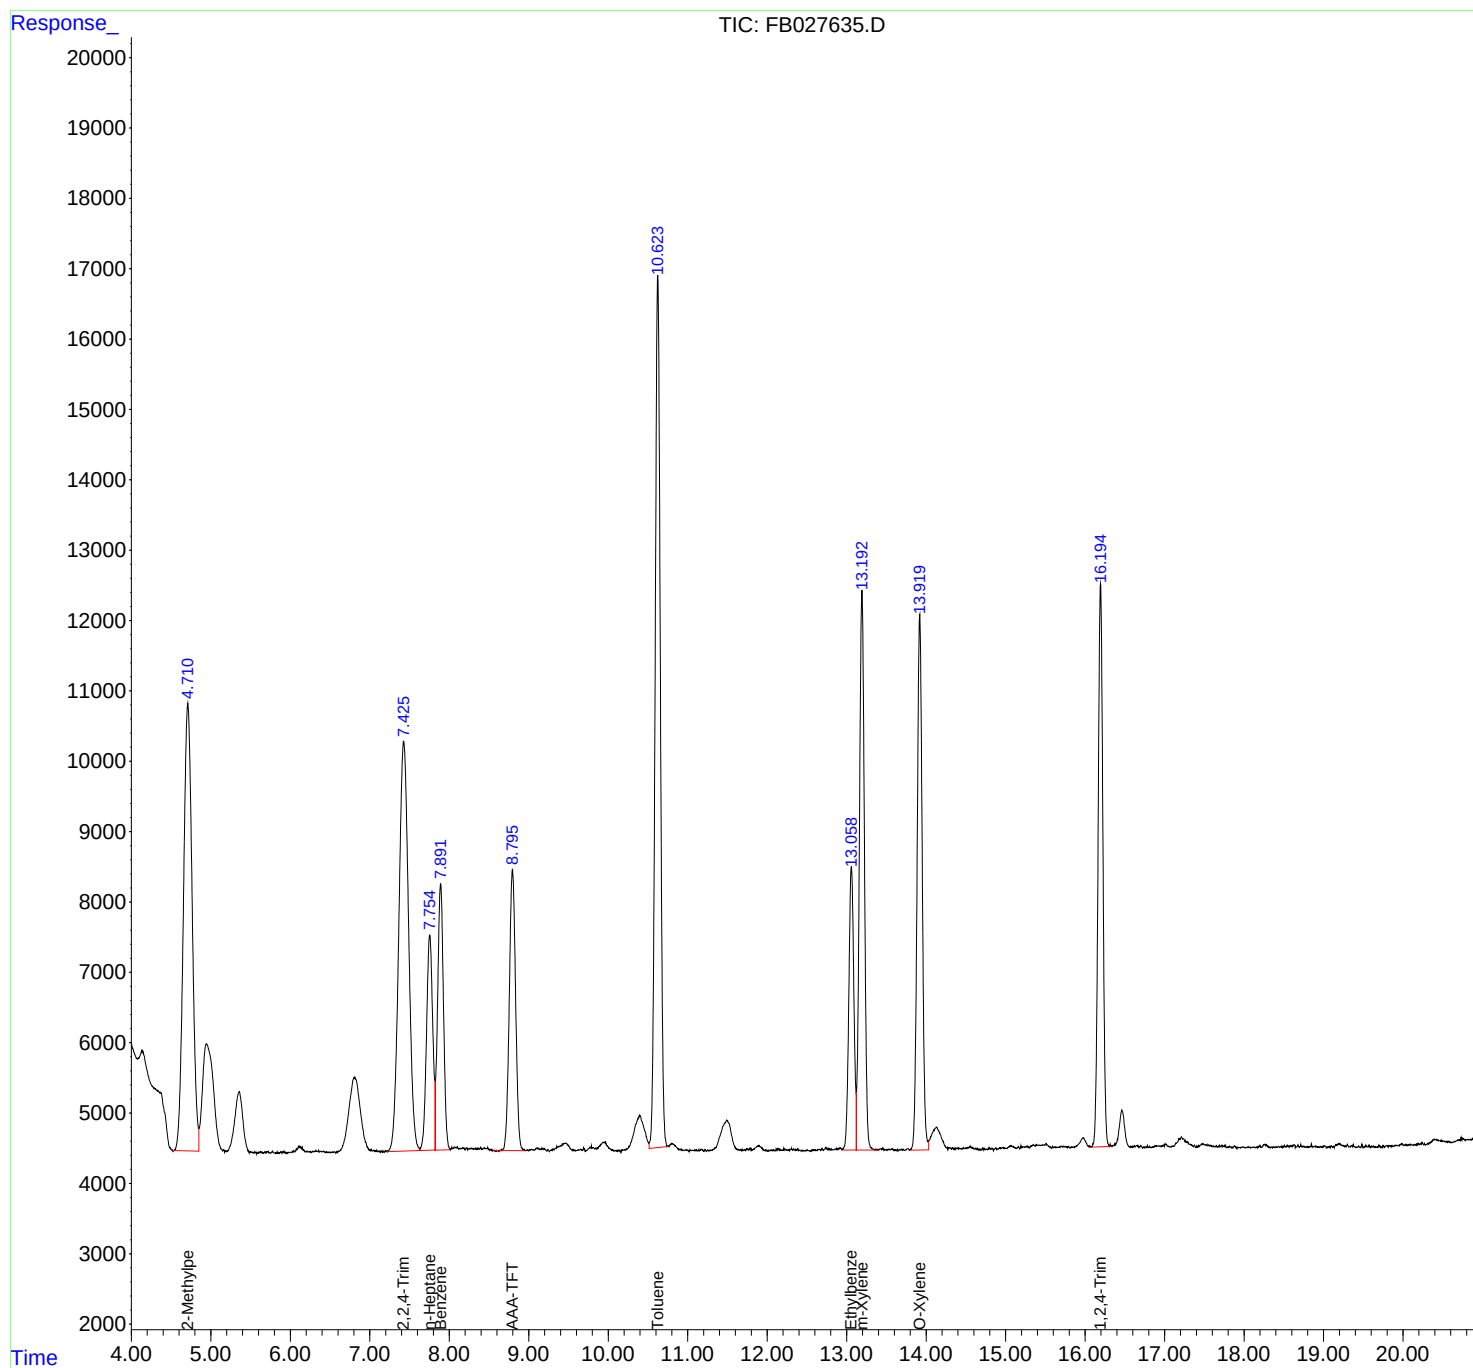

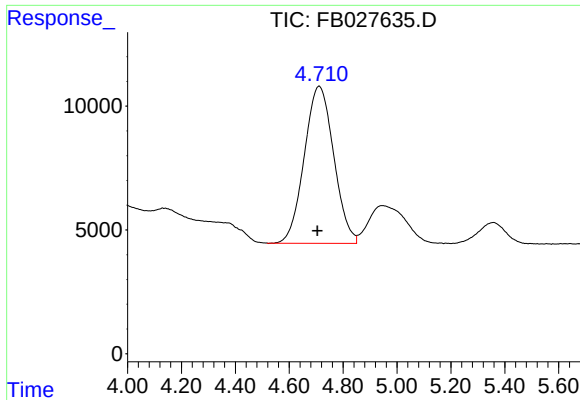


#1 2-Methylpentane

R.T.: 4.712 min
Delta R.T.: 0.008 min
Response: 481712
Conc: 28.59 ng/ml

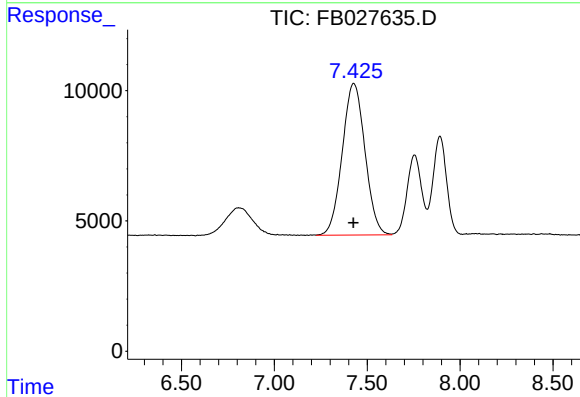


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.000 min
Response: 494362
Conc: 28.16 ng/ml

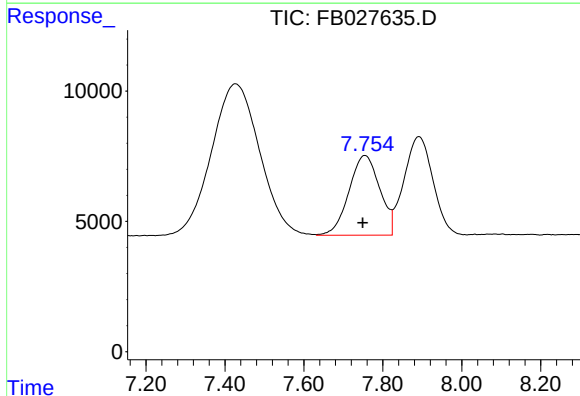


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.006 min
Response: 165987
Conc: 9.47 ng/ml

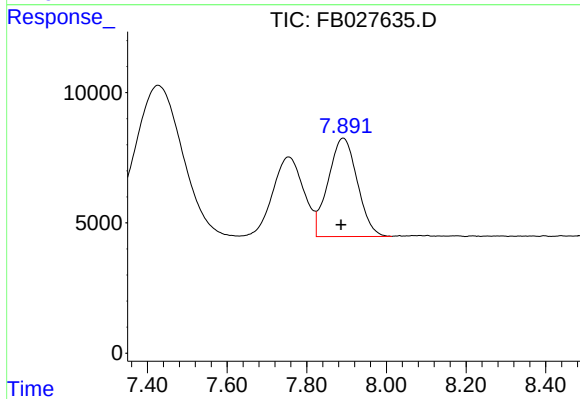


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.006 min
Response: 192407
Conc: 9.44 ng/ml

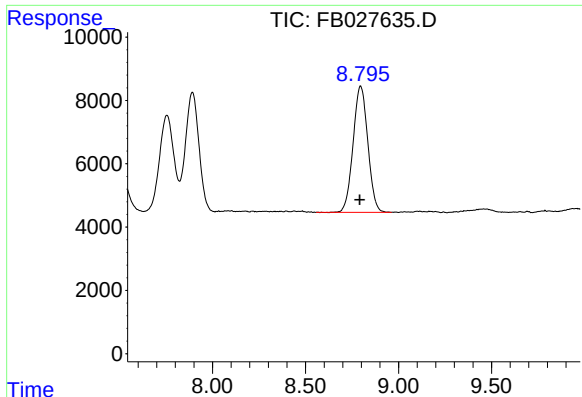


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: 0.005 min
Response: 218831
Conc: 19.51 ng/ml

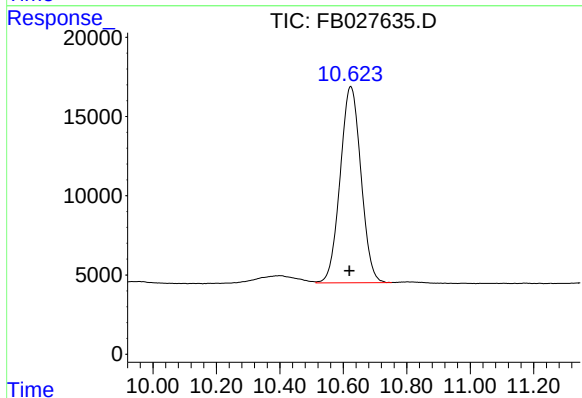


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.005 min
Response: 562806
Conc: 29.07 ng/ml

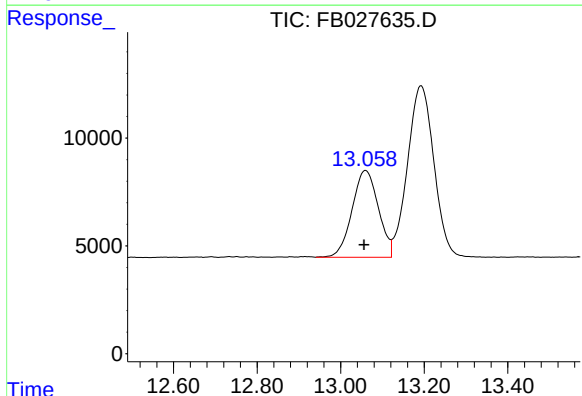


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.004 min
Response: 175793
Conc: 9.71 ng/ml

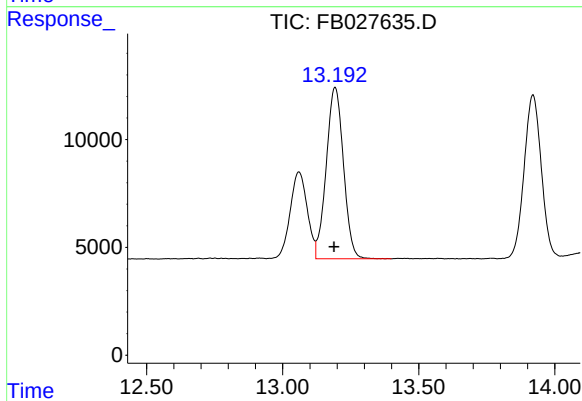

#8 m-Xylene

R.T.: 13.193 min
Delta R.T.: 0.004 min
Response: 349601
Conc: 19.61 ng/ml

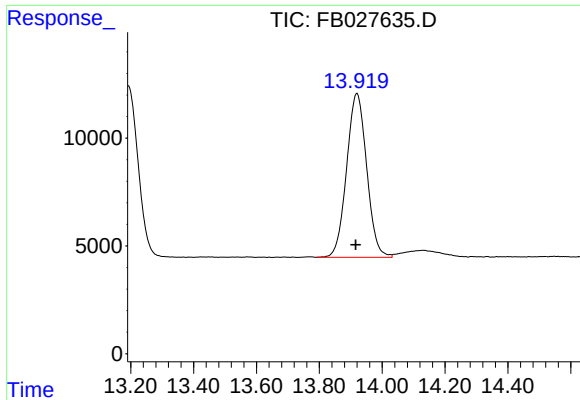


#9 O-Xylene

R.T.: 13.920 min

Delta R.T.: 0.004 min

Response: 336489

Conc: 19.37 ng/ml

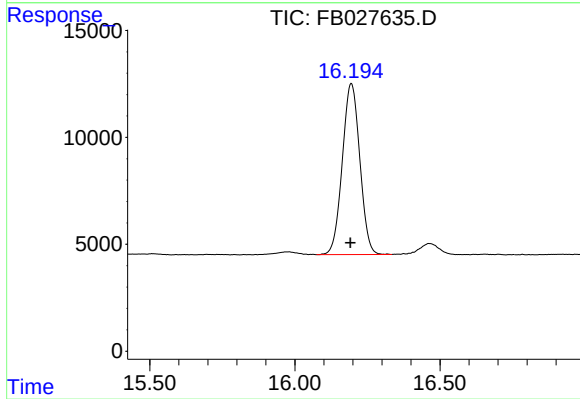

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min

Delta R.T.: 0.004 min

Response: 334958

Conc: 19.50 ng/ml