

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070722\
 Data File : FB027636.D
 Signal(s) : FID2B.CH
 Acq On : 7 Jul 2022 13:46
 Operator : AJ/MA
 Sample : N3581-01MSD
 Misc : 4.87G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 08 03:30:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	214316	19.107 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	501169	29.748 ng/ml
2) t 2,2,4-Trimethylpentane	7.434	549564	31.299 ng/ml
3) t n-Heptane	7.755	163227	9.317 ng/ml
4) t Benzene	7.892	202096	9.910 ng/ml
6) t Toluene	10.624	569100	29.393 ng/ml
7) t Ethylbenzene	13.061	181430	10.019 ng/ml
8) t m-Xylene	13.194	364500	20.448 ng/ml
9) t O-Xylene	13.921	360180	20.729 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	372092	21.661 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070722\
Data File : FB027636.D
Signal(s) : FID2B.CH
Acq On : 7 Jul 2022 13:46
Operator : AJ/MA
Sample : N3581-01MSD
Misc : 4.87G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 08 03:30:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

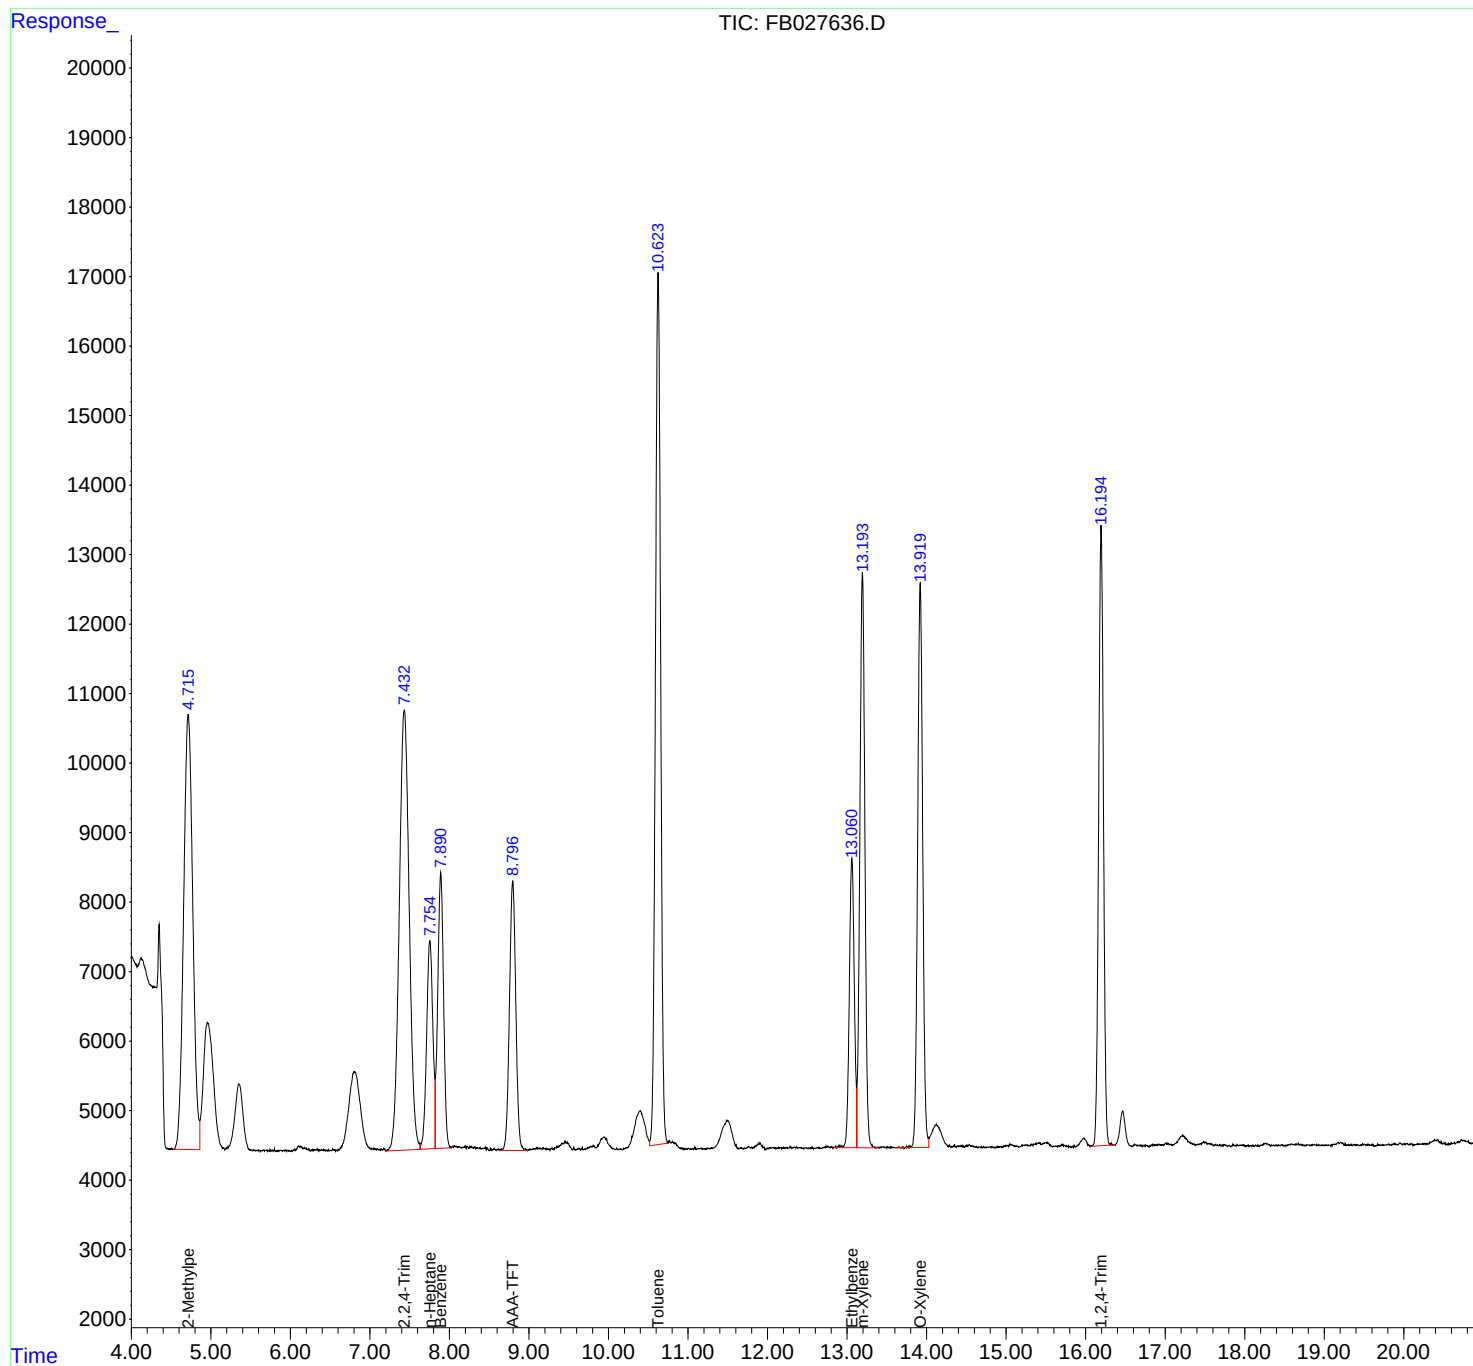

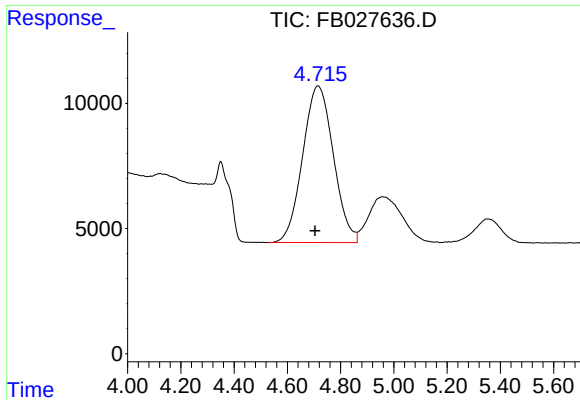


#1 2-Methylpentane

R.T.: 4.716 min
Delta R.T.: 0.012 min
Response: 501169
Conc: 29.75 ng/ml

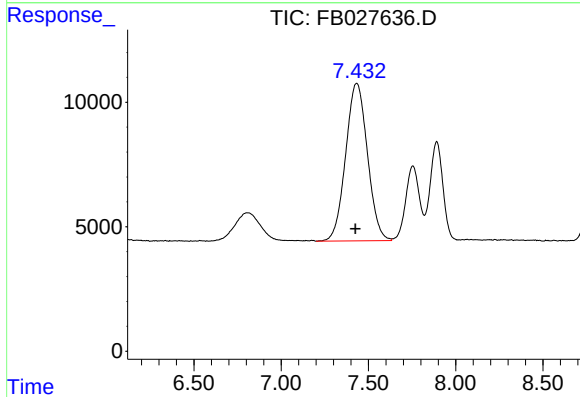


#2 2,2,4-Trimethylpentane

R.T.: 7.434 min
Delta R.T.: 0.007 min
Response: 549564
Conc: 31.30 ng/ml

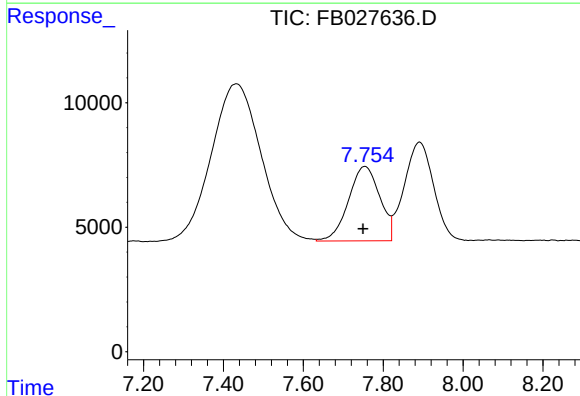


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.005 min
Response: 163227
Conc: 9.32 ng/ml

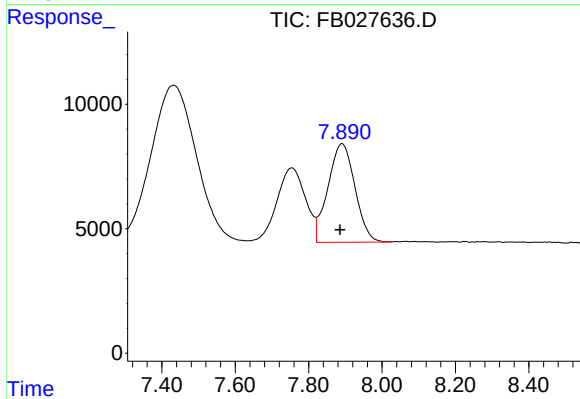


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.006 min
Response: 202096
Conc: 9.91 ng/ml

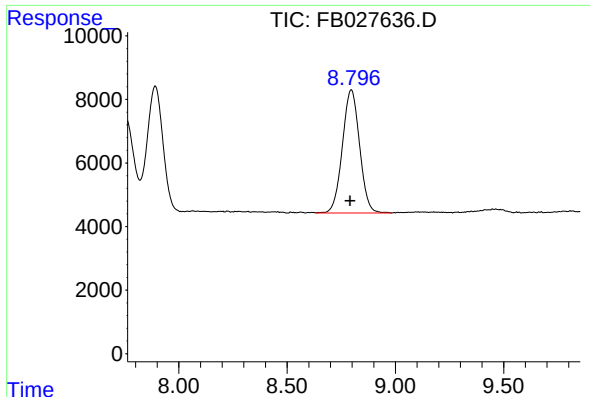


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.006 min
Response: 214316
Conc: 19.11 ng/ml

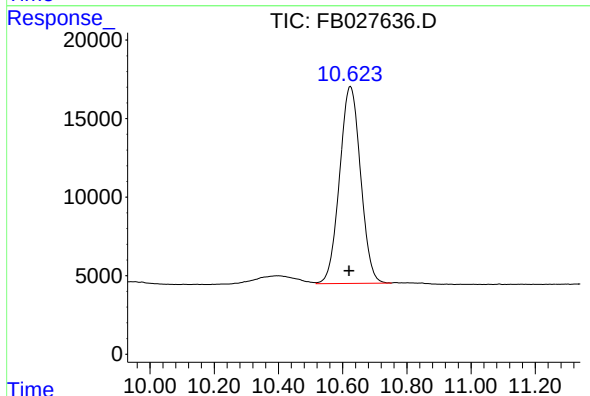


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.005 min
Response: 569100
Conc: 29.39 ng/ml

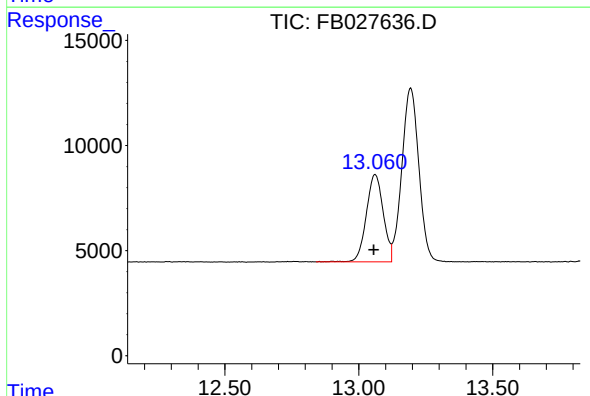


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: 0.005 min
Response: 181430
Conc: 10.02 ng/ml

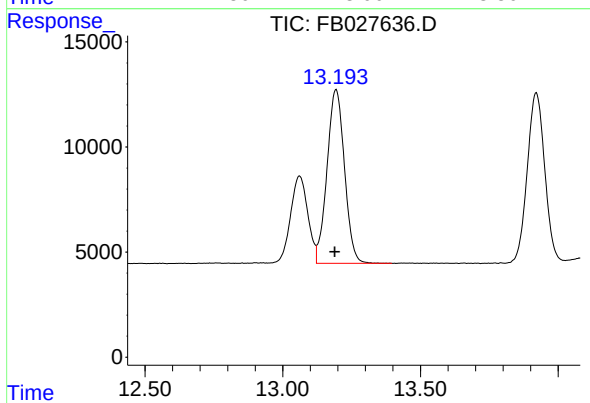


#8 m-Xylene

R.T.: 13.194 min
Delta R.T.: 0.005 min
Response: 364500
Conc: 20.45 ng/ml

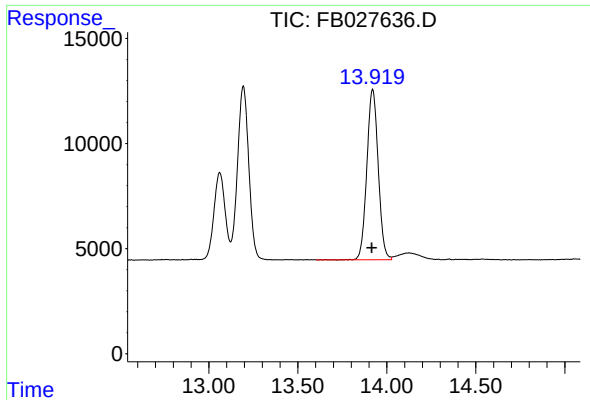

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.005 min
Response: 360180
Conc: 20.73 ng/ml

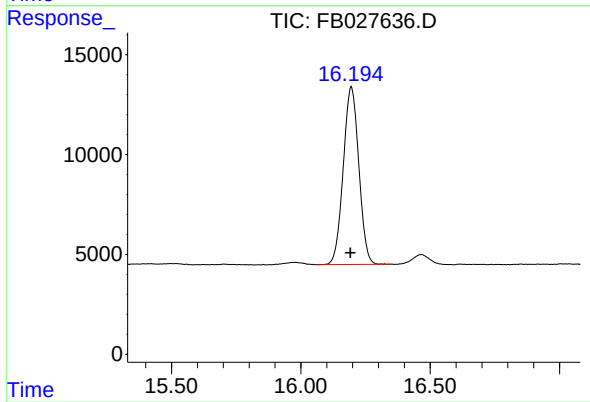

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.004 min
Response: 372092
Conc: 21.66 ng/ml