

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070722\
 Data File : FB027637.D
 Signal(s) : FID2B.CH
 Acq On : 7 Jul 2022 14:24
 Operator : AJ/MA
 Sample : BSF0707S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 08 03:30:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	201553	17.969 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.715	434163	25.771 ng/ml
2) t 2,2,4-Trimethylpentane	7.432	483602	27.543 ng/ml
3) t n-Heptane	7.754	145463	8.303 ng/ml
4) t Benzene	7.892	175948	8.628 ng/ml
6) t Toluene	10.625	604808	31.237 ng/ml
7) t Ethylbenzene	13.061	161365	8.911 ng/ml
8) t m-Xylene	13.194	325351	18.251 ng/ml
9) t O-Xylene	13.921	320789	18.462 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	336581	19.593 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070722\
Data File : FB027637.D
Signal(s) : FID2B.CH
Acq On : 7 Jul 2022 14:24
Operator : AJ/MA
Sample : BSF0707S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 08 03:30:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

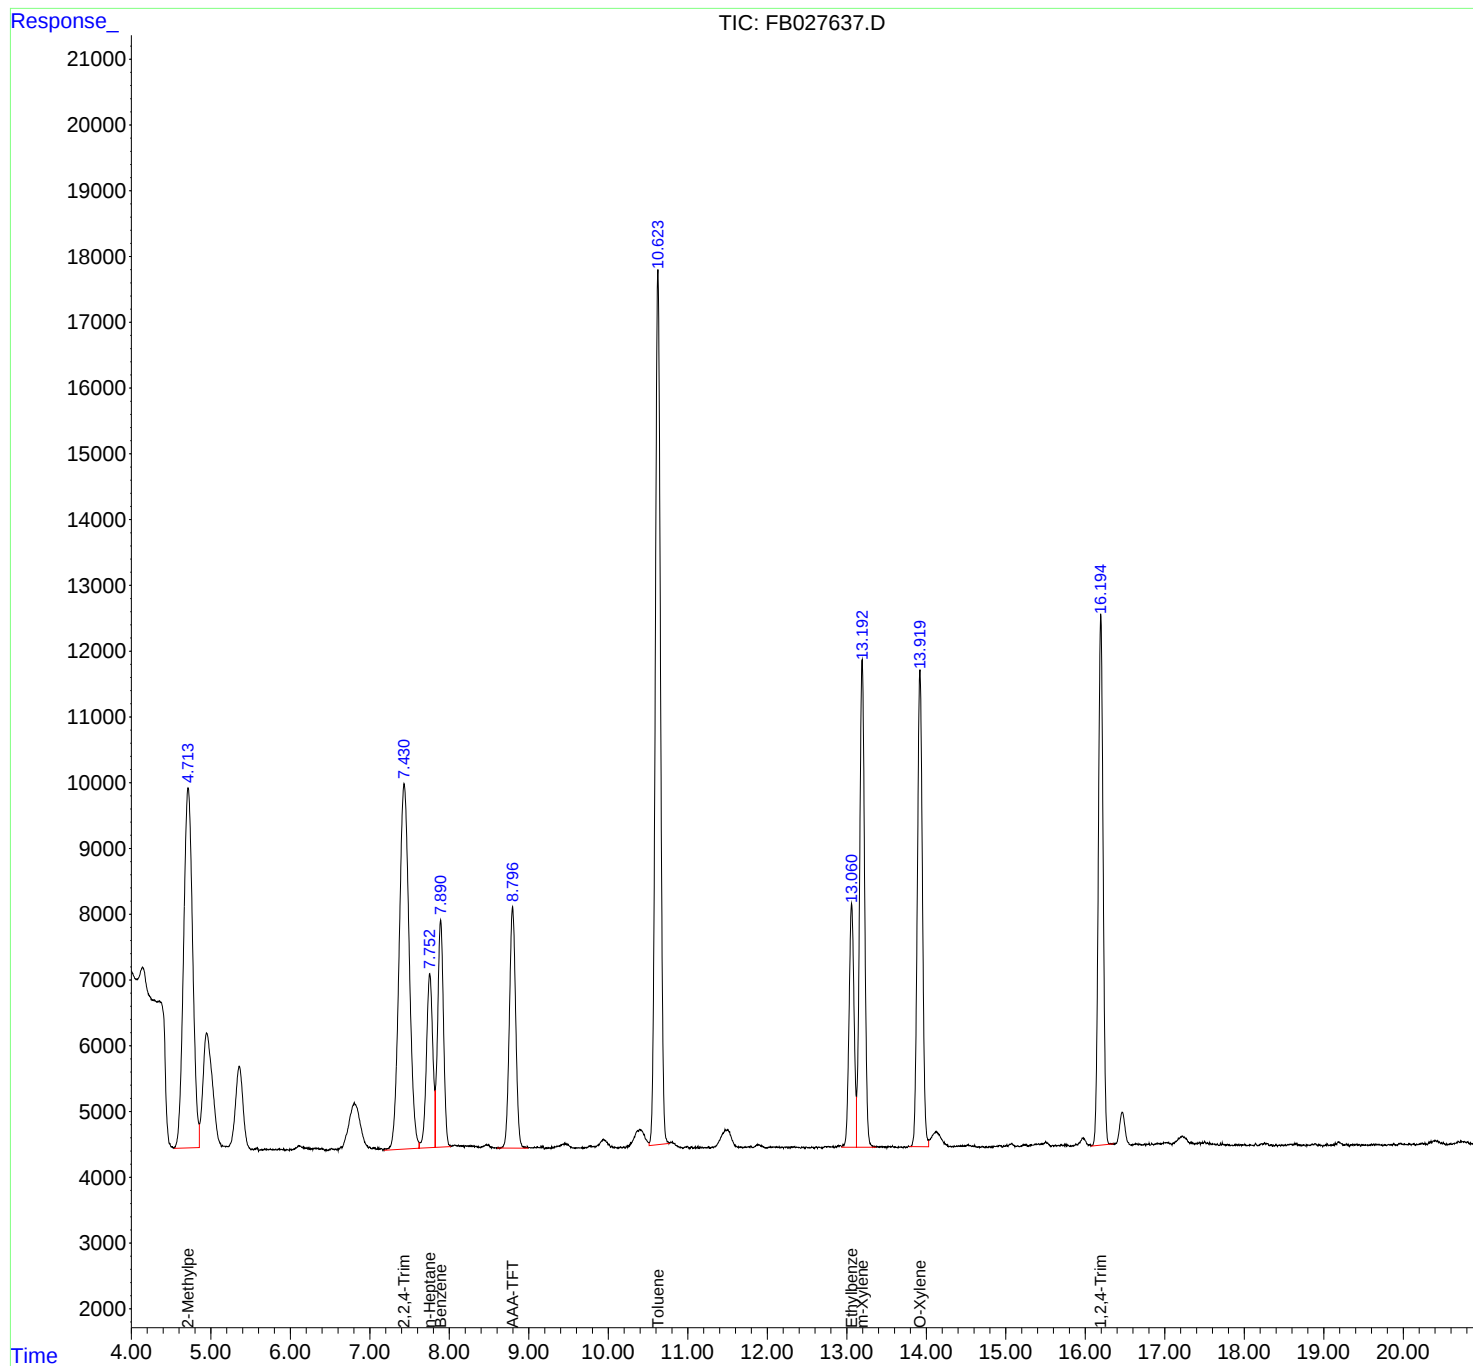

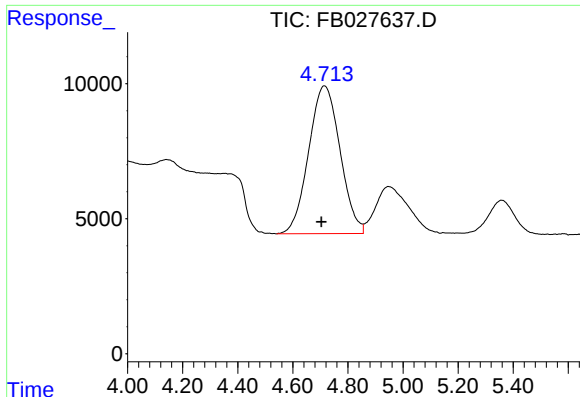


#1 2-Methylpentane

R.T.: 4.715 min
Delta R.T.: 0.011 min
Response: 434163
Conc: 25.77 ng/ml

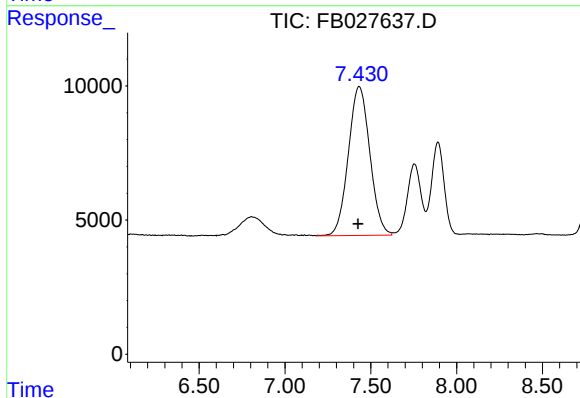


#2 2,2,4-Trimethylpentane

R.T.: 7.432 min
Delta R.T.: 0.006 min
Response: 483602
Conc: 27.54 ng/ml

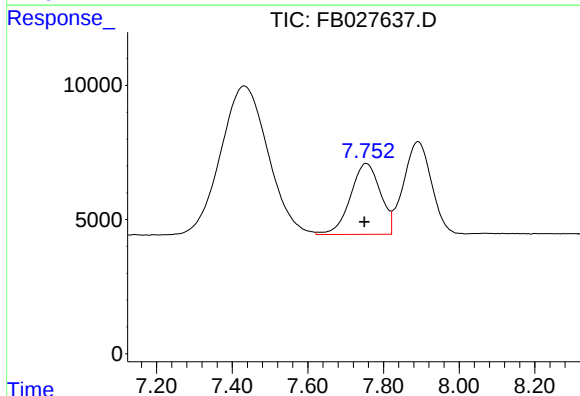


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.004 min
Response: 145463
Conc: 8.30 ng/ml

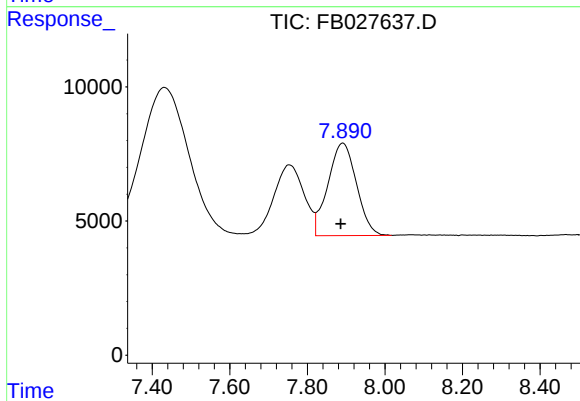


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.006 min
Response: 175948
Conc: 8.63 ng/ml

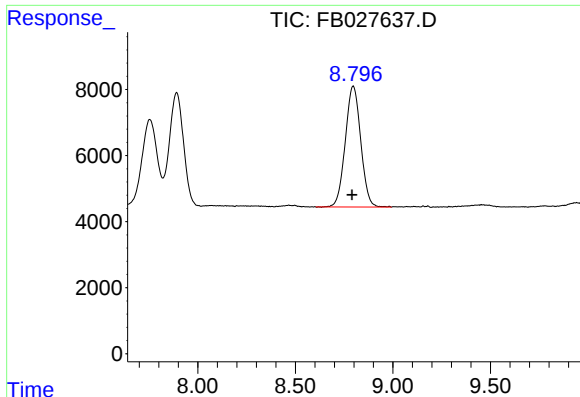


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.006 min
Response: 201553
Conc: 17.97 ng/ml

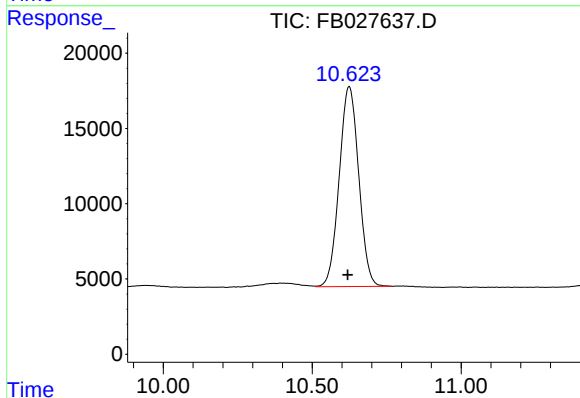


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.005 min
Response: 604808
Conc: 31.24 ng/ml

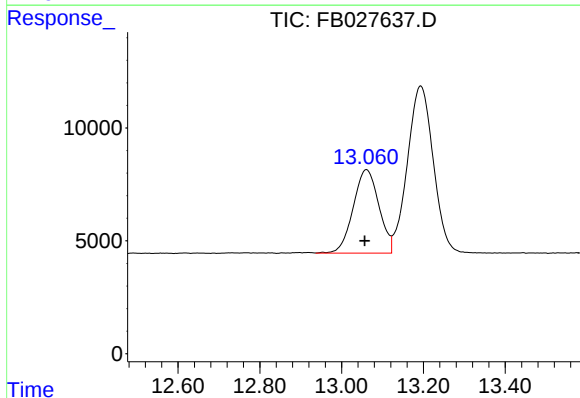


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: 0.005 min
Response: 161365
Conc: 8.91 ng/ml

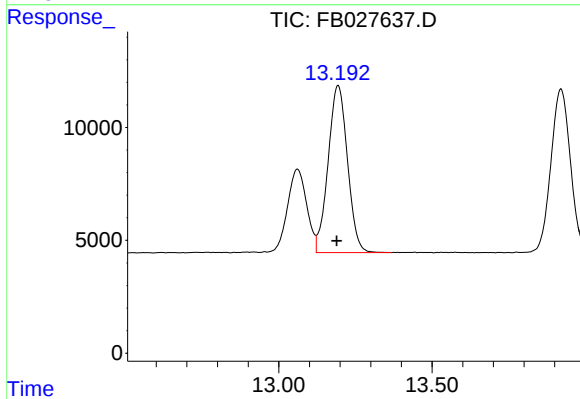


#8 m-Xylene

R.T.: 13.194 min
Delta R.T.: 0.005 min
Response: 325351
Conc: 18.25 ng/ml

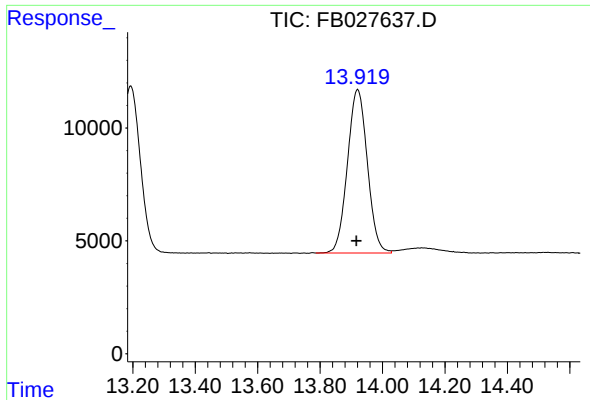

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.005 min
Response: 320789
Conc: 18.46 ng/ml

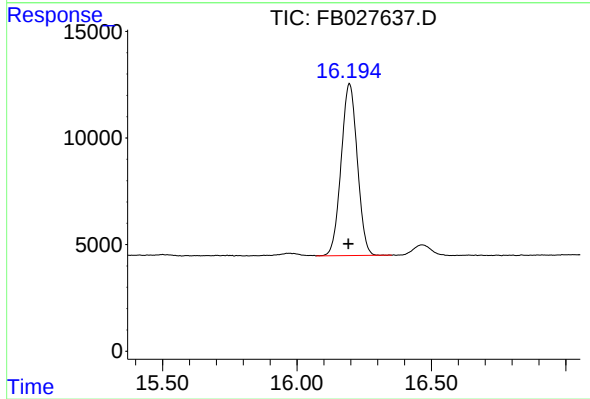

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.004 min
Response: 336581
Conc: 19.59 ng/ml