

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB070820\  
 Data File : FB024546.D  
 Signal(s) : FID2B.CH  
 Acq On : 8 Jul 2020 9:44  
 Operator : DD/AJ  
 Sample : VBF0708S1  
 Misc : 5.00gm/5.00ml DI WATER  
 ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e  
 Quant Time: Jul 09 00:53:19 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB060920.M  
 Quant Title :  
 QLast Update : Tue Jun 09 11:17:18 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.797  | 490043   | 20.255 ng/ml |
| Target Compounds             |        |          |              |
| 1) t 2-Methylpentane         | 4.693  | 1225     | 0.038 ng/ml  |
| 2) t 2,2,4-Trimethylpentane  | 7.428  | 555      | 0.017 ng/ml  |
| 6) t Toluene                 | 10.626 | 8398     | 0.214 ng/ml  |
| 7) t Ethylbenzene            | 13.076 | 3326     | 0.095 ng/ml  |
| 8) t m-Xylene                | 13.206 | 8365     | 0.244 ng/ml  |
| 9) t o-Xylene                | 13.936 | 1165     | 0.035 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.208 | 2677     | 0.096 ng/ml  |
| -----                        |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB070820\  
Data File : FB024546.D  
Signal(s) : FID2B.CH  
Acq On : 8 Jul 2020 9:44  
Operator : DD/AJ  
Sample : VBF0708S1  
Misc : 5.00gm/5.00ml DI WATER  
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Jul 09 00:53:19 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB060920.M  
Quant Title :  
QLast Update : Tue Jun 09 11:17:18 2020  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

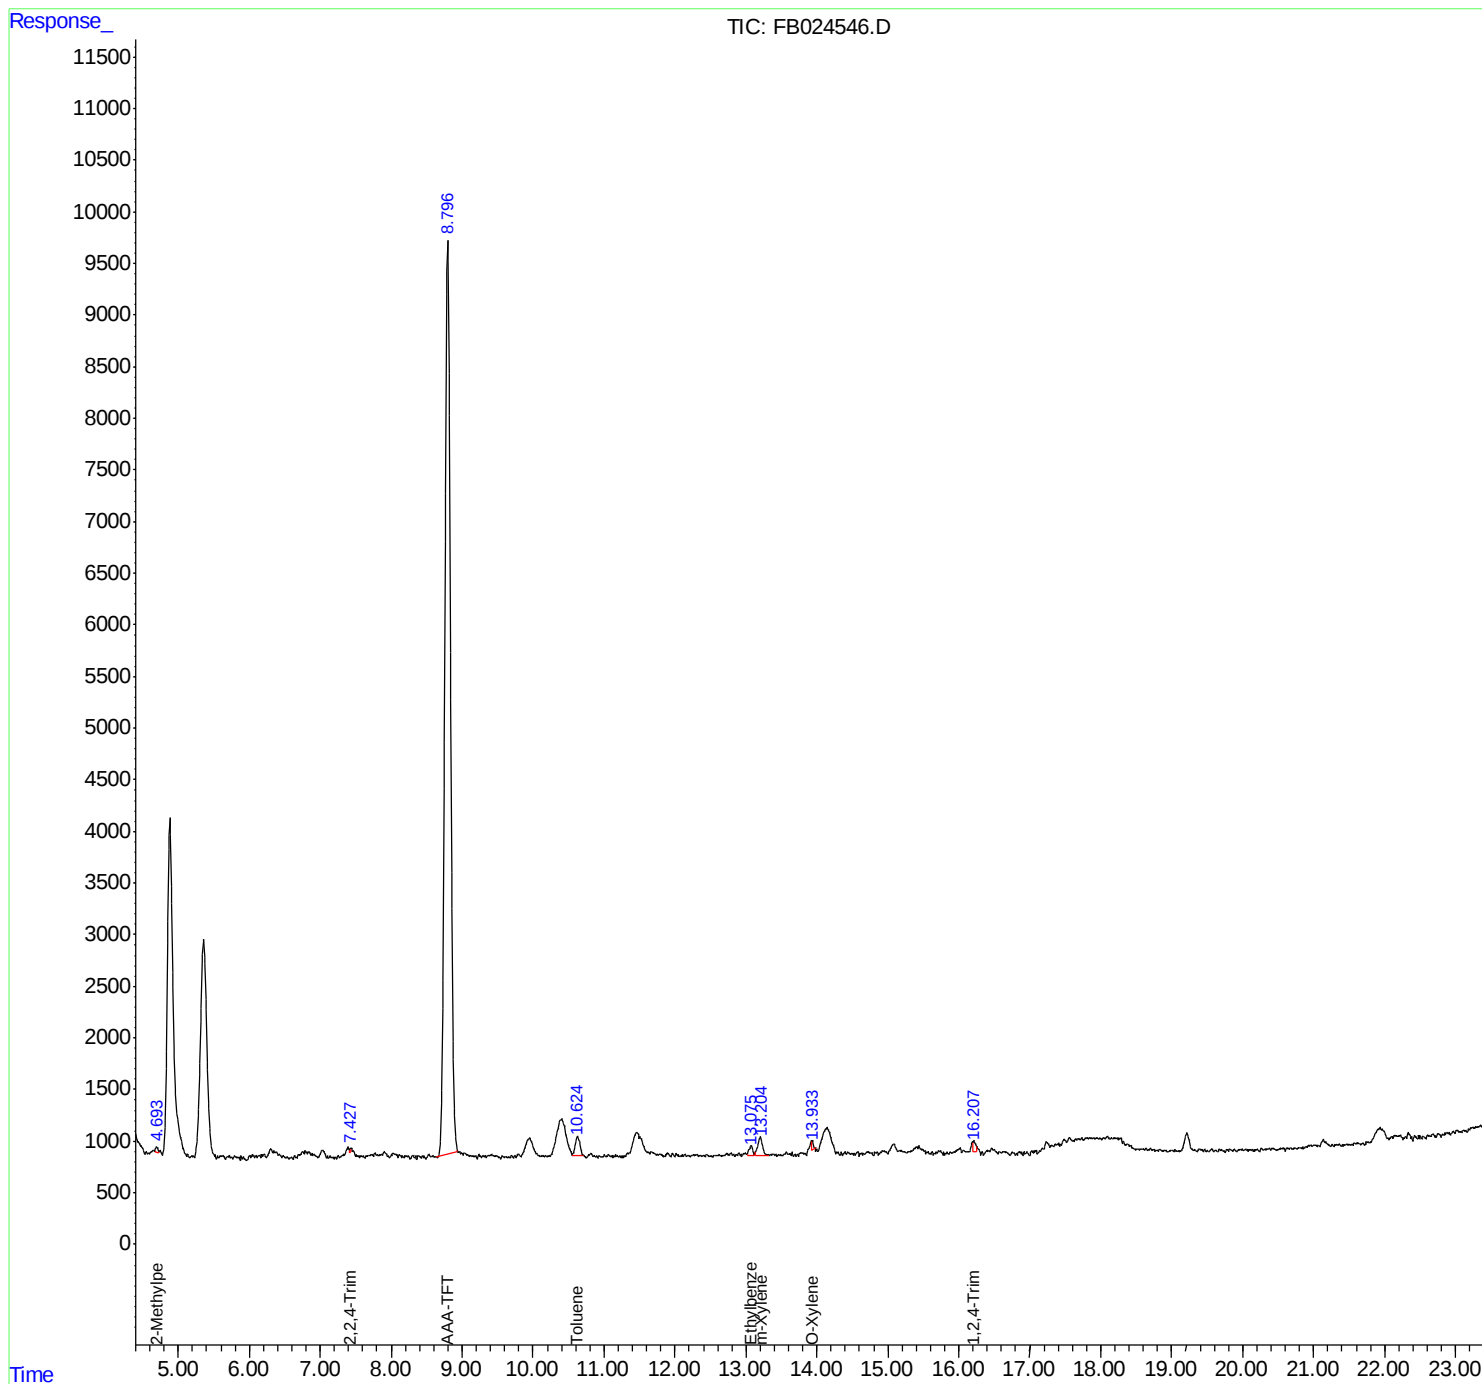

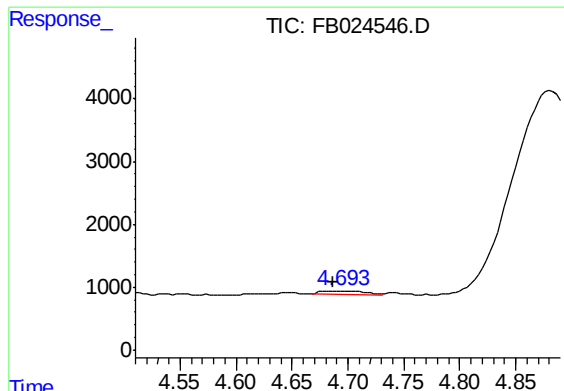


#1 2-Methylpentane

R.T.: 4.693 min  
Delta R.T.: 0.006 min  
Response: 1225  
Conc: 0.04 ng/ml

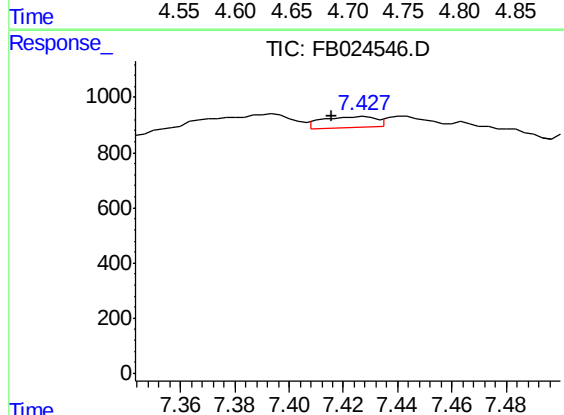


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min  
Delta R.T.: 0.012 min  
Response: 555  
Conc: 0.02 ng/ml

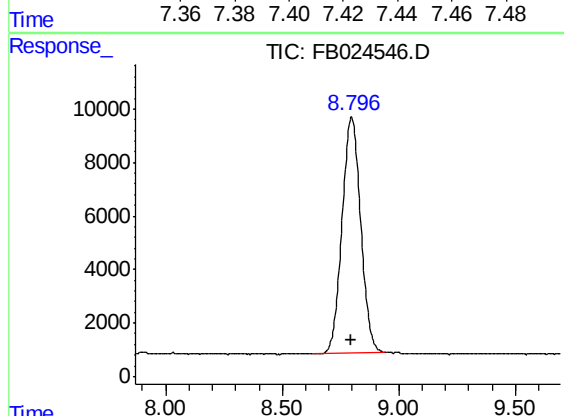


#5 AAA-TFT

R.T.: 8.797 min  
Delta R.T.: 0.000 min  
Response: 490043  
Conc: 20.25 ng/ml

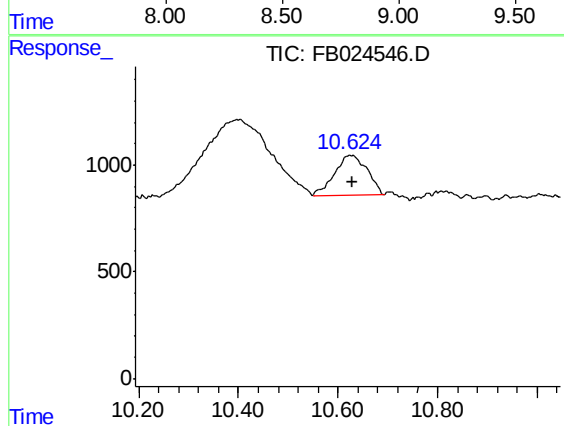


#6 Toluene

R.T.: 10.626 min  
Delta R.T.: -0.003 min  
Response: 8398  
Conc: 0.21 ng/ml

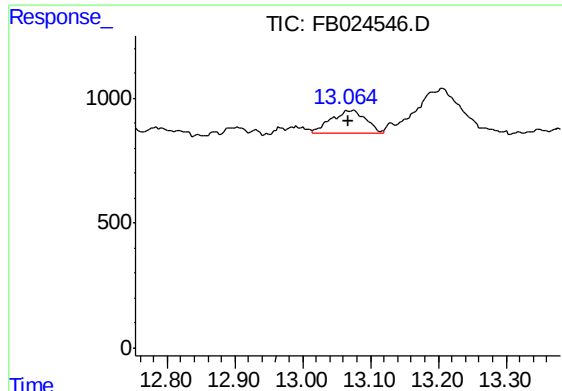


#7 Ethylbenzene

R.T.: 13.076 min  
Delta R.T.: 0.009 min  
Response: 3326  
Conc: 0.09 ng/ml

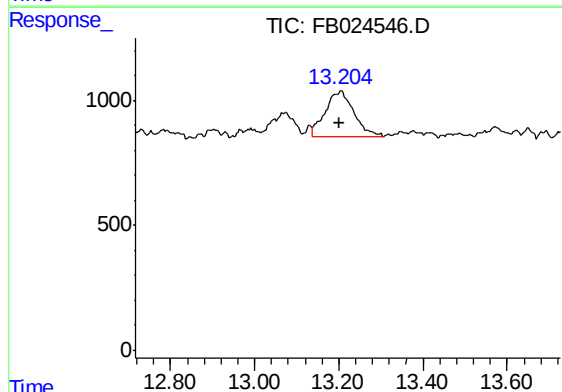


#8 m-Xylene

R.T.: 13.206 min  
Delta R.T.: 0.005 min  
Response: 8365  
Conc: 0.24 ng/ml

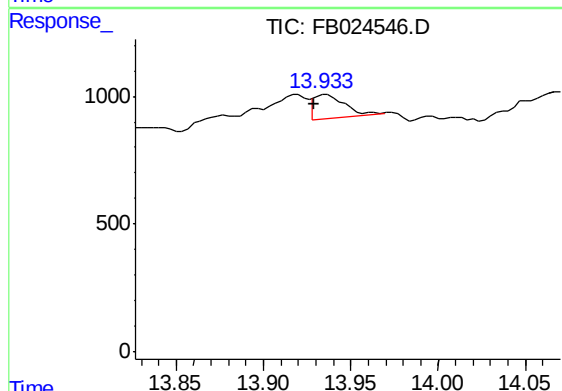

#9 O-Xylene

R.T.: 13.936 min  
Delta R.T.: 0.007 min  
Response: 1165  
Conc: 0.03 ng/ml

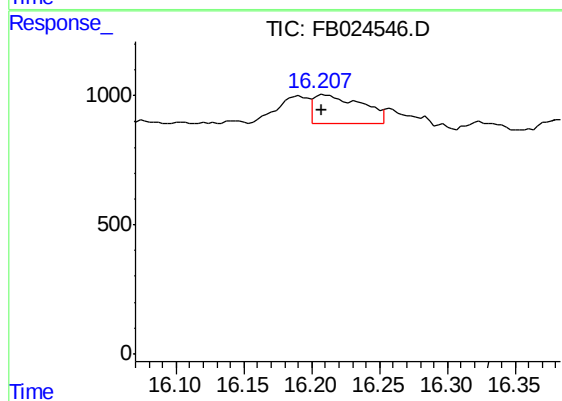

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min  
Delta R.T.: 0.001 min  
Response: 2677  
Conc: 0.10 ng/ml