

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070820\
Data File : FB024549.D
Signal(s) : FID2B.CH
Acq On : 8 Jul 2020 11:41
Operator : DD/AJ
Sample : L3187-02
Misc : 5.06gm/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 09 00:53:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	473413	19.567 ng/ml
Target Compounds			
6) t Toluene	10.633	4184	0.106 ng/ml
8) t m-Xylene	13.207	2470	0.072 ng/ml
9) t O-Xylene	13.941	788	0.024 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070820\
Data File : FB024549.D
Signal(s) : FID2B.CH
Acq On : 8 Jul 2020 11:41
Operator : DD/AJ
Sample : L3187-02
Misc : 5.06gm/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 09 00:53:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

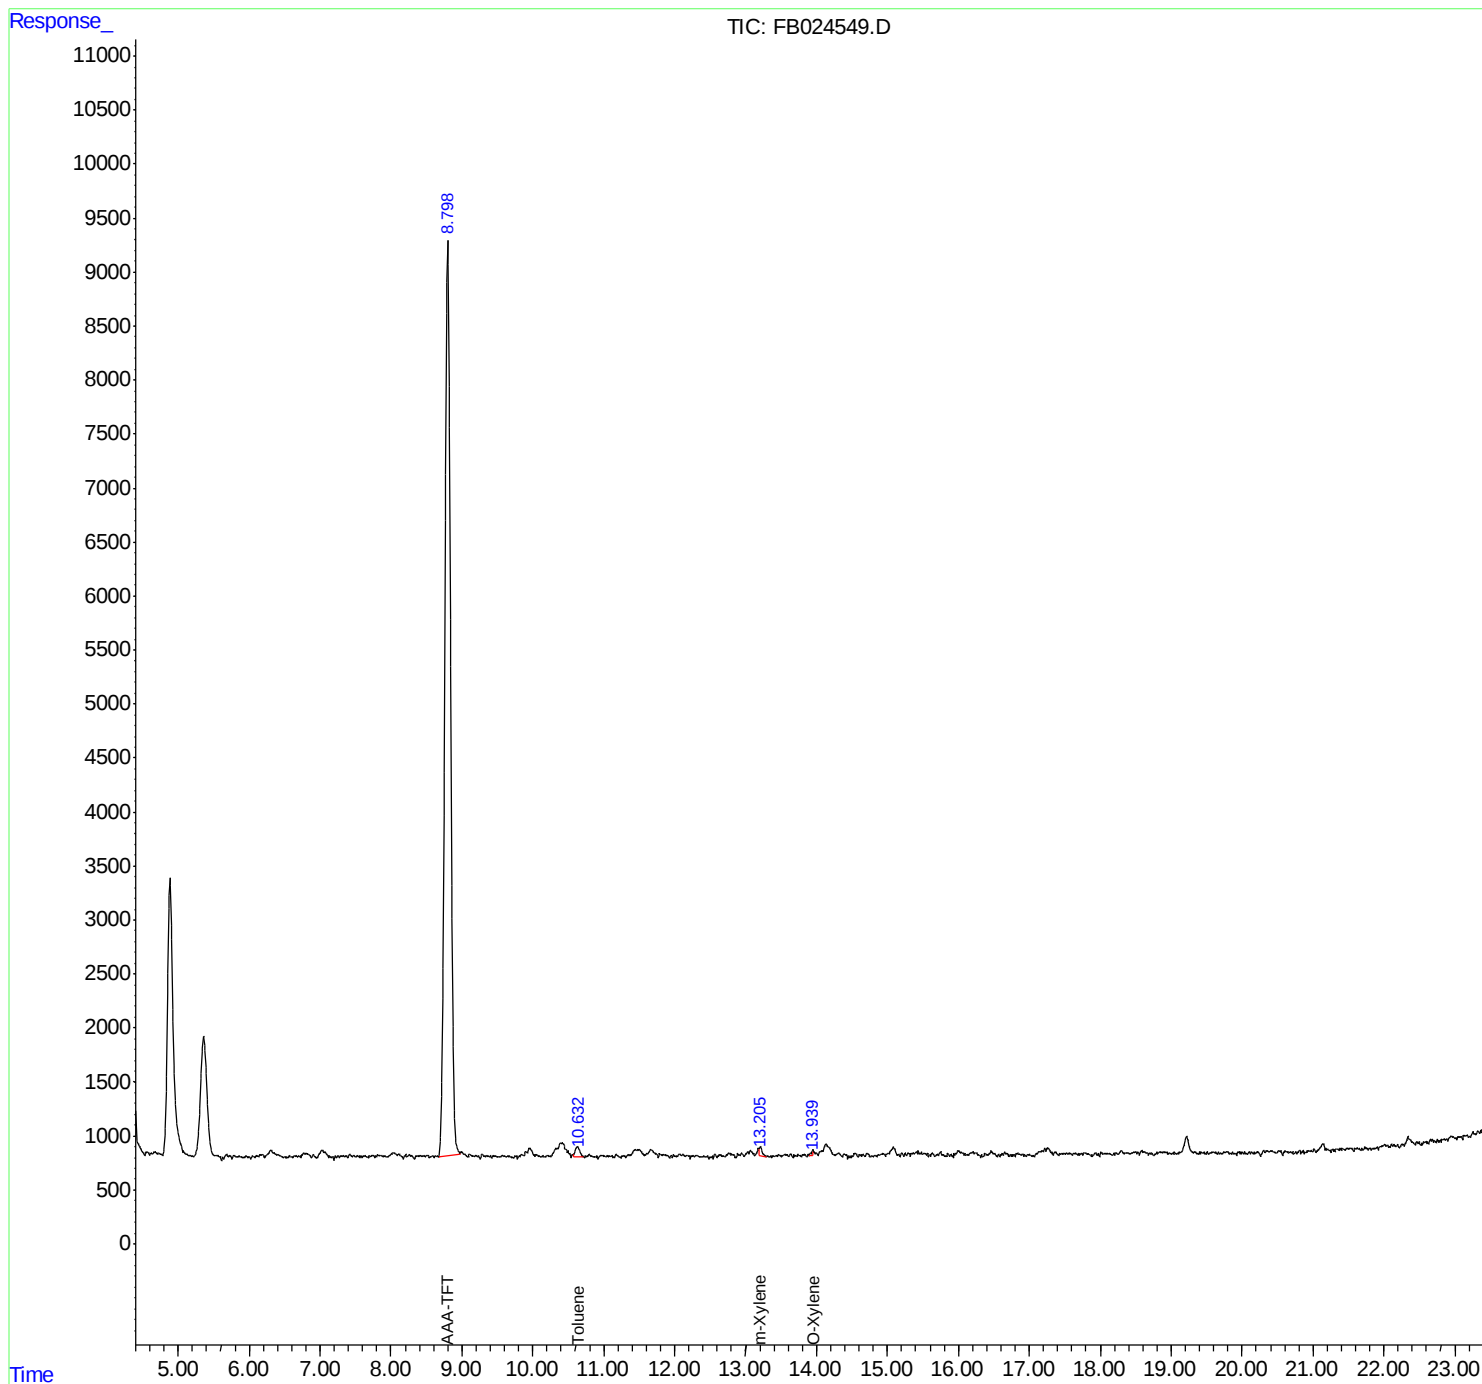

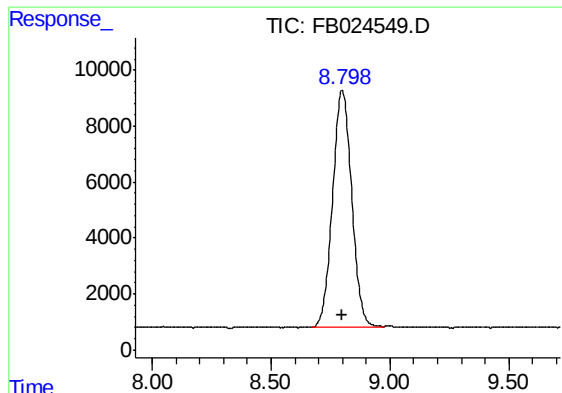


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.002 min
Response: 473413
Conc: 19.57 ng/ml

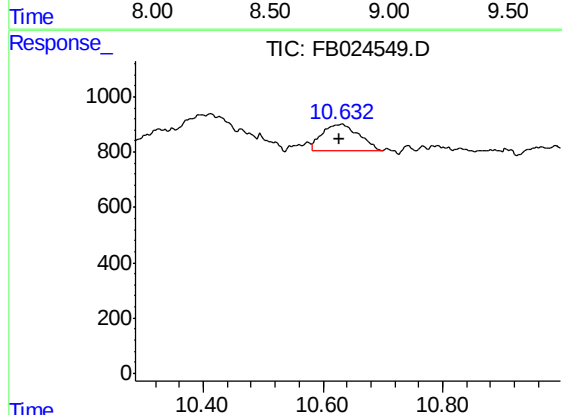


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.005 min
Response: 4184
Conc: 0.11 ng/ml

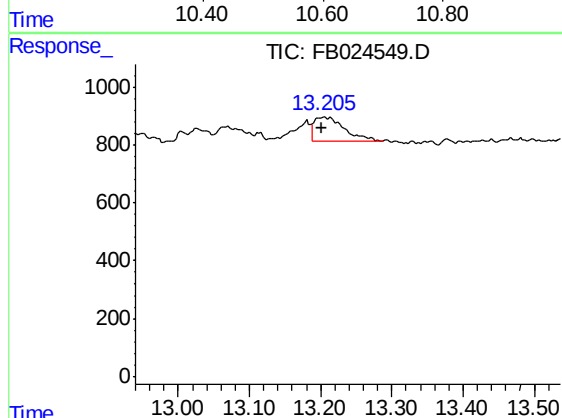

#8 m-Xylene

R.T.: 13.207 min
Delta R.T.: 0.005 min
Response: 2470
Conc: 0.07 ng/ml

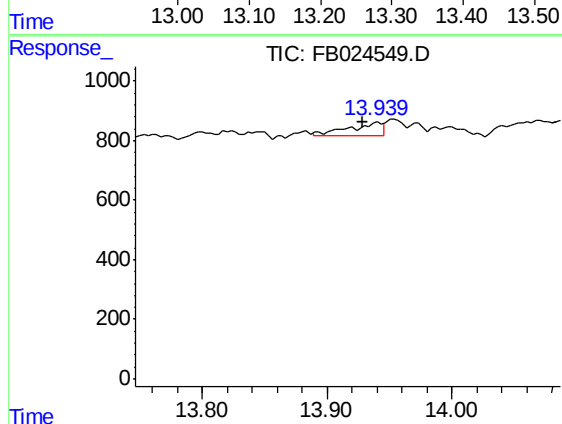

#9 O-Xylene

R.T.: 13.941 min
Delta R.T.: 0.012 min
Response: 788
Conc: 0.02 ng/ml