

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070820\
 Data File : FB024547.D
 Signal(s) : FID2B.CH
 Acq On : 8 Jul 2020 10:15
 Operator : DD/AJ
 Sample : BSF0708S1
 Misc : 5.01gm/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 09 00:53:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	521444	21.553 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	984064	30.787 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	1073435	32.020 ng/ml
3) t n-Heptane	7.757	354922	10.495 ng/ml
4) t Benzene	7.891	427109	10.565 ng/ml
6) t Toluene	10.629	1204638	30.654 ng/ml
7) t Ethylbenzene	13.069	362831	10.340 ng/ml
8) t m-Xylene	13.202	717103	20.940 ng/ml
9) t O-Xylene	13.930	705333	21.038 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	599964	21.608 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070820\
Data File : FB024547.D
Signal(s) : FID2B.CH
Acq On : 8 Jul 2020 10:15
Operator : DD/AJ
Sample : BSF0708S1
Misc : 5.01gm/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 09 00:53:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

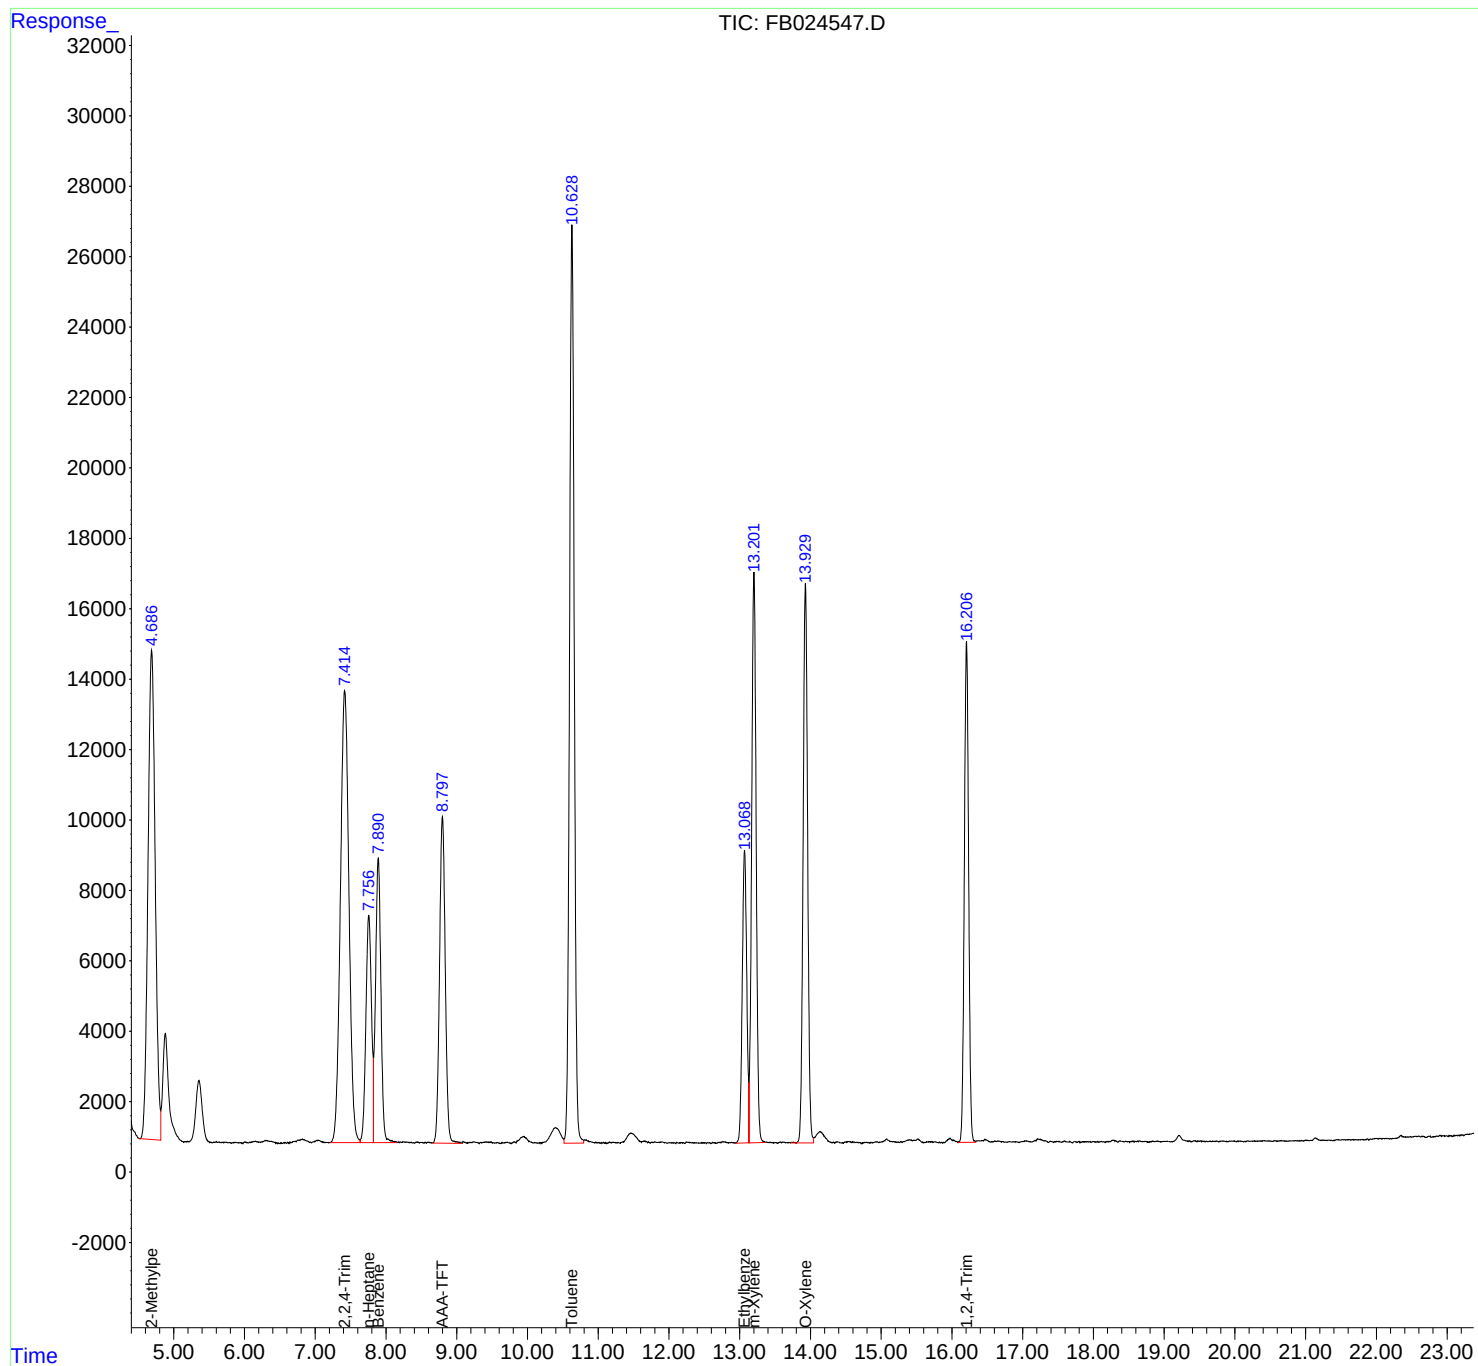

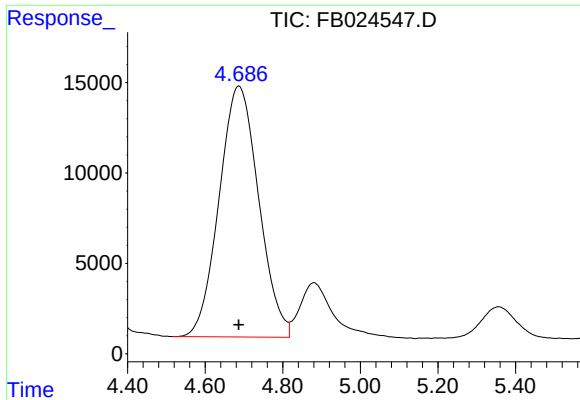


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 984064
Conc: 30.79 ng/ml

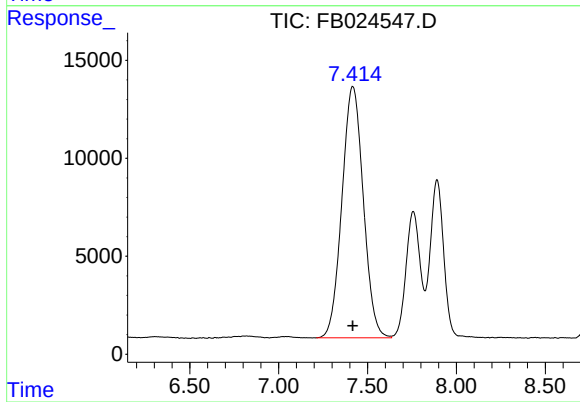


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 1073435
Conc: 32.02 ng/ml

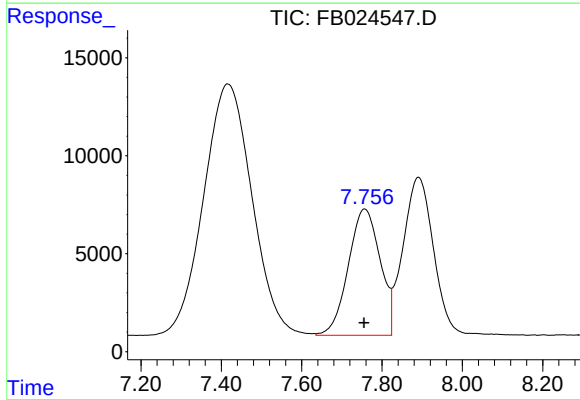


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.002 min
Response: 354922
Conc: 10.50 ng/ml

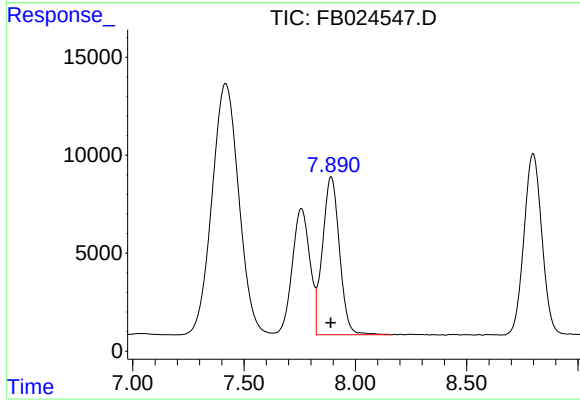


#4 Benzene

R.T.: 7.891 min
Delta R.T.: 0.001 min
Response: 427109
Conc: 10.57 ng/ml

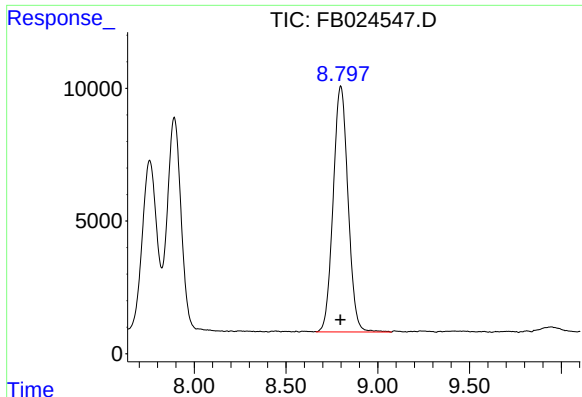


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.002 min
Response: 521444
Conc: 21.55 ng/ml

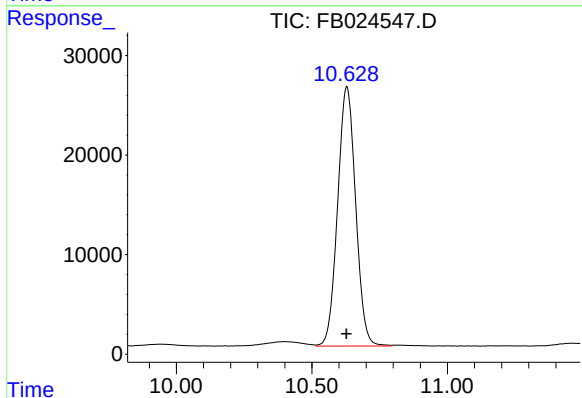


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.001 min
Response: 1204638
Conc: 30.65 ng/ml

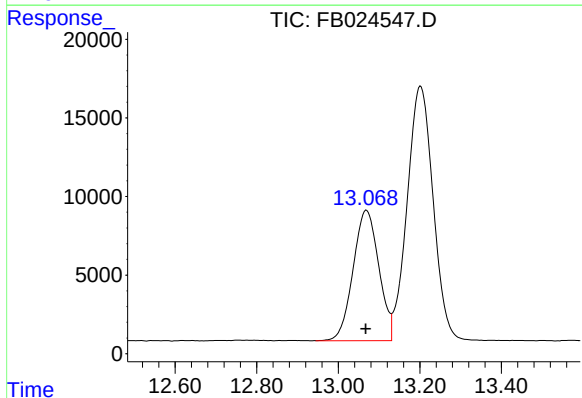


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.001 min
Response: 362831
Conc: 10.34 ng/ml

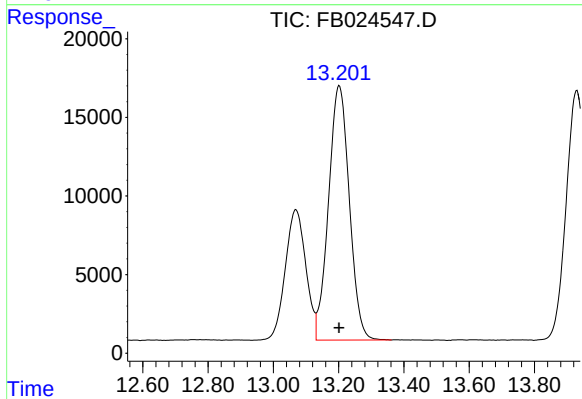


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: 0.000 min
Response: 717103
Conc: 20.94 ng/ml

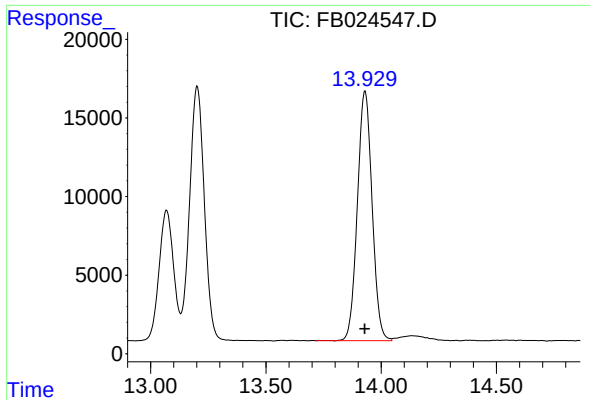

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: 0.000 min
Response: 705333
Conc: 21.04 ng/ml

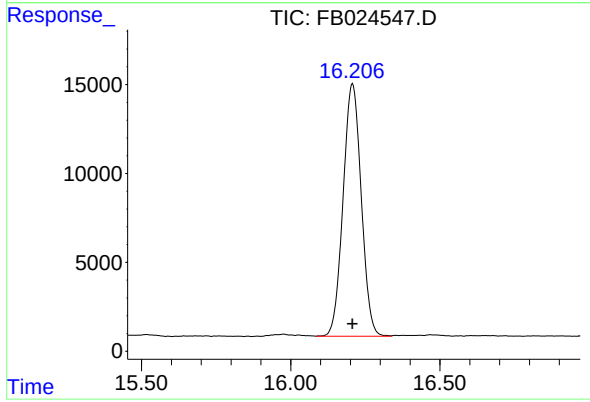

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: 0.000 min
Response: 599964
Conc: 21.61 ng/ml