

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070821\
 Data File : FB025999.D
 Signal(s) : FID2B.CH
 Acq On : 8 Jul 2021 11:04
 Operator : AJ/MA
 Sample : BSF0708S1
 Misc : 5.00g/5.00 ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 08 21:40:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
 Quant Title :
 QLast Update : Wed Jun 09 13:39:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.226	563735	23.327 ng/ml
Target Compounds				
1) t	2-Methylpentane	5.189	645371	24.523 ng/ml
2) t	2,2,4-Trimethylpentane	7.883	573365	28.462 ng/ml
3) t	n-Heptane	8.202	301500	8.388 ng/ml
4) t	Benzene	8.354	390688	9.359 ng/ml
6) t	Toluene	11.044	1096523	26.646 ng/ml
7) t	Ethylbenzene	13.449	334586	8.779 ng/ml
8) t	m-Xylene	13.580	641780	16.325 ng/ml
9) t	O-Xylene	14.302	565051	17.722 ng/ml
10) t	1,2,4-Trimethylbenzene	16.553	352250	17.896 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070821\
Data File : FB025999.D
Signal(s) : FID2B.CH
Acq On : 8 Jul 2021 11:04
Operator : AJ/MA
Sample : BSF0708S1
Misc : 5.00g/5.00 ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 08 21:40:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

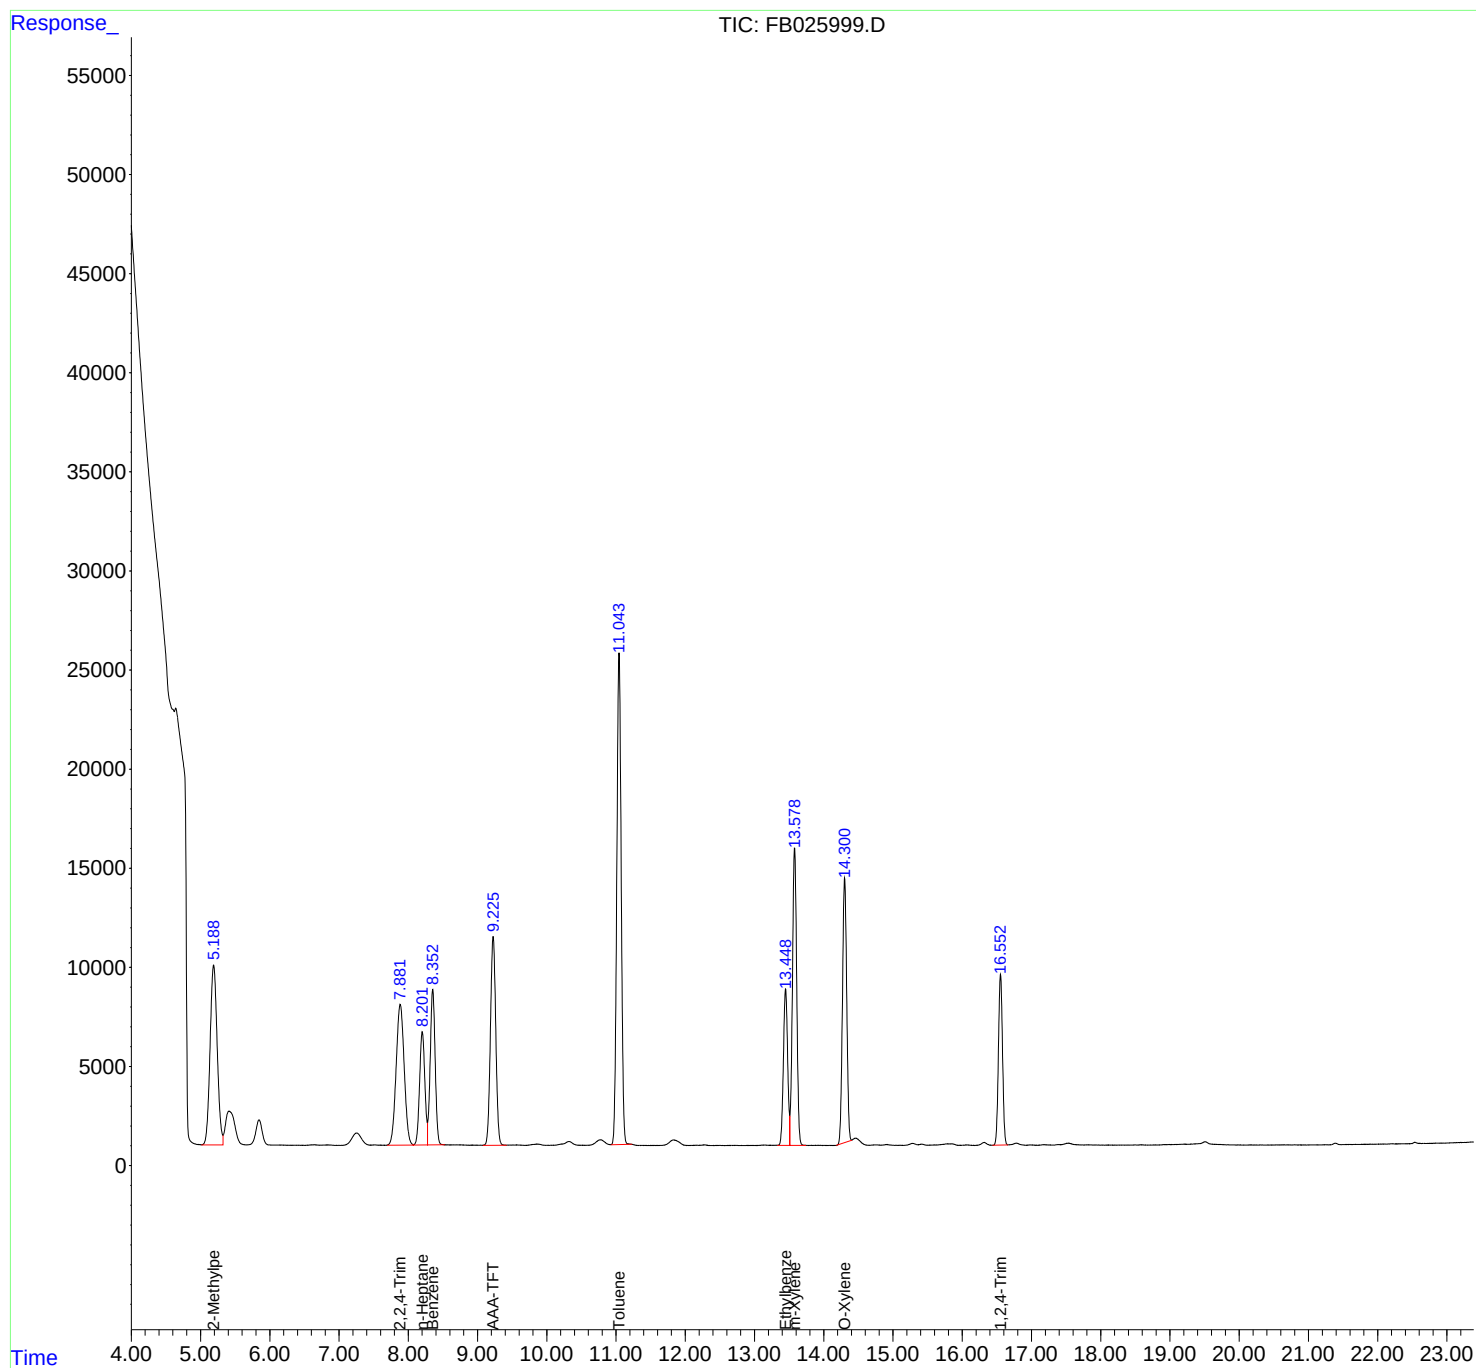

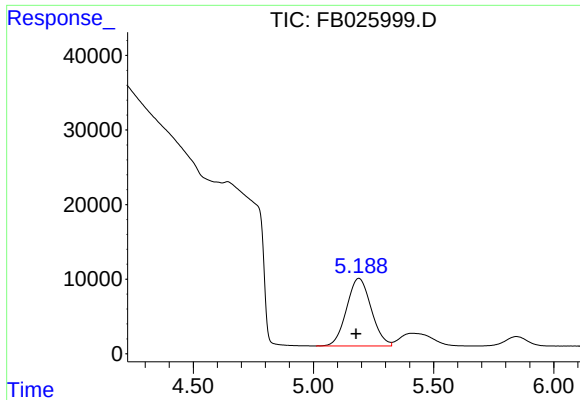


#1 2-Methylpentane

R.T.: 5.189 min
Delta R.T.: 0.012 min
Response: 645371
Conc: 24.52 ng/ml

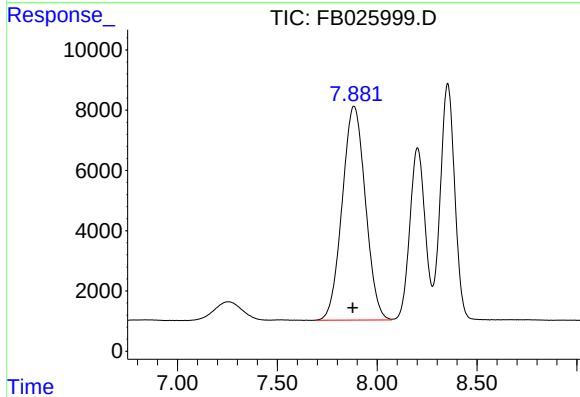


#2 2,2,4-Trimethylpentane

R.T.: 7.883 min
Delta R.T.: 0.005 min
Response: 573365
Conc: 28.46 ng/ml

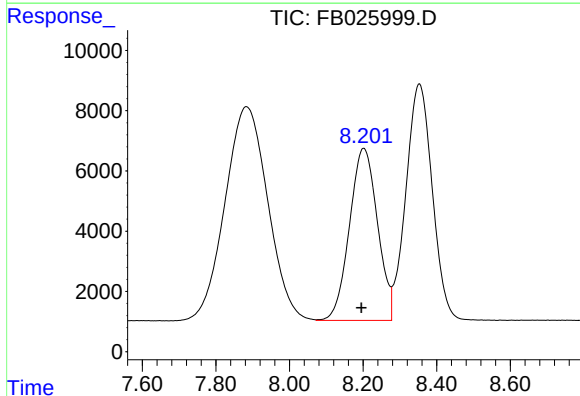


#3 n-Heptane

R.T.: 8.202 min
Delta R.T.: 0.006 min
Response: 301500
Conc: 8.39 ng/ml

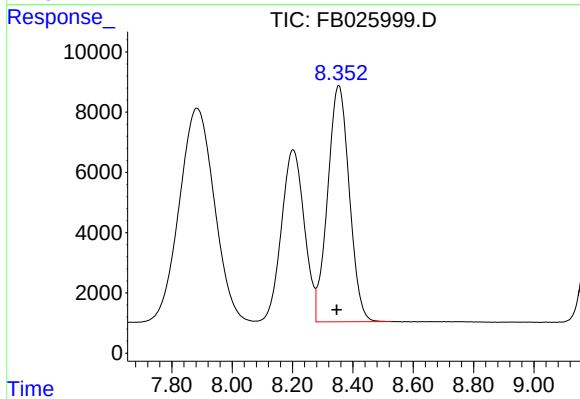


#4 Benzene

R.T.: 8.354 min
Delta R.T.: 0.007 min
Response: 390688
Conc: 9.36 ng/ml

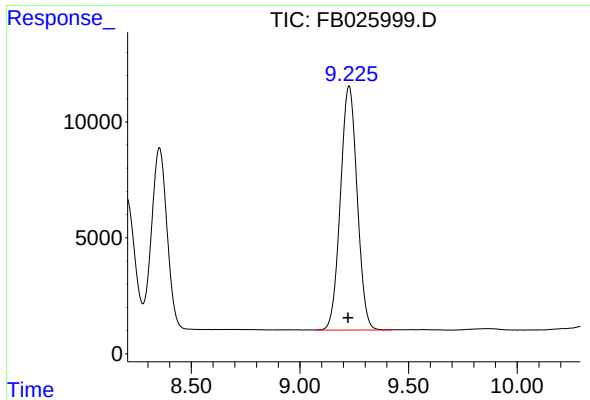


#5 AAA-TFT

R.T.: 9.226 min
Delta R.T.: 0.005 min
Response: 563735
Conc: 23.33 ng/ml

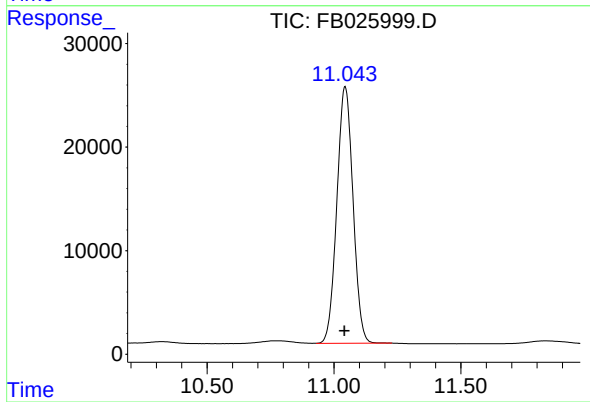


#6 Toluene

R.T.: 11.044 min
Delta R.T.: 0.003 min
Response: 1096523
Conc: 26.65 ng/ml

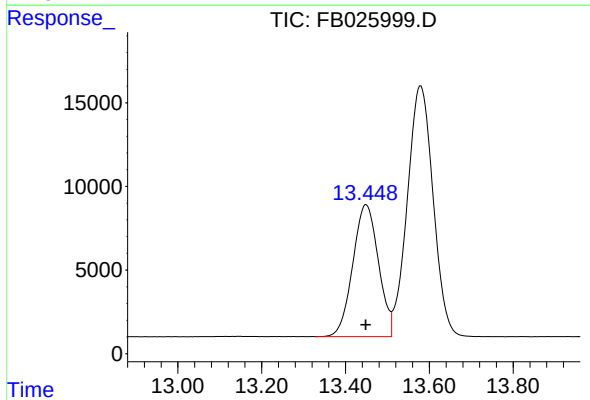


#7 Ethylbenzene

R.T.: 13.449 min
Delta R.T.: 0.001 min
Response: 334586
Conc: 8.78 ng/ml

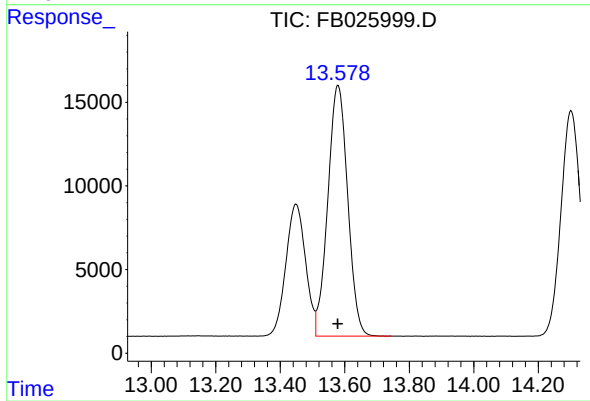

#8 m-Xylene

R.T.: 13.580 min
Delta R.T.: 0.000 min
Response: 641780
Conc: 16.33 ng/ml

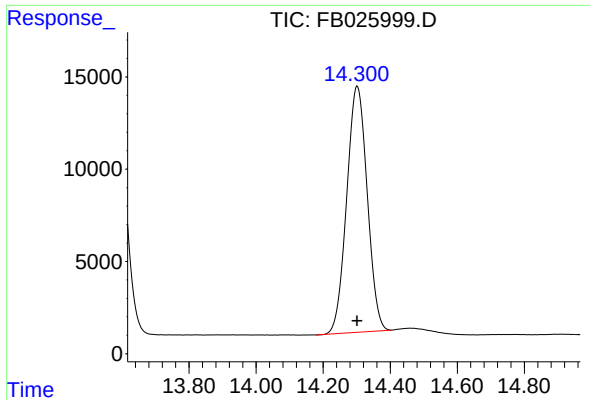


#9 O-Xylene

R.T.: 14.302 min

Delta R.T.: 0.000 min

Response: 565051

Conc: 17.72 ng/ml

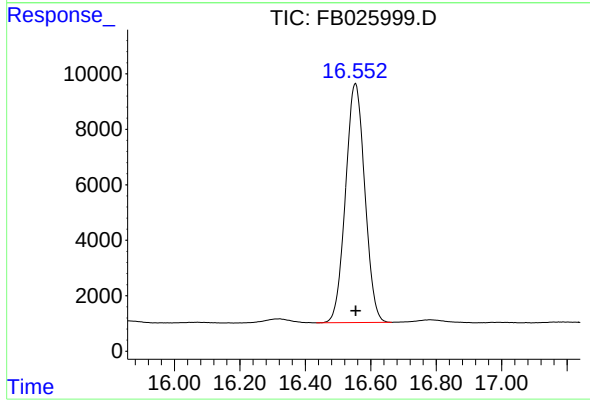

#10 1,2,4-Trimethylbenzene

R.T.: 16.553 min

Delta R.T.: 0.000 min

Response: 352250

Conc: 17.90 ng/ml