

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070825\
 Data File : FB032016.D
 Signal(s) : FID2B.CH
 Acq On : 8 Jul 2025 15:04
 Operator : YP/AJ
 Sample : BSF0708S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0708S1

Integration File: SAMPLE.e
 Quant Time: Jul 09 05:40:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
 Quant Title :
 QLast Update : Mon Jun 23 13:56:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	281695	18.259 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.718	608515	23.919 ng/ml
2) t 2,2,4-Trimethylpentane	7.433	757222	28.079 ng/ml
3) t n-Heptane	7.761	227086	9.101 ng/ml
4) t Benzene	7.900	312074	9.179 ng/ml
6) t Toluene	10.630	927861	25.948 ng/ml
7) t Ethylbenzene	13.066	271812	8.608 ng/ml
8) t m-Xylene	13.199	571045	17.410 ng/ml
9) t O-Xylene	13.926	545522	17.576 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	463981	17.548 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070825\
Data File : FB032016.D
Signal(s) : FID2B.CH
Acq On : 8 Jul 2025 15:04
Operator : YP/AJ
Sample : BSF0708S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0708S1

Integration File: SAMPLE.e
Quant Time: Jul 09 05:40:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

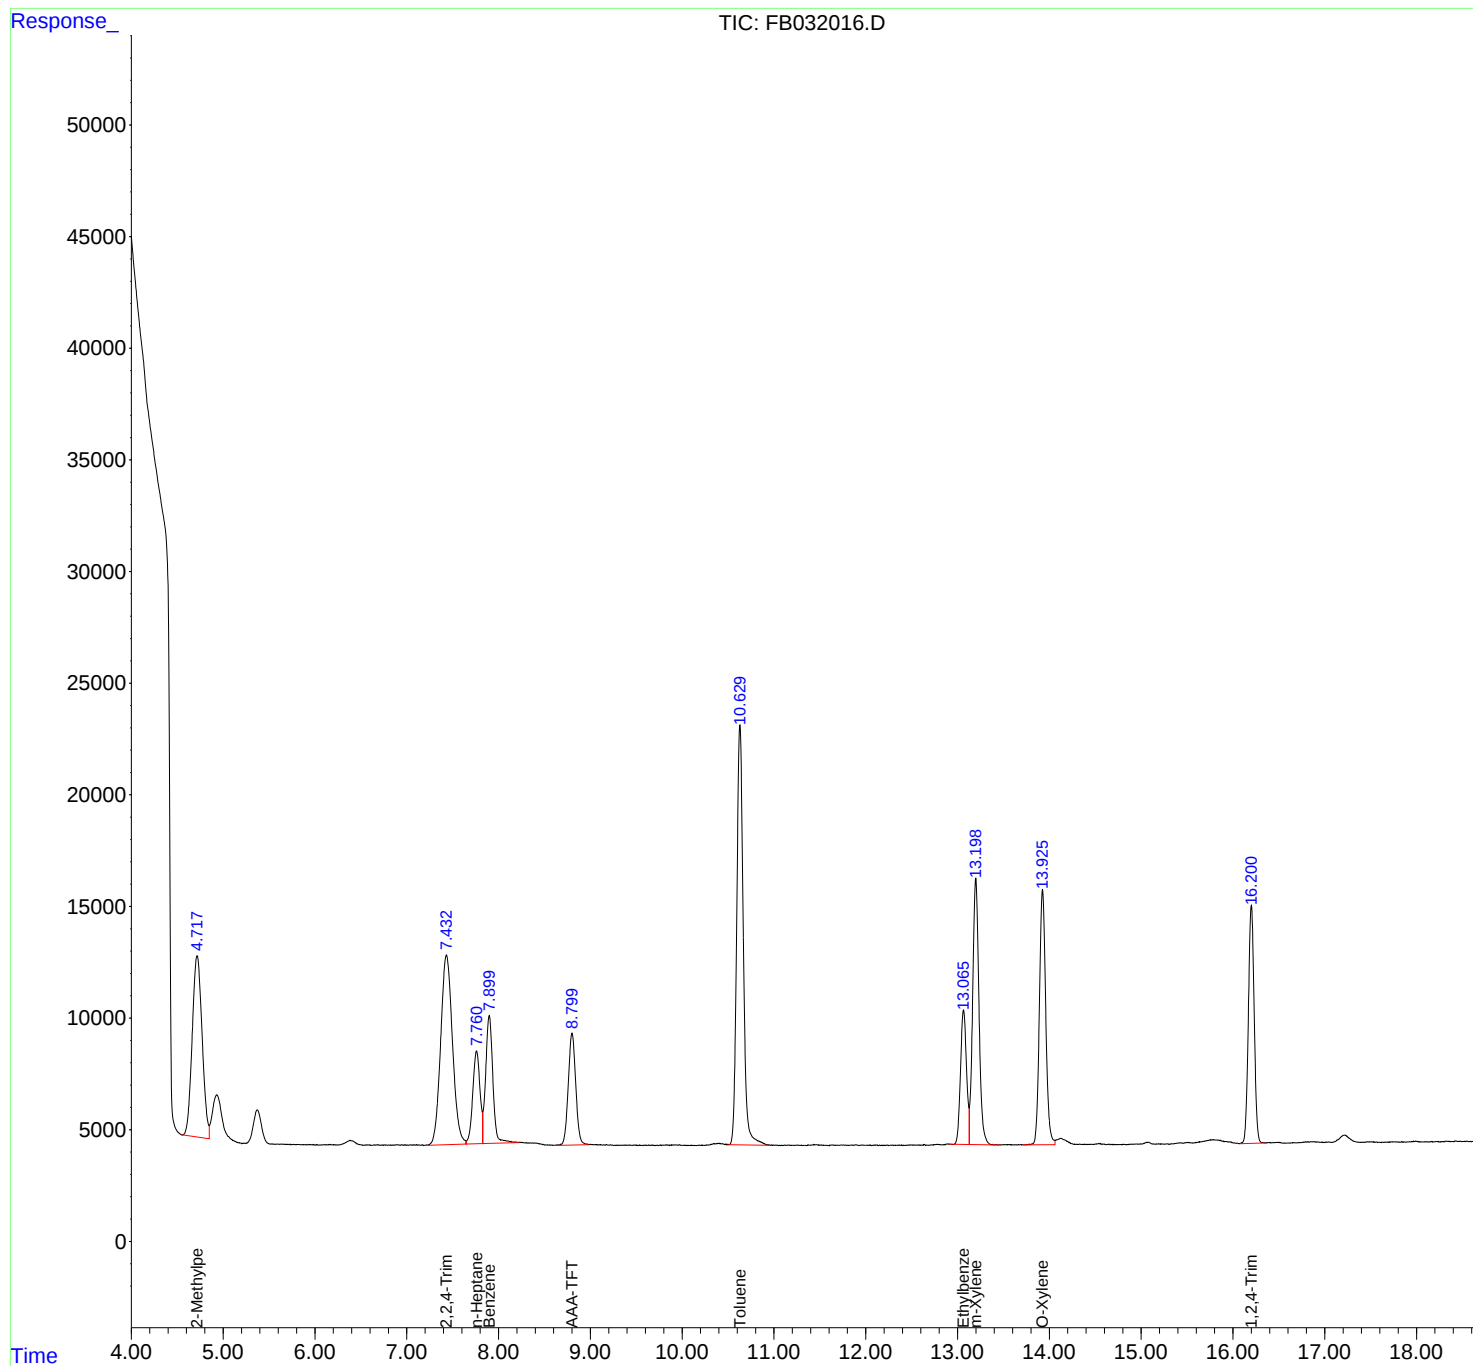


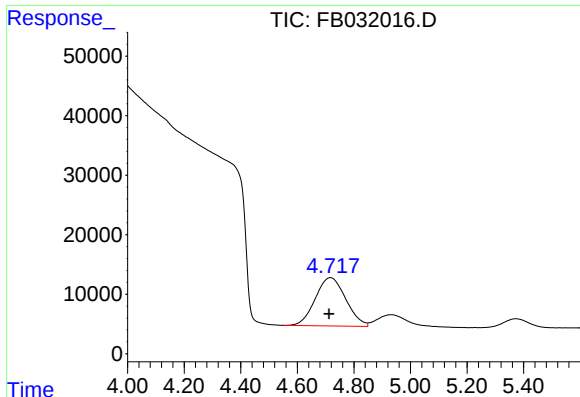

#1 2-Methylpentane


R.T.: 4.718 min
Delta R.T.: 0.005 min
Response: 608515
Conc: 23.92 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0708S1

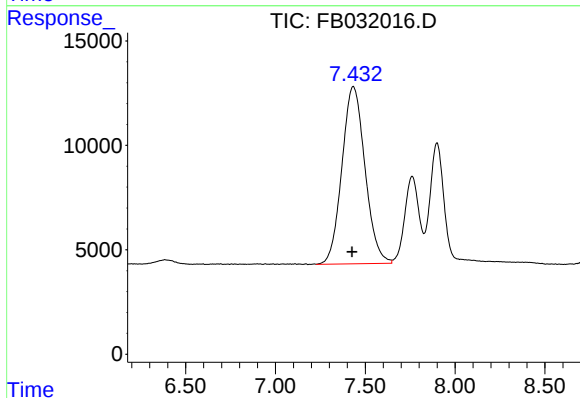


#2 2,2,4-Trimethylpentane

R.T.: 7.433 min
Delta R.T.: 0.007 min
Response: 757222
Conc: 28.08 ng/ml

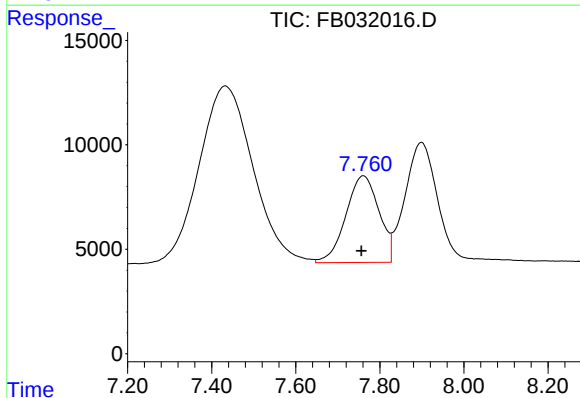


#3 n-Heptane

R.T.: 7.761 min
Delta R.T.: 0.005 min
Response: 227086
Conc: 9.10 ng/ml

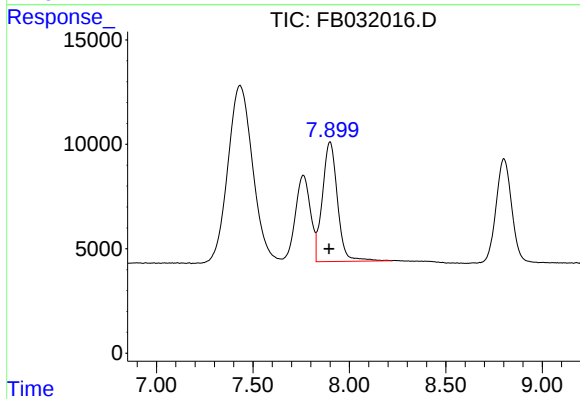

#4 Benzene


R.T.: 7.900 min
Delta R.T.: 0.004 min
Response: 312074
Conc: 9.18 ng/ml

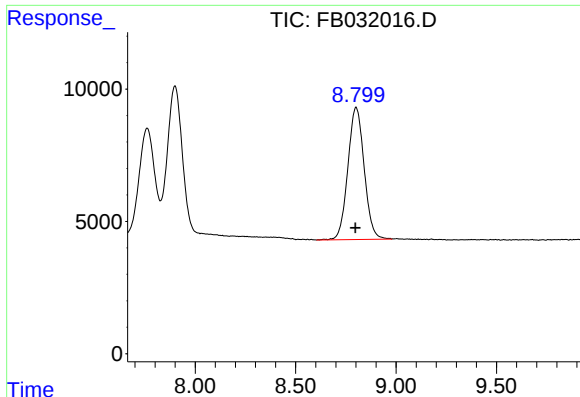

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.003 min
Response: 281695
Conc: 18.26 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0708S1

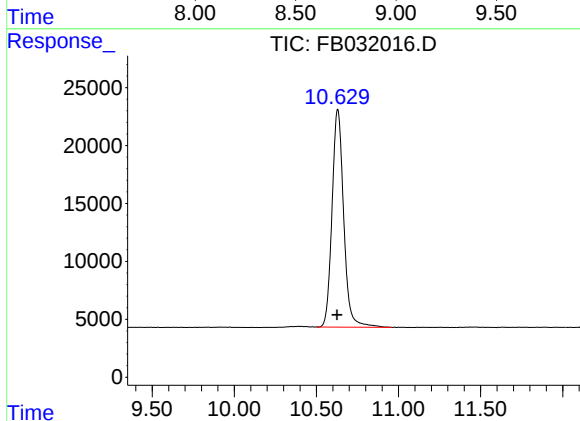


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.004 min
Response: 927861
Conc: 25.95 ng/ml

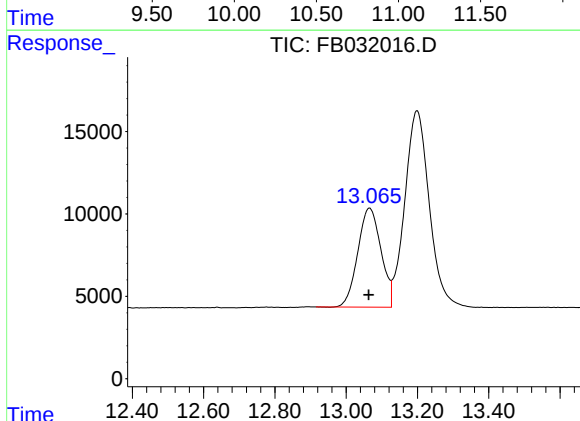


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: 0.003 min
Response: 271812
Conc: 8.61 ng/ml

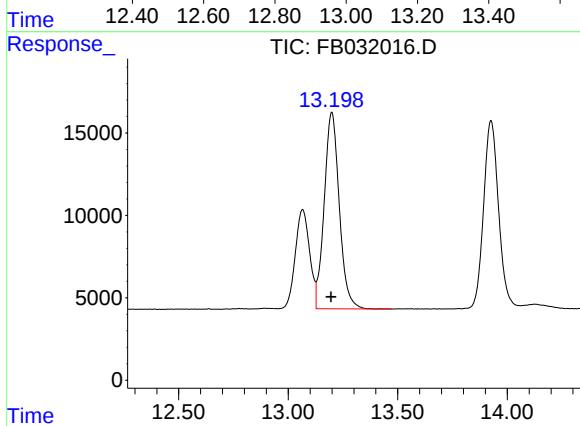

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: 0.004 min
Response: 571045
Conc: 17.41 ng/ml

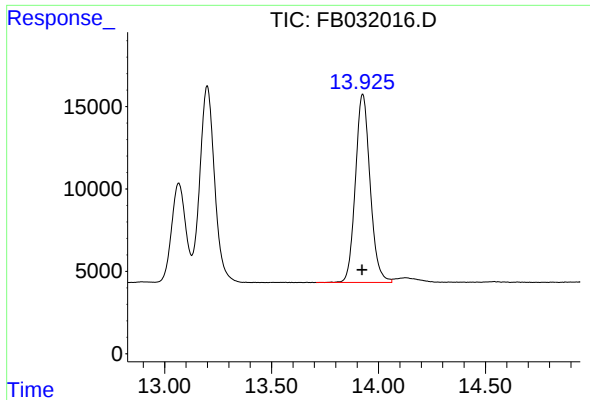

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: 0.004 min
Response: 545522
Conc: 17.58 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0708S1

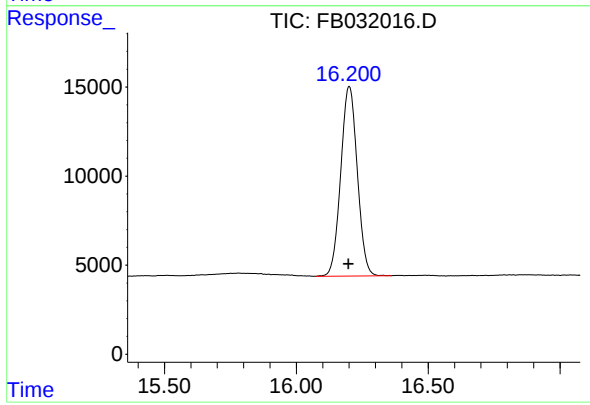

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: 0.003 min
Response: 463981
Conc: 17.55 ng/ml