

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070825\
 Data File : FB032023.D
 Signal(s) : FID2B.CH
 Acq On : 8 Jul 2025 18:33
 Operator : YP/AJ
 Sample : BSF0708S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0708S2

Integration File: SAMPLE.e
 Quant Time: Jul 09 05:41:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
 Quant Title :
 QLast Update : Mon Jun 23 13:56:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	309207	20.042 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	599935	23.582 ng/ml
2) t 2,2,4-Trimethylpentane	7.433	781040	28.962 ng/ml
3) t n-Heptane	7.762	226081	9.061 ng/ml
4) t Benzene	7.900	314131	9.239 ng/ml
6) t Toluene	10.631	951366	26.606 ng/ml
7) t Ethylbenzene	13.067	280177	8.873 ng/ml
8) t m-Xylene	13.200	586023	17.867 ng/ml
9) t O-Xylene	13.927	561099	18.078 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	472240	17.860 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070825\
Data File : FB032023.D
Signal(s) : FID2B.CH
Acq On : 8 Jul 2025 18:33
Operator : YP/AJ
Sample : BSF0708S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0708S2

Integration File: SAMPLE.e
Quant Time: Jul 09 05:41:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

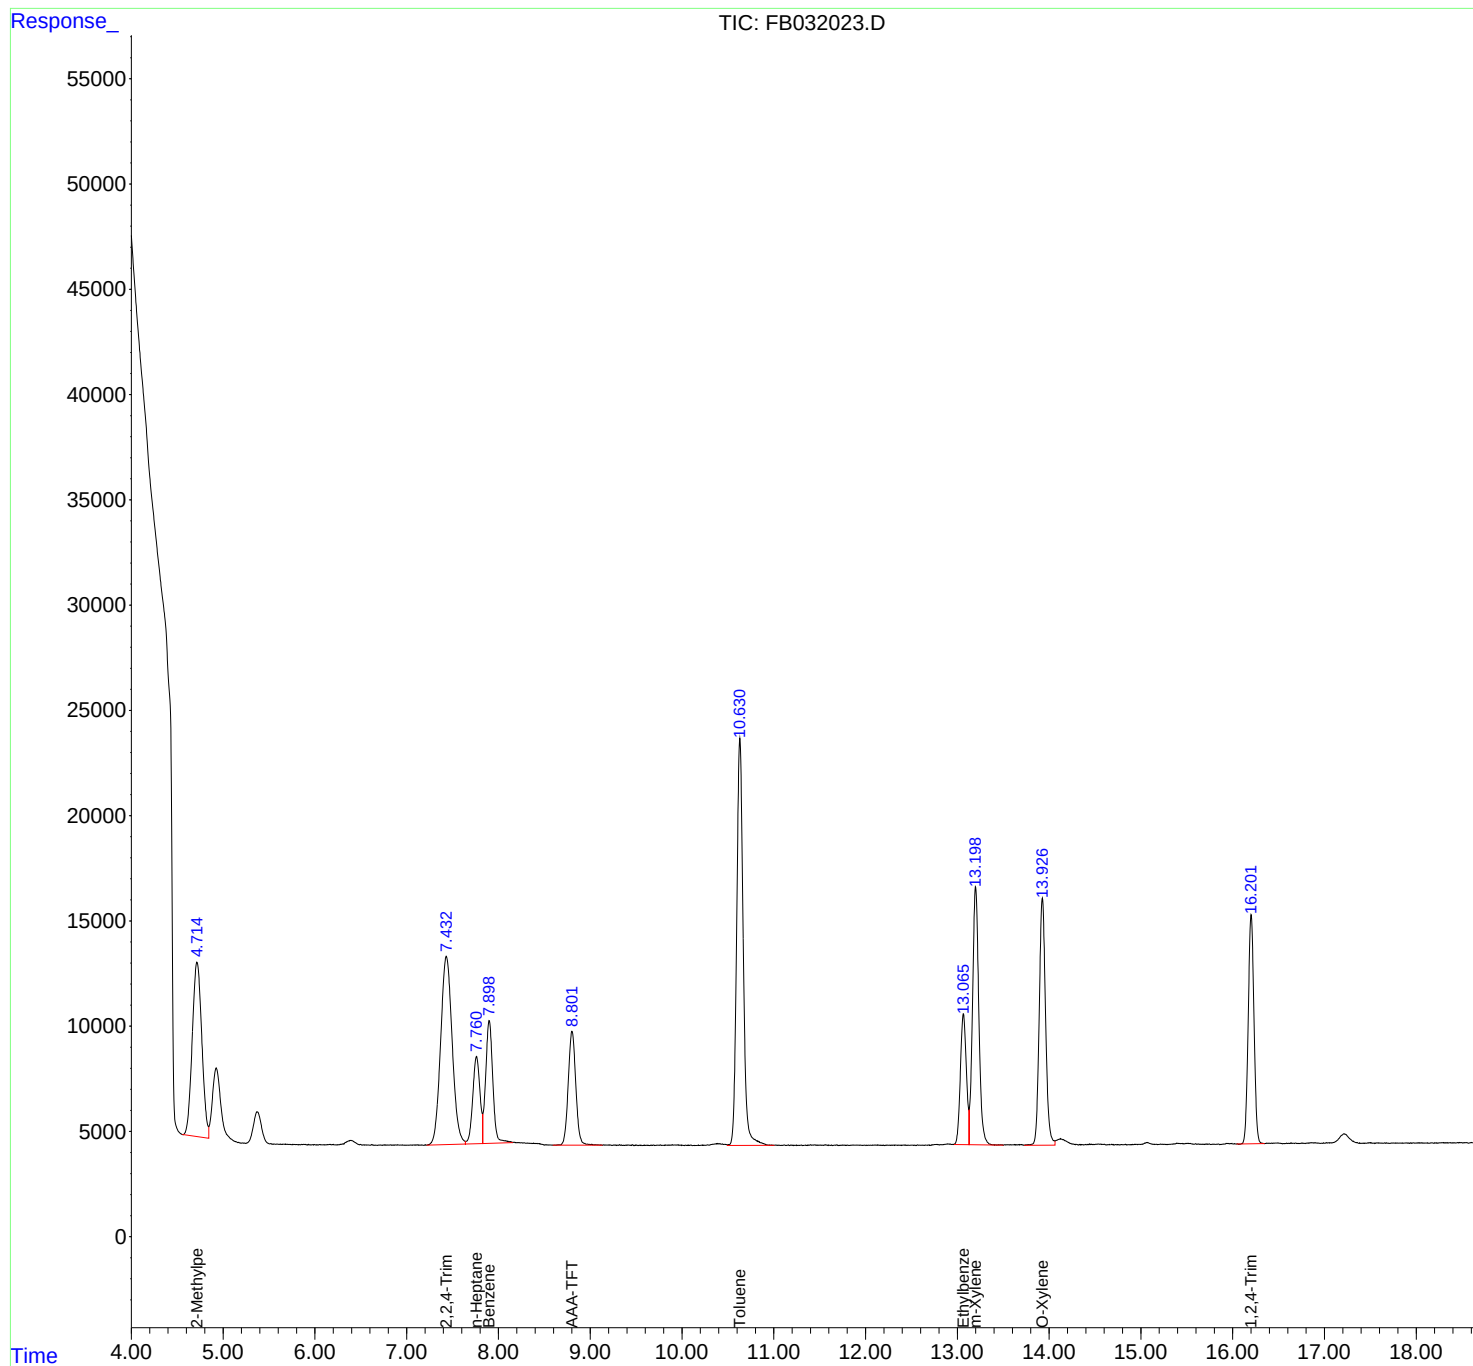


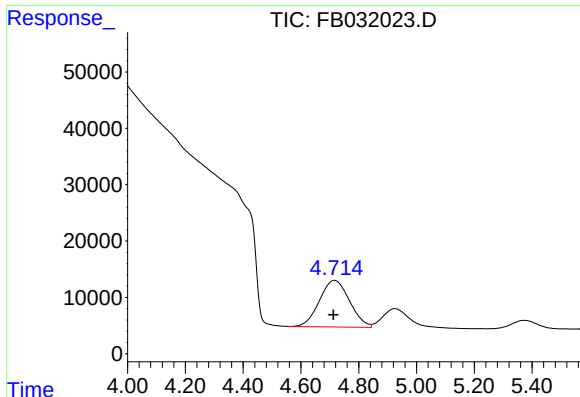

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: 0.003 min
Response: 599935
Conc: 23.58 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0708S2

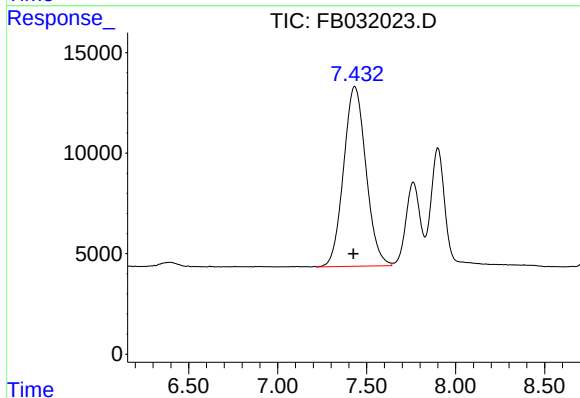


#2 2,2,4-Trimethylpentane

R.T.: 7.433 min
Delta R.T.: 0.007 min
Response: 781040
Conc: 28.96 ng/ml

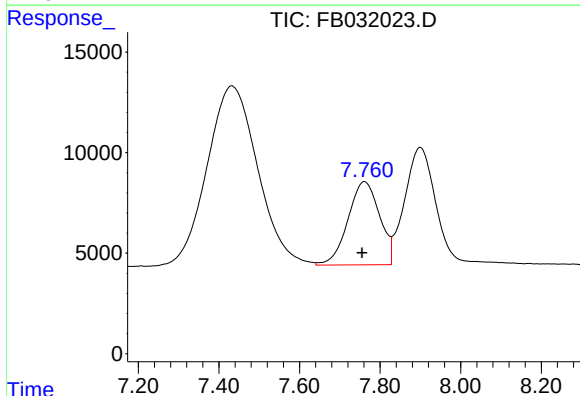


#3 n-Heptane

R.T.: 7.762 min
Delta R.T.: 0.006 min
Response: 226081
Conc: 9.06 ng/ml

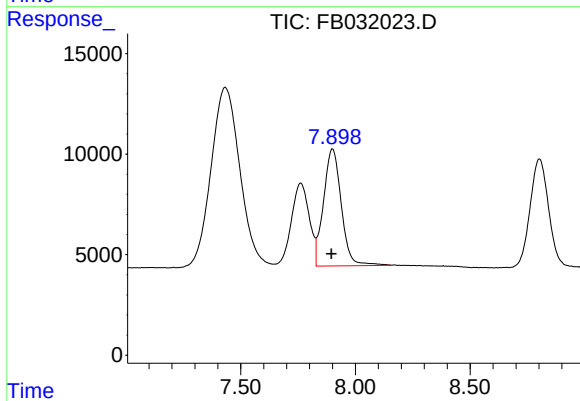

#4 Benzene


R.T.: 7.900 min
Delta R.T.: 0.005 min
Response: 314131
Conc: 9.24 ng/ml

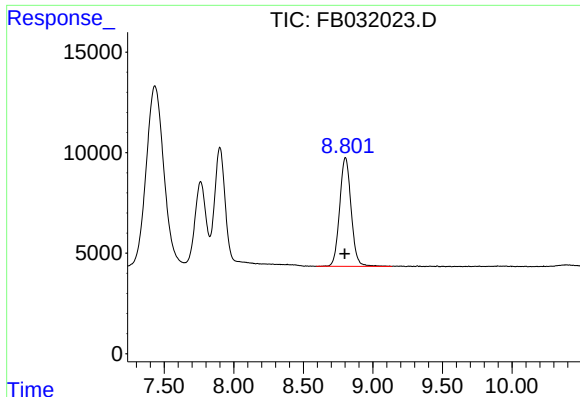

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.005 min
Response: 309207
Conc: 20.04 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0708S2

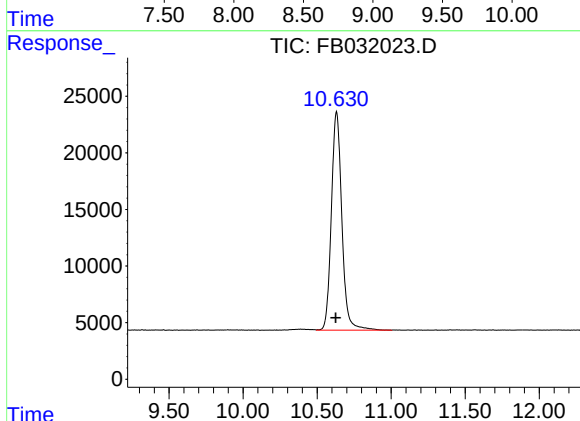


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.005 min
Response: 951366
Conc: 26.61 ng/ml

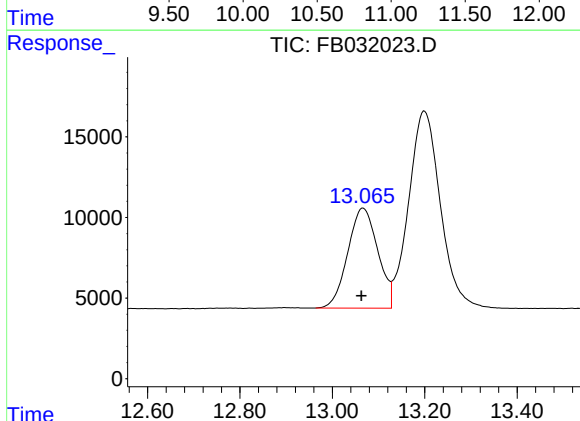


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: 0.004 min
Response: 280177
Conc: 8.87 ng/ml

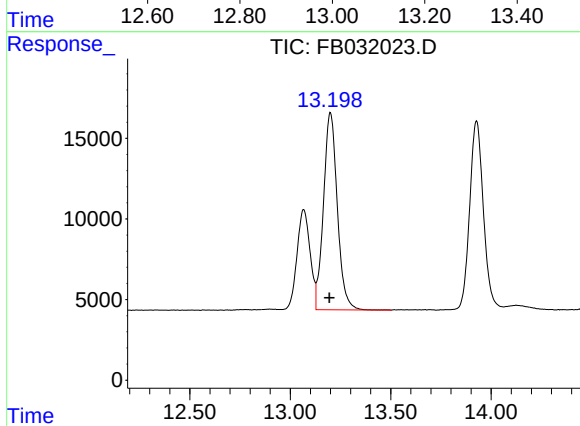

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: 0.004 min
Response: 586023
Conc: 17.87 ng/ml

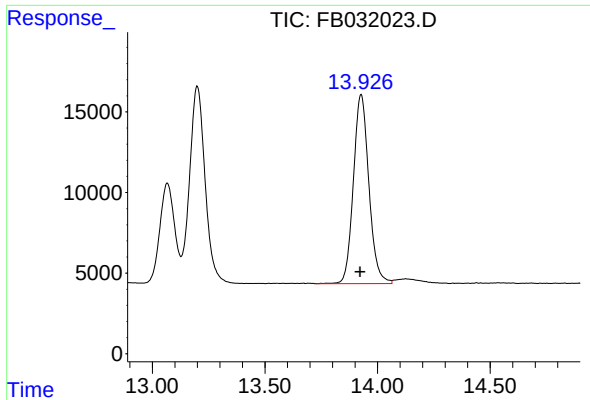

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: 0.004 min
Response: 561099
Conc: 18.08 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0708S2

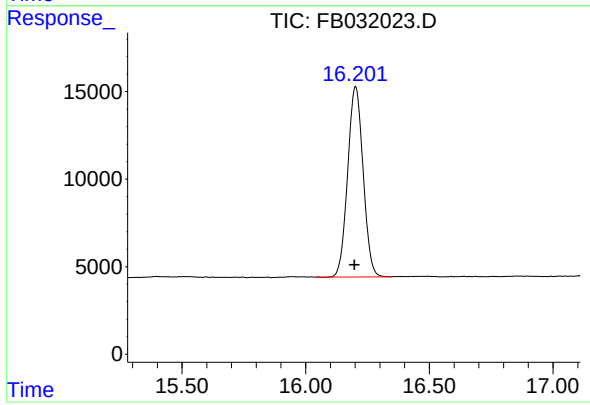

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: 0.004 min
Response: 472240
Conc: 17.86 ng/ml