

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070918\
 Data File : FB016625.D
 Signal(s) : FID2B.CH
 Acq On : 9 Jul 2018 16:52
 Operator : MJ/SJ
 Sample : BSF0709S1
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0709S1

Integration File: Calibration.e
 Quant Time: Jul 10 17:22:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070918.M
 Quant Title :
 QLast Update : Mon Jul 09 13:06:15 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.117	181005	20.761 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.968	412001	28.360 ng/ml
2) t 2,2,4-Trimethylpentane	7.732	437047	31.422 ng/ml
3) t n-Heptane	8.072	135734	10.017 ng/ml
4) t Benzene	8.211	190558	10.269 ng/ml
6) t Toluene	10.965	441439	30.229 ng/ml
7) t Ethylbenzene	13.415	136193	9.273 ng/ml
8) t m-Xylene	13.548	283219	18.182 ng/ml
9) t O-Xylene	14.280	295534	17.855 ng/ml
10) t 1,2,4-Trimethylbenzene	16.562	365429	18.685 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070918\
Data File : FB016625.D
Signal(s) : FID2B.CH
Acq On : 9 Jul 2018 16:52
Operator : MJ/SJ
Sample : BSF0709S1
Misc : 5.00g/5.00mL DI Water
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0709S1

Integration File: Calibration.e
Quant Time: Jul 10 17:22:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070918.M
Quant Title :
QLast Update : Mon Jul 09 13:06:15 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

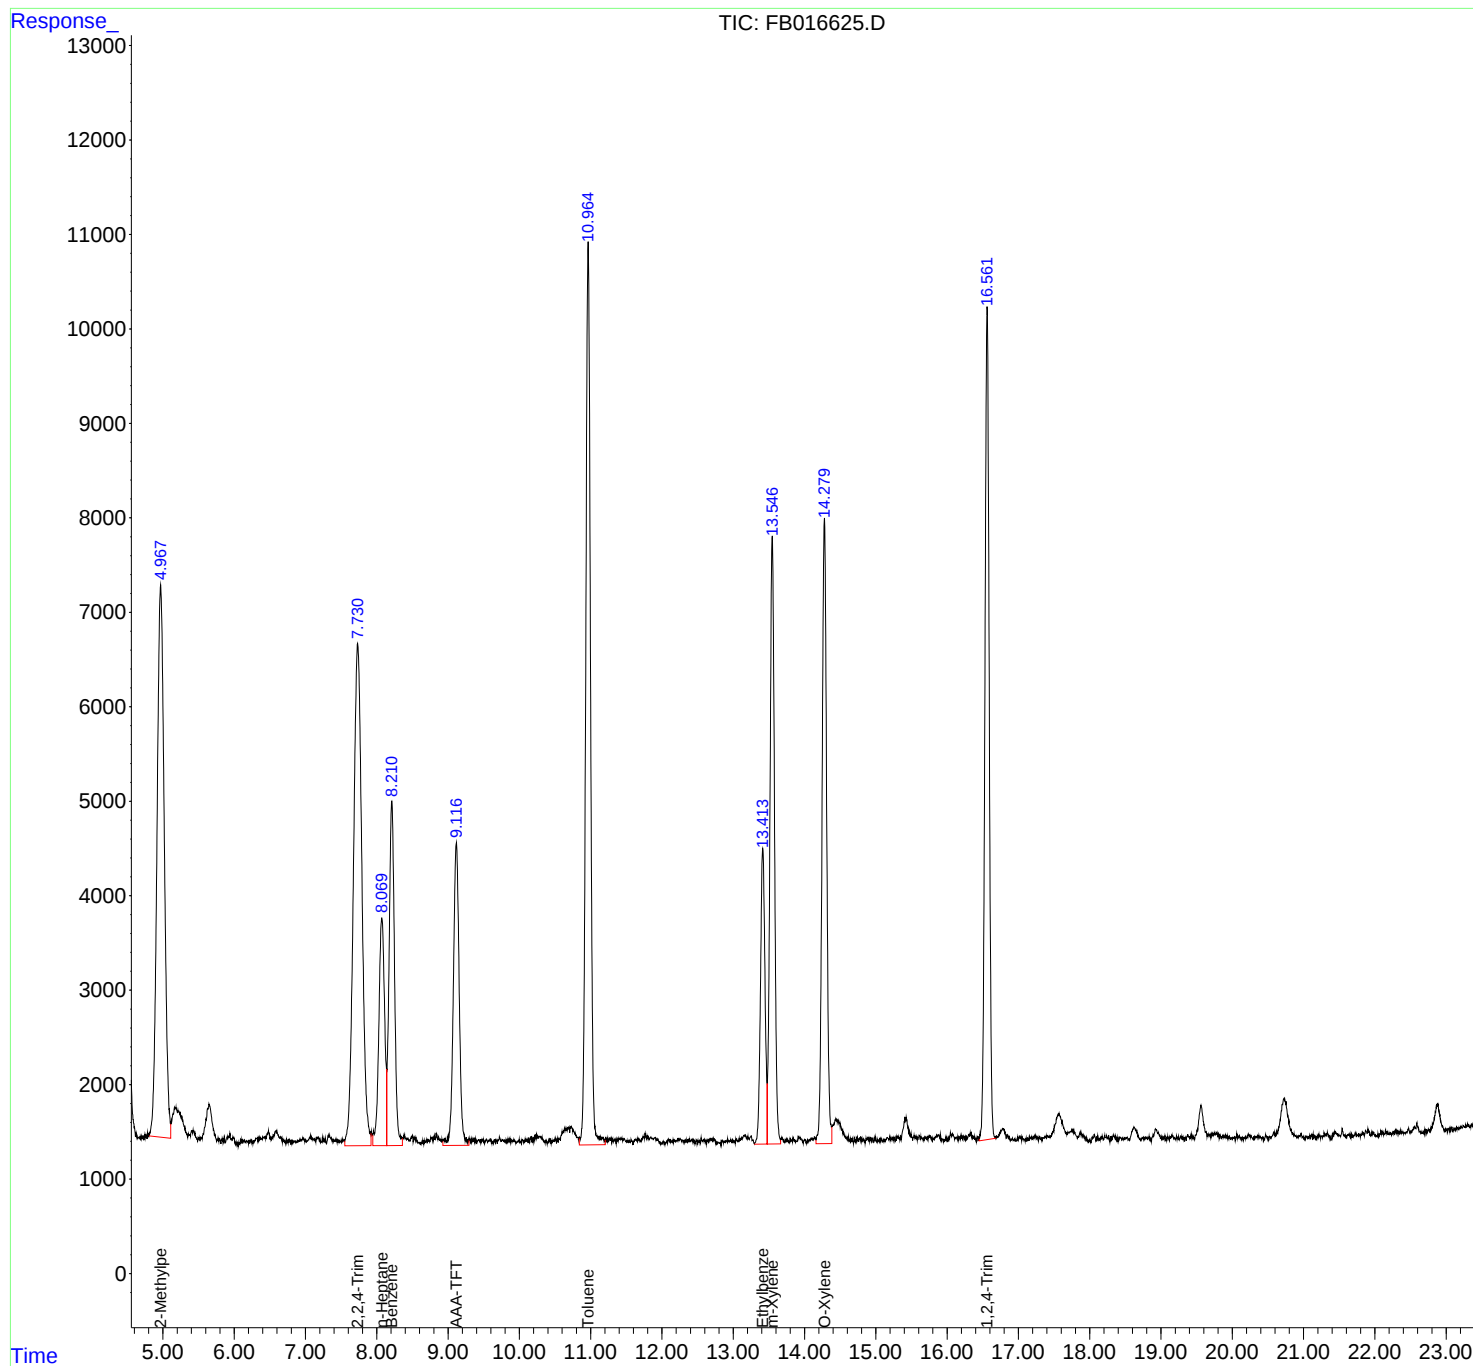


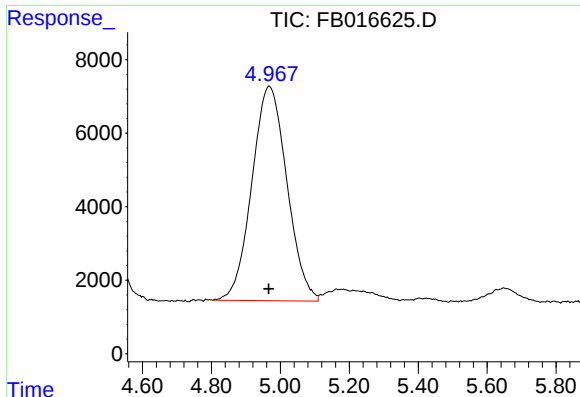

#1 2-Methylpentane


R.T.: 4.968 min
Delta R.T.: 0.002 min
Response: 412001
Conc: 28.36 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0709S1

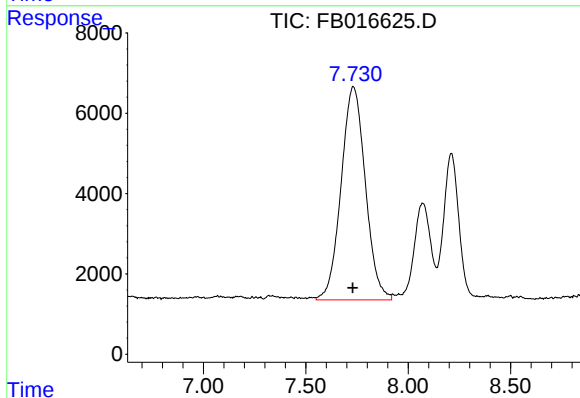


#2 2,2,4-Trimethylpentane

R.T.: 7.732 min
Delta R.T.: 0.003 min
Response: 437047
Conc: 31.42 ng/ml

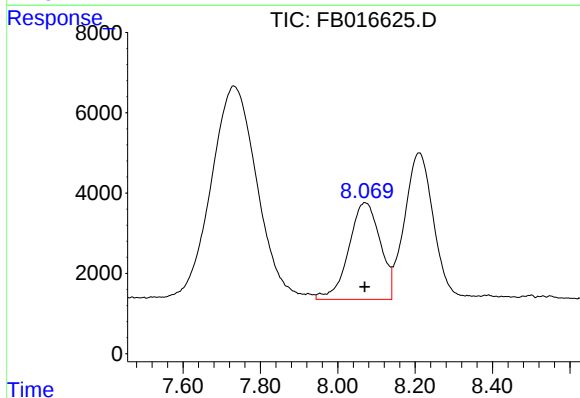


#3 n-Heptane

R.T.: 8.072 min
Delta R.T.: 0.002 min
Response: 135734
Conc: 10.02 ng/ml

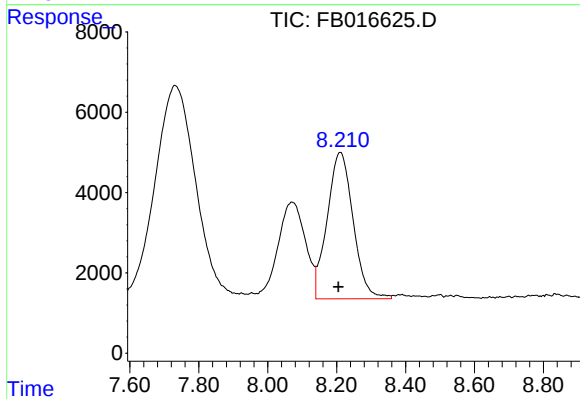

#4 Benzene


R.T.: 8.211 min
Delta R.T.: 0.005 min
Response: 190558
Conc: 10.27 ng/ml

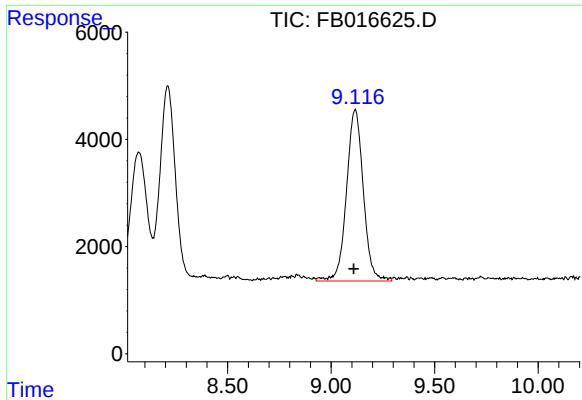

#5 AAA-TFT


R.T.: 9.117 min
Delta R.T.: 0.006 min
Response: 181005
Conc: 20.76 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0709S1

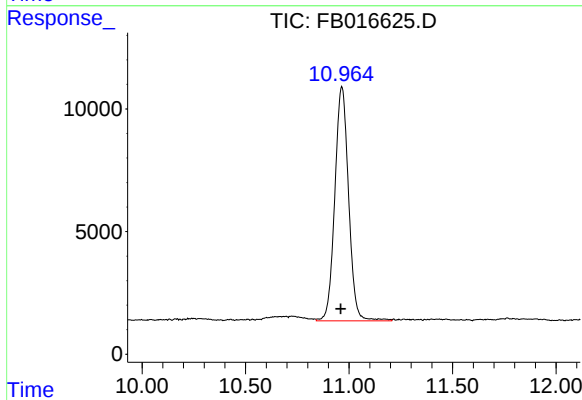


#6 Toluene

R.T.: 10.965 min
Delta R.T.: 0.006 min
Response: 441439
Conc: 30.23 ng/ml

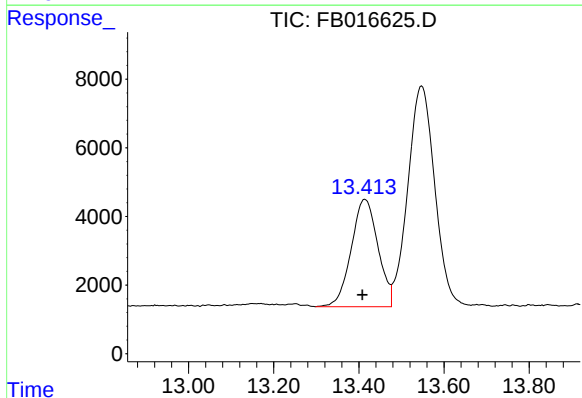


#7 Ethylbenzene

R.T.: 13.415 min
Delta R.T.: 0.006 min
Response: 136193
Conc: 9.27 ng/ml

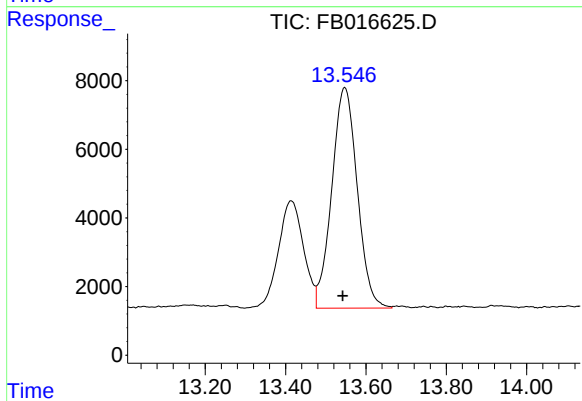

#8 m-Xylene


R.T.: 13.548 min
Delta R.T.: 0.006 min
Response: 283219
Conc: 18.18 ng/ml

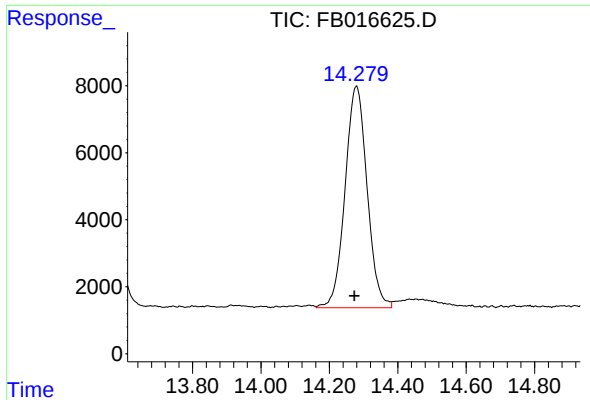

#9 O-Xylene

R.T.: 14.280 min
Delta R.T.: 0.006 min
Response: 295534
Conc: 17.85 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0709S1

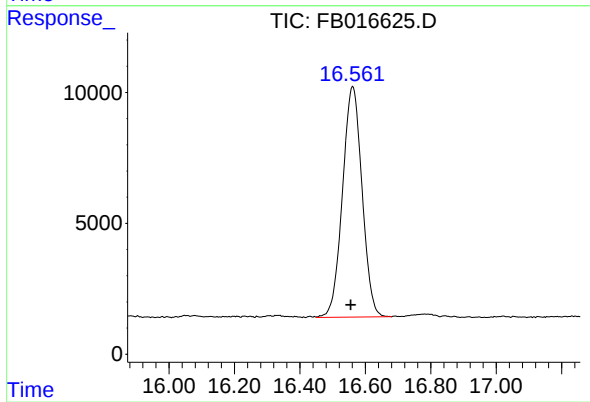

#10 1,2,4-Trimethylbenzene

R.T.: 16.562 min
Delta R.T.: 0.006 min
Response: 365429
Conc: 18.69 ng/ml