

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070920\
 Data File : FB024563.D
 Signal(s) : FID2B.CH
 Acq On : 9 Jul 2020 14:22
 Operator : DD/AJ
 Sample : L3186-02MS
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OR-02-070820MS

Integration File: Calibration.e
 Quant Time: Jul 09 15:39:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
 Quant Title :
 QLast Update : Thu Jul 09 10:49:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	420860	18.270 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	804234	27.176 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	828562	26.466 ng/ml
3) t n-Heptane	7.759	271510	8.732 ng/ml
4) t Benzene	7.893	353592	9.276 ng/ml
6) t Toluene	10.631	1011214	27.656 ng/ml
7) t Ethylbenzene	13.071	357966	10.480 ng/ml
8) t m-Xylene	13.204	615812	18.248 ng/ml
9) t O-Xylene	13.932	640708	19.494 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	505970	18.757 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070920\
Data File : FB024563.D
Signal(s) : FID2B.CH
Acq On : 9 Jul 2020 14:22
Operator : DD/AJ
Sample : L3186-02MS
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OR-02-070820MS

Integration File: Calibration.e
Quant Time: Jul 09 15:39:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

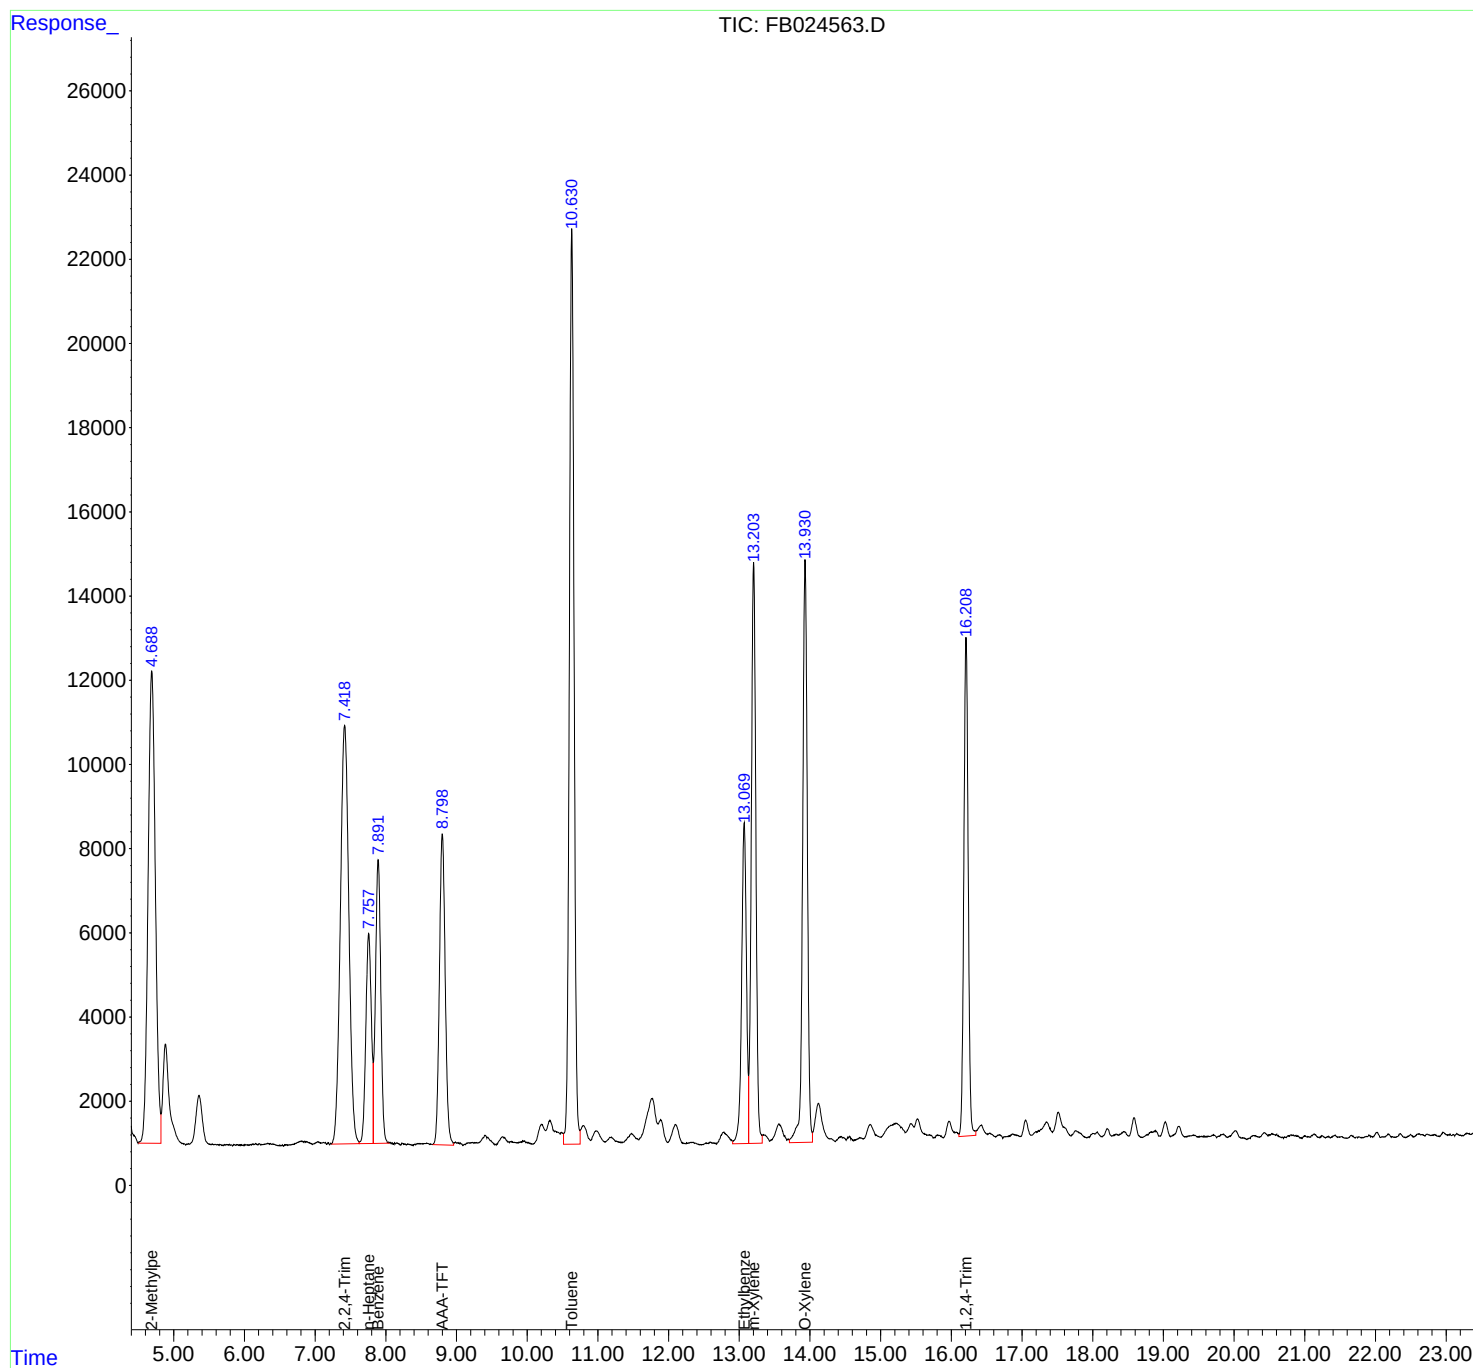


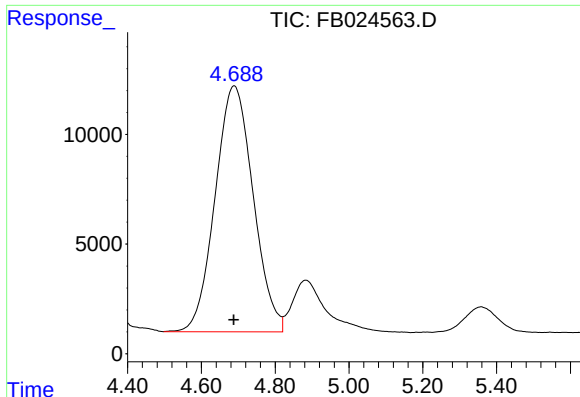

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: 0.002 min
Response: 804234
Conc: 27.18 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-070820MS

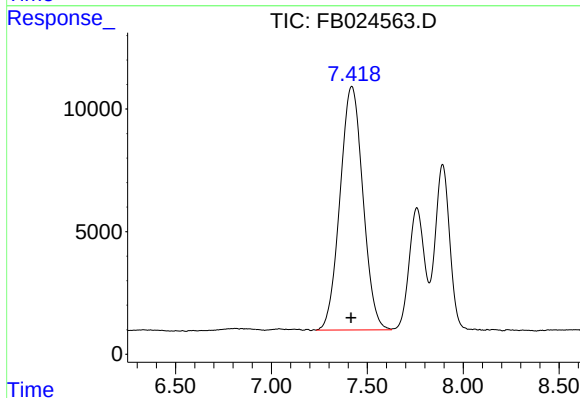


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.003 min
Response: 828562
Conc: 26.47 ng/ml

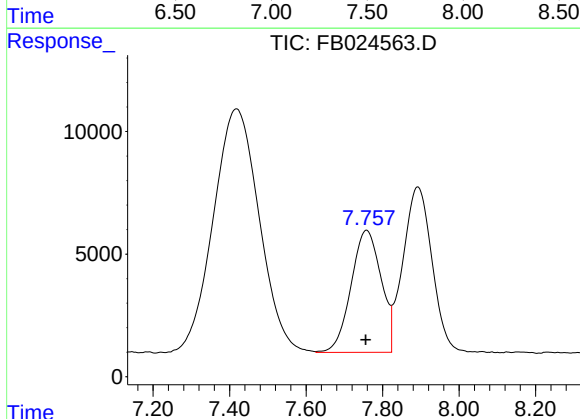


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.003 min
Response: 271510
Conc: 8.73 ng/ml

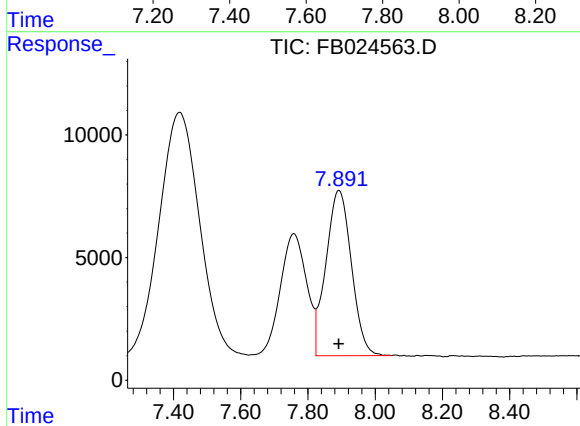

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 353592
Conc: 9.28 ng/ml

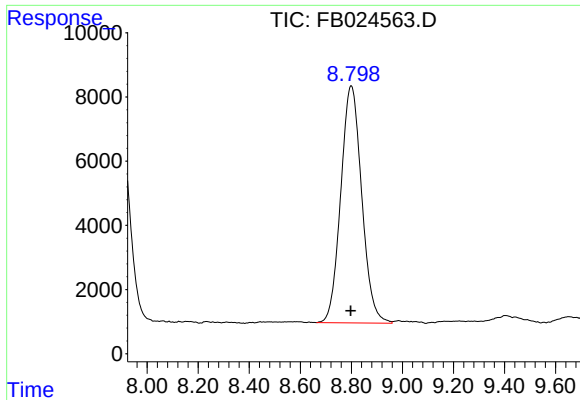

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.002 min
Response: 420860
Conc: 18.27 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-070820MS

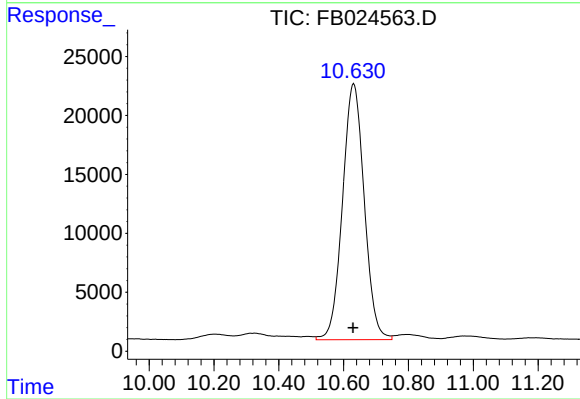


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.002 min
Response: 1011214
Conc: 27.66 ng/ml

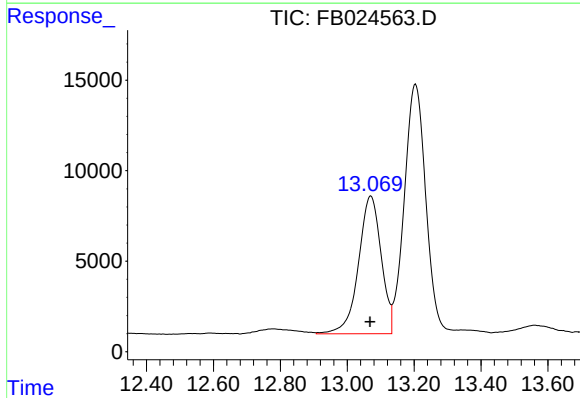


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.002 min
Response: 357966
Conc: 10.48 ng/ml

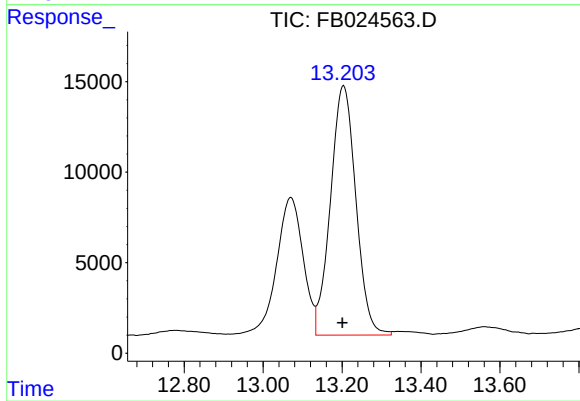

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.003 min
Response: 615812
Conc: 18.25 ng/ml

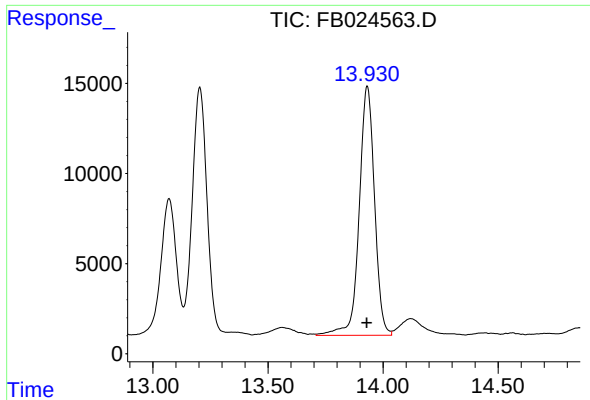

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.003 min
Response: 640708
Conc: 19.49 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-070820MS

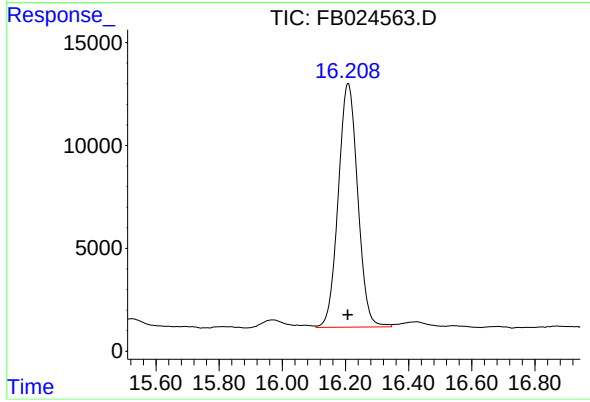

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.002 min
Response: 505970
Conc: 18.76 ng/ml