

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070920\
 Data File : FB024564.D
 Signal(s) : FID2B.CH
 Acq On : 9 Jul 2020 14:53
 Operator : DD/AJ
 Sample : L3186-02MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OR-02-070820MSD

Integration File: Calibration.e
 Quant Time: Jul 09 15:39:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
 Quant Title :
 QLast Update : Thu Jul 09 10:49:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	436779	18.961 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	718004	24.263 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	681448	21.767 ng/ml
3) t n-Heptane	7.760	226414	7.282 ng/ml
4) t Benzene	7.893	338271	8.874 ng/ml
6) t Toluene	10.632	966395	26.430 ng/ml
7) t Ethylbenzene	13.070	398901	11.679 ng/ml
8) t m-Xylene	13.204	583298	17.285 ng/ml
9) t O-Xylene	13.932	655356	19.940 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	457154	16.948 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070920\
Data File : FB024564.D
Signal(s) : FID2B.CH
Acq On : 9 Jul 2020 14:53
Operator : DD/AJ
Sample : L3186-02MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OR-02-070820MSD

Integration File: Calibration.e
Quant Time: Jul 09 15:39:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

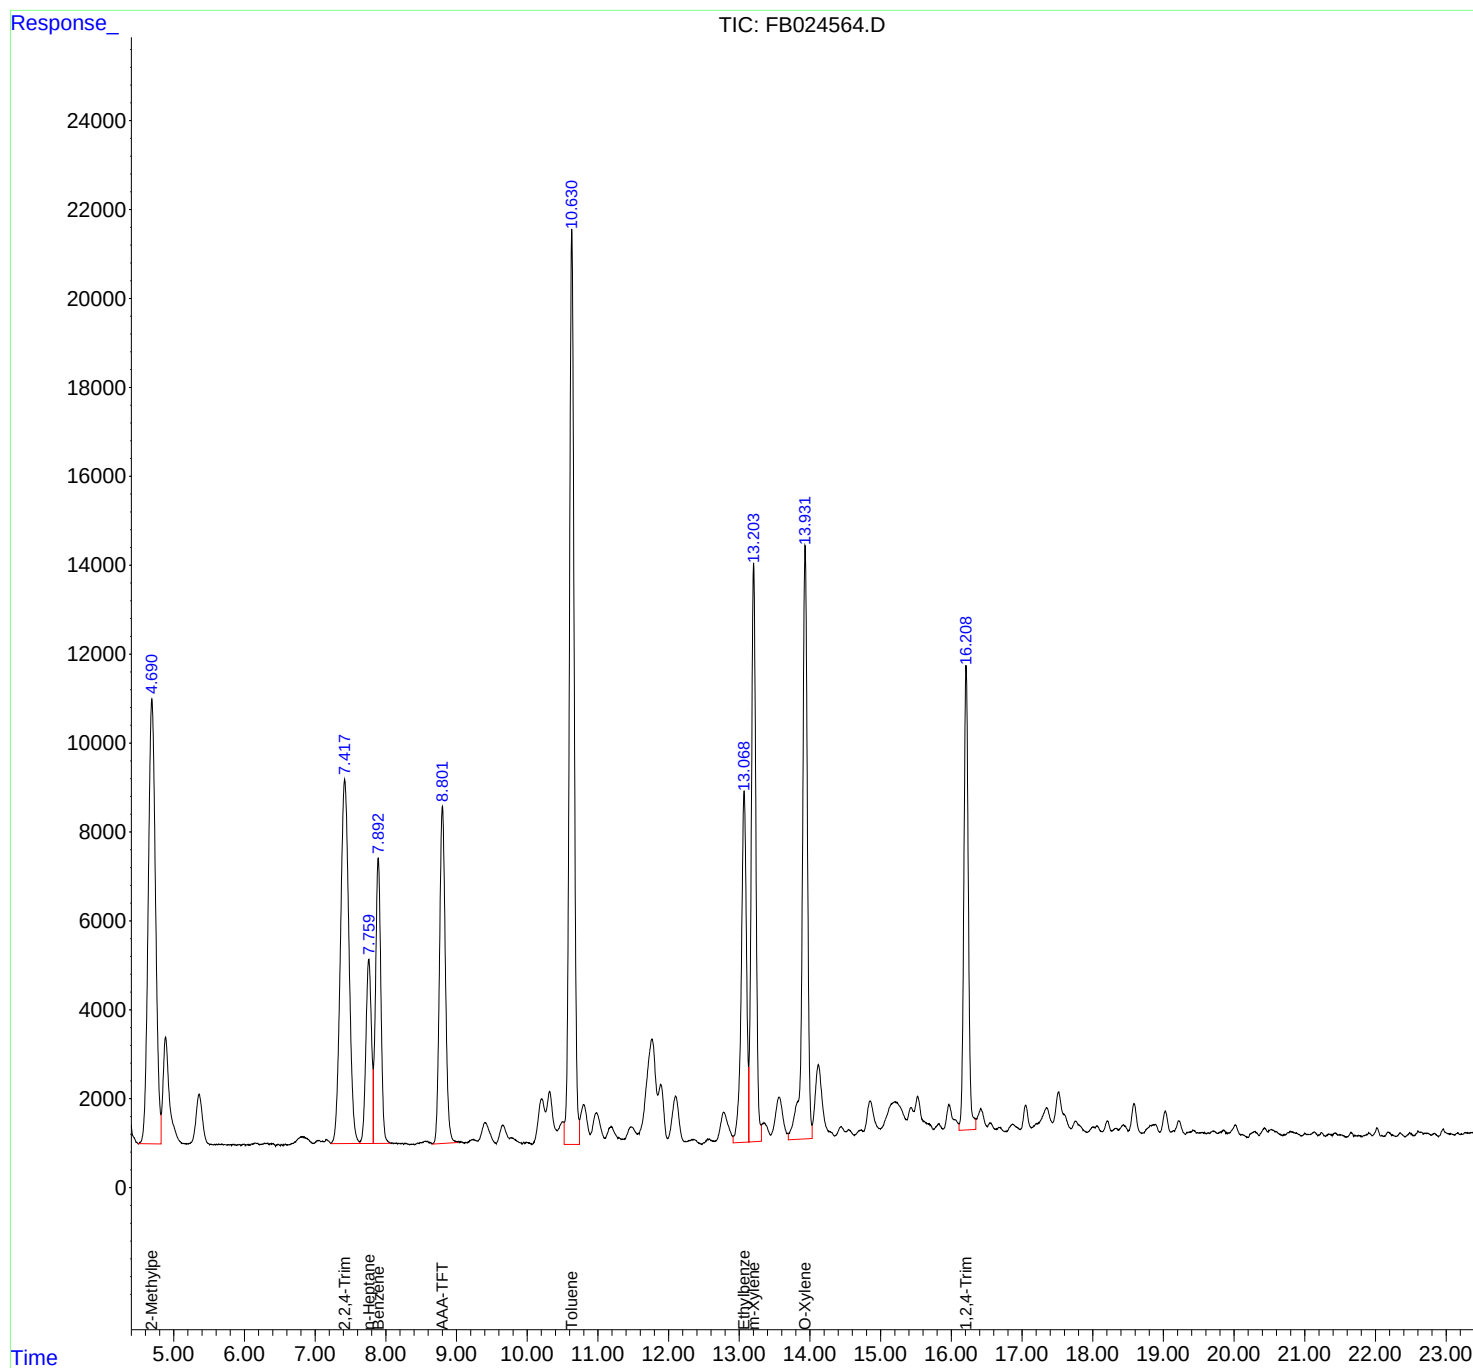


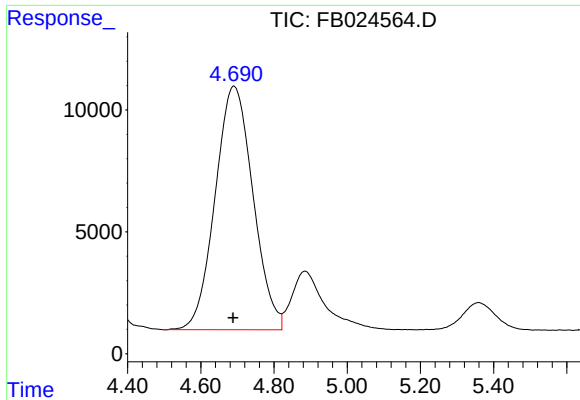

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.003 min
Response: 718004
Conc: 24.26 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-070820MSD

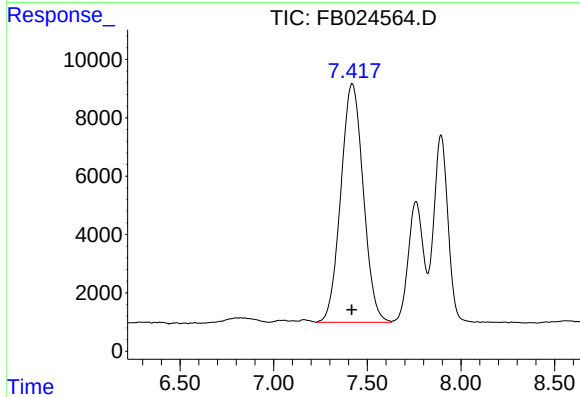


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.002 min
Response: 681448
Conc: 21.77 ng/ml

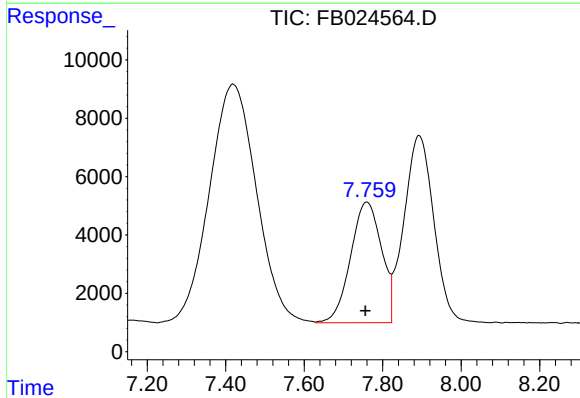


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.004 min
Response: 226414
Conc: 7.28 ng/ml

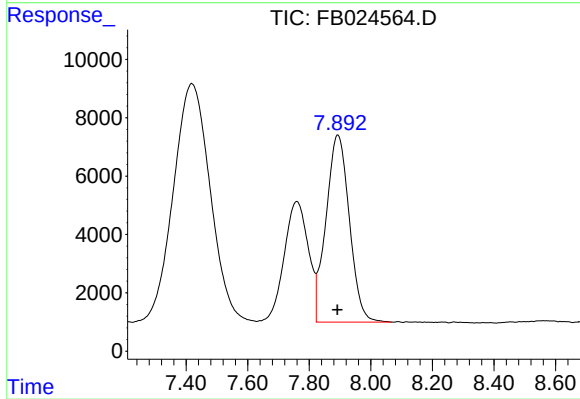

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.001 min
Response: 338271
Conc: 8.87 ng/ml

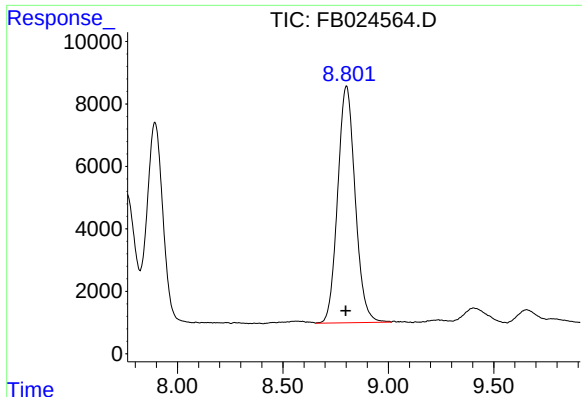

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.004 min
Response: 436779
Conc: 18.96 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-070820MSD

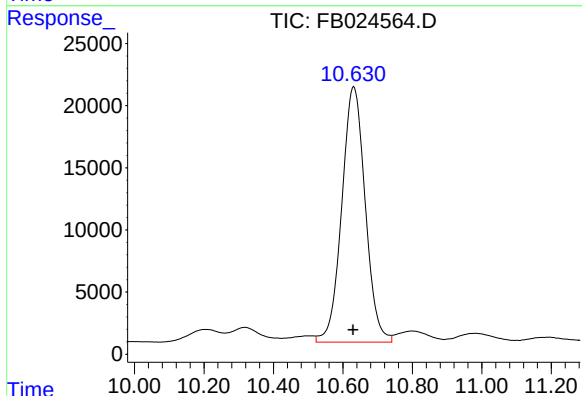


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.003 min
Response: 966395
Conc: 26.43 ng/ml

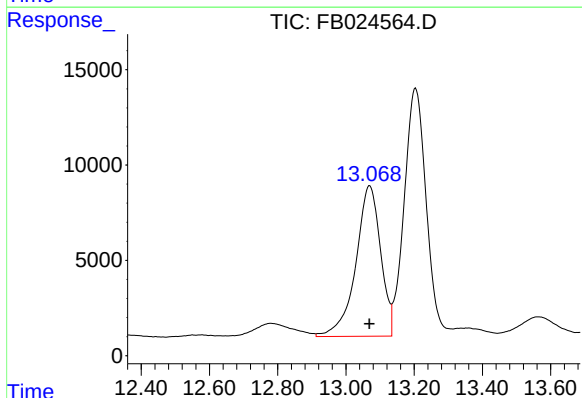


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 398901
Conc: 11.68 ng/ml

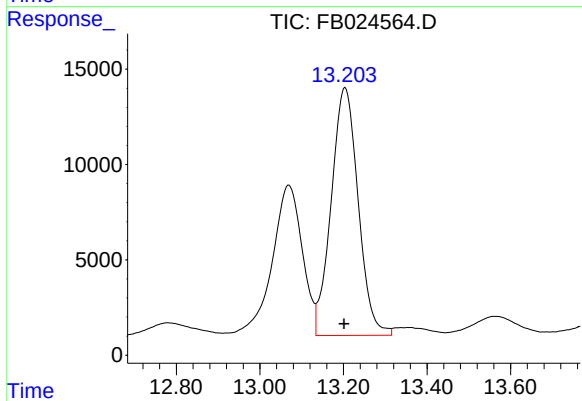

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.003 min
Response: 583298
Conc: 17.28 ng/ml

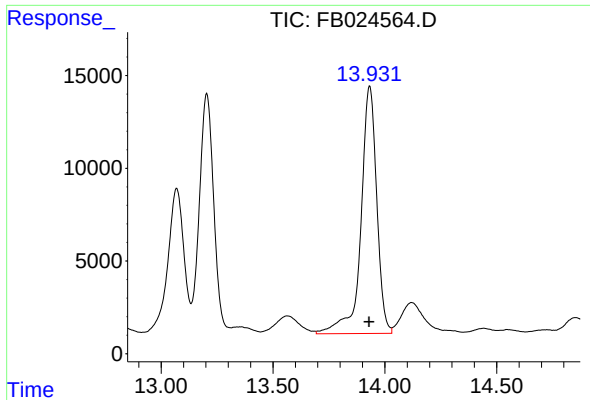

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.003 min
Response: 655356
Conc: 19.94 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-070820MSD

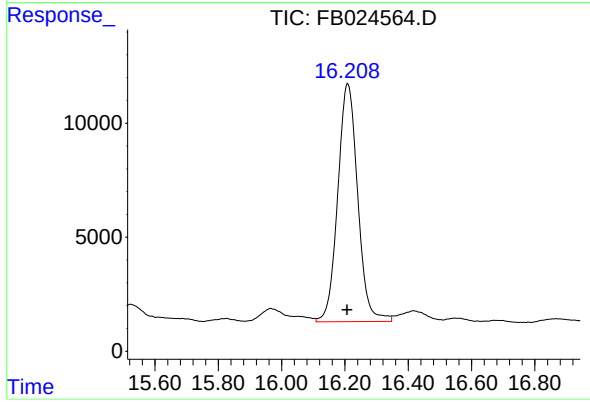

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.003 min
Response: 457154
Conc: 16.95 ng/ml