

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070920\
 Data File : FB024573.D
 Signal(s) : FID2B.CH
 Acq On : 9 Jul 2020 19:42
 Operator : DD/AJ
 Sample : L3216-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2020

Integration File: Calibration.e
 Quant Time: Jul 10 02:27:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
 Quant Title :
 QLast Update : Thu Jul 09 10:49:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	433089	18.801 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	187911	6.350 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	201426	6.434 ng/ml
3) t n-Heptane	7.757	65868	2.118 ng/ml
4) t Benzene	7.895	78962	2.072 ng/ml
6) t Toluene	10.634	233426	6.384 ng/ml
7) t Ethylbenzene	13.074	75539	2.212 ng/ml
8) t m-Xylene	13.206	150783	4.468 ng/ml
9) t O-Xylene	13.933	143742	4.373 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	114620	4.249 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070920\
Data File : FB024573.D
Signal(s) : FID2B.CH
Acq On : 9 Jul 2020 19:42
Operator : DD/AJ
Sample : L3216-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT3-2020

Integration File: Calibration.e
Quant Time: Jul 10 02:27:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

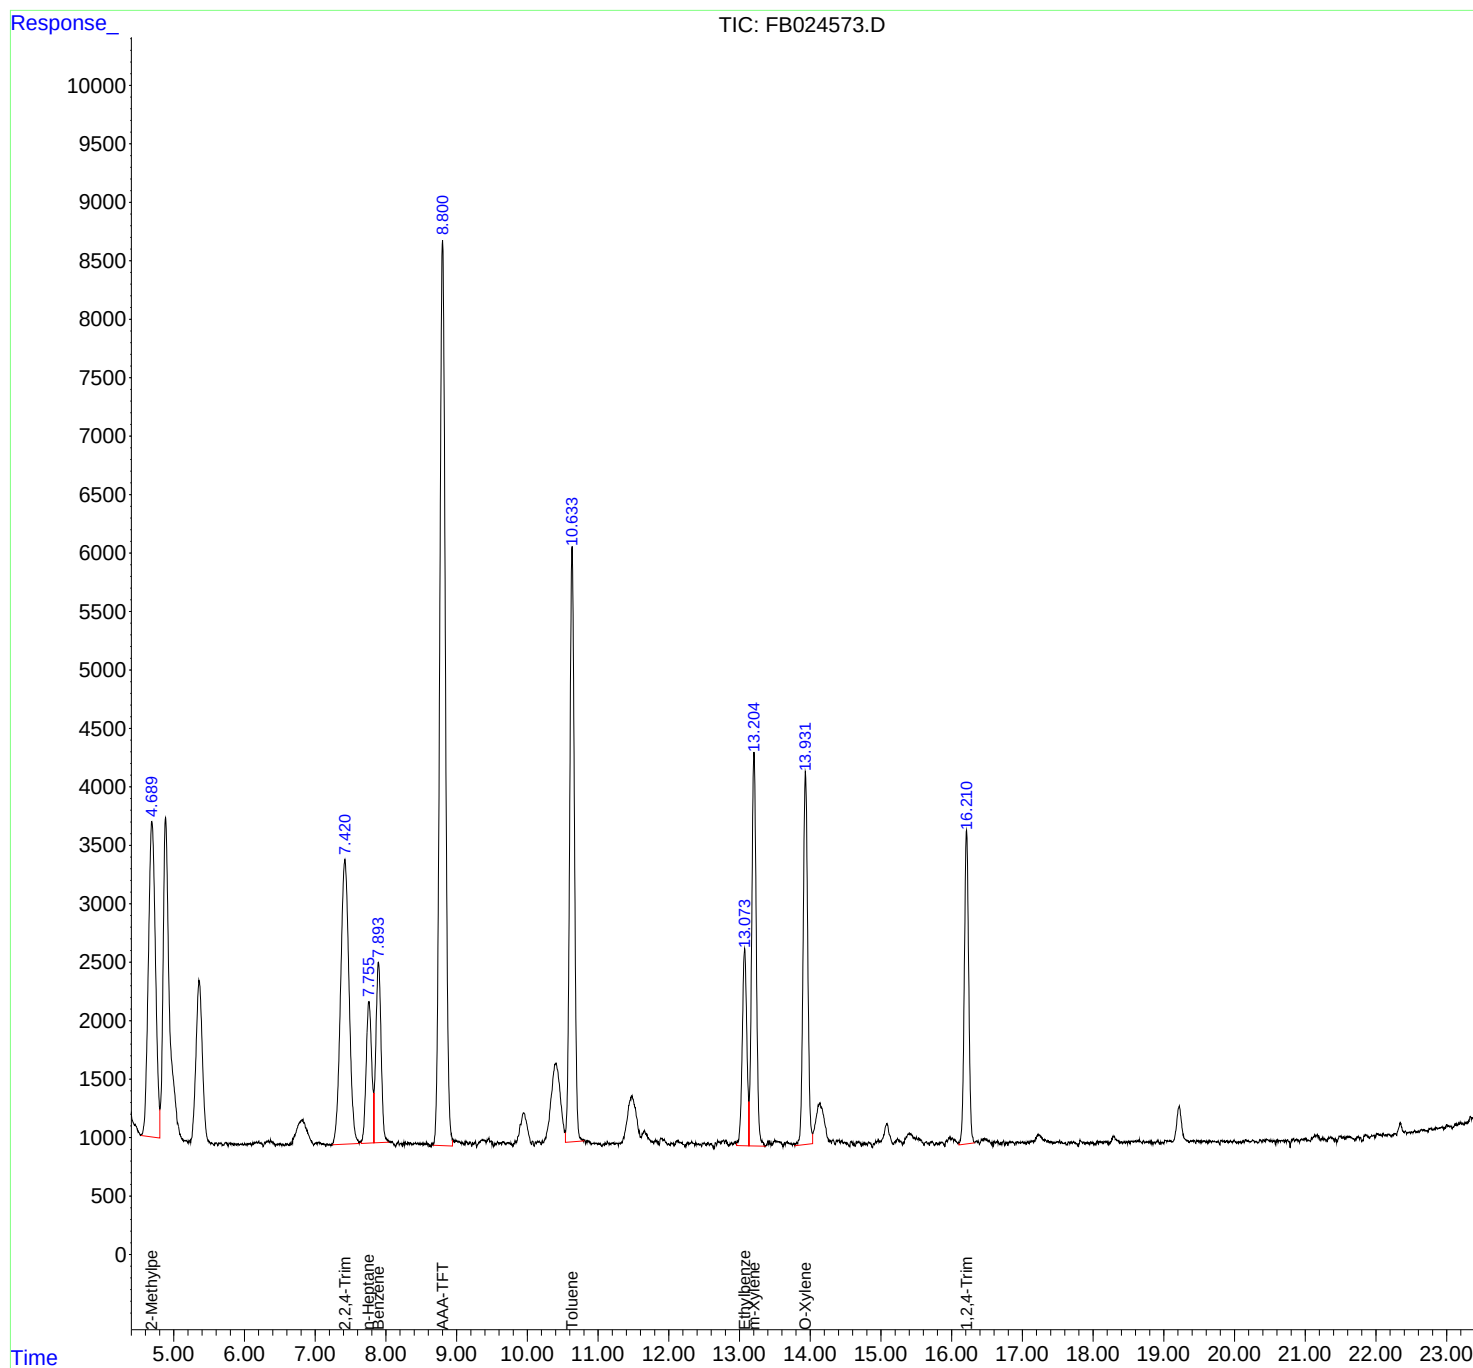


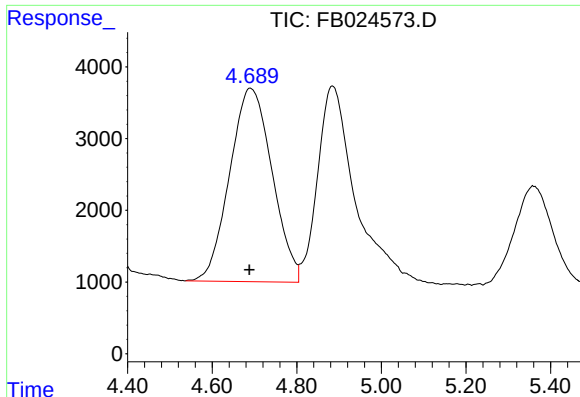

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: 0.002 min
Response: 187911
Conc: 6.35 ng/ml

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT3-2020

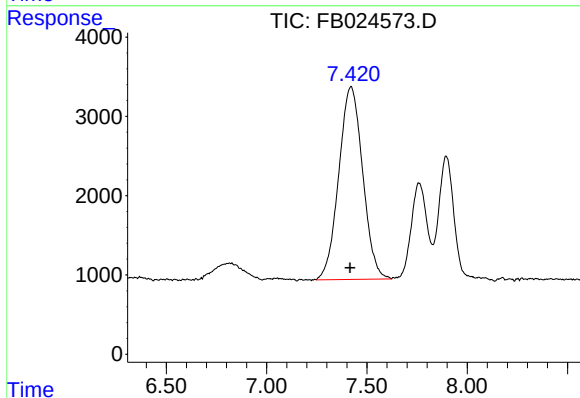


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.006 min
Response: 201426
Conc: 6.43 ng/ml

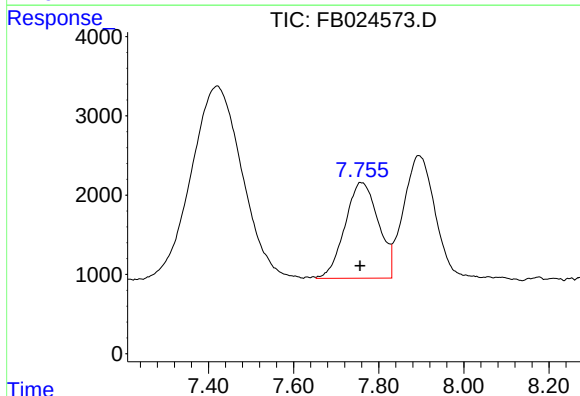


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.002 min
Response: 65868
Conc: 2.12 ng/ml

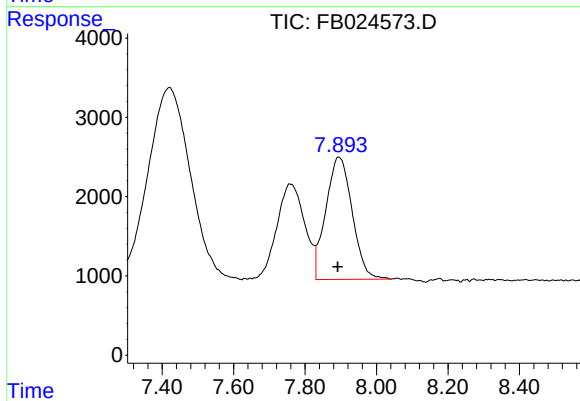


#4 Benzene

R.T.: 7.895 min
Delta R.T.: 0.003 min
Response: 78962
Conc: 2.07 ng/ml

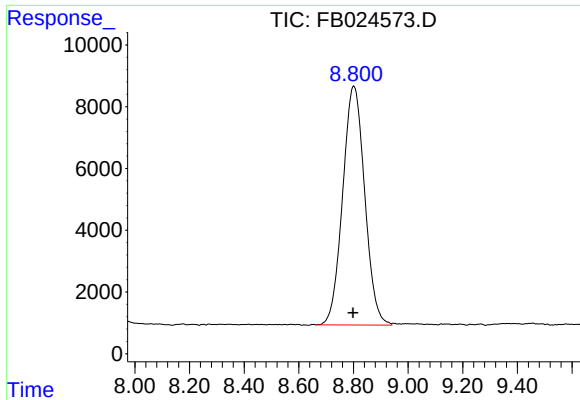


#5 AAA-TFT
 R.T.: 8.801 min
 Delta R.T.: 0.003 min
 Response: 433089
 Conc: 18.80 ng/ml


Instrument :
 FID_B
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2020

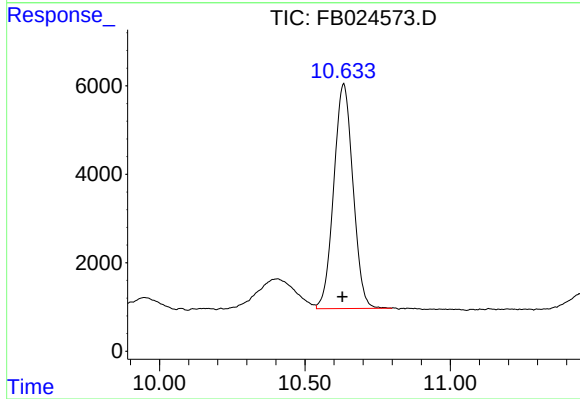


#6 Toluene
 R.T.: 10.634 min
 Delta R.T.: 0.005 min
 Response: 233426
 Conc: 6.38 ng/ml

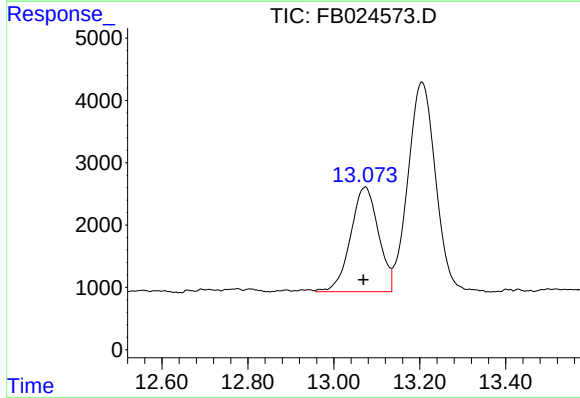

#7 Ethylbenzene
 R.T.: 13.074 min
 Delta R.T.: 0.006 min
 Response: 75539
 Conc: 2.21 ng/ml

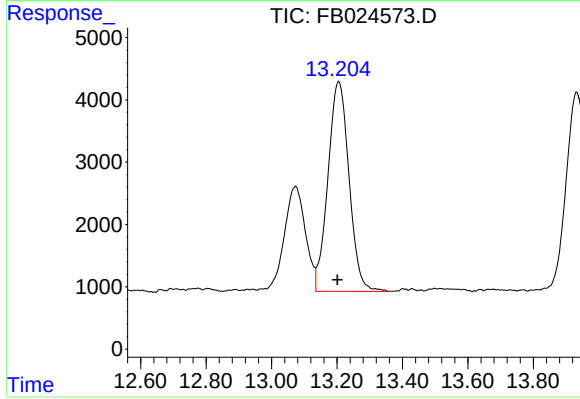


#8 m-Xylene
 R.T.: 13.206 min
 Delta R.T.: 0.004 min
 Response: 150783
 Conc: 4.47 ng/ml

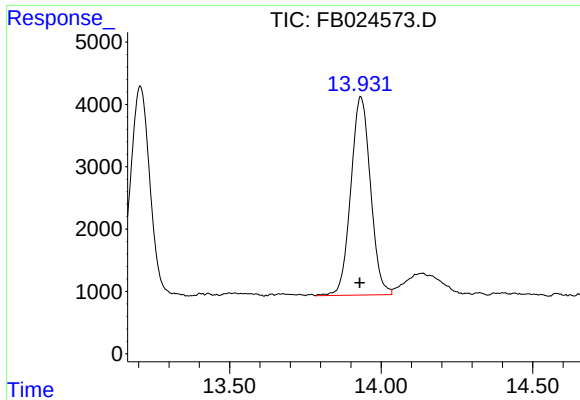

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.004 min
Response: 143742
Conc: 4.37 ng/ml

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT3-2020

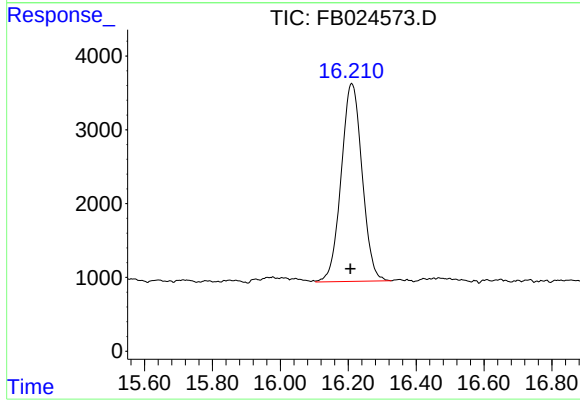

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.004 min
Response: 114620
Conc: 4.25 ng/ml