

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070925\
Data File : FB032034.D
Signal(s) : FID2B.CH
Acq On : 9 Jul 2025 9:18
Operator : YP/AJ
Sample : VBF0708S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0708S1

Integration File: SAMPLE.e
Quant Time: Jul 10 01:21:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.797	360801	23.386 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.723	149	0.006 ng/ml
2) t	2,2,4-Trimethylpentane	7.411	278	0.010 ng/ml
3) t	n-Heptane	7.752	1617	0.065 ng/ml
4) t	Benzene	7.905	744	0.022 ng/ml
6) t	Toluene	10.625	6564	0.184 ng/ml
7) t	Ethylbenzene	13.062	3638	0.115 ng/ml
8) t	m-Xylene	13.199	7763	0.237 ng/ml
9) t	O-Xylene	13.925	8068	0.260 ng/ml
10) t	1,2,4-Trimethylbenzene	16.196	11317	0.428 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070925\
Data File : FB032034.D
Signal(s) : FID2B.CH
Acq On : 9 Jul 2025 9:18
Operator : YP/AJ
Sample : VBF0708S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0708S1

Integration File: SAMPLE.e
Quant Time: Jul 10 01:21:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

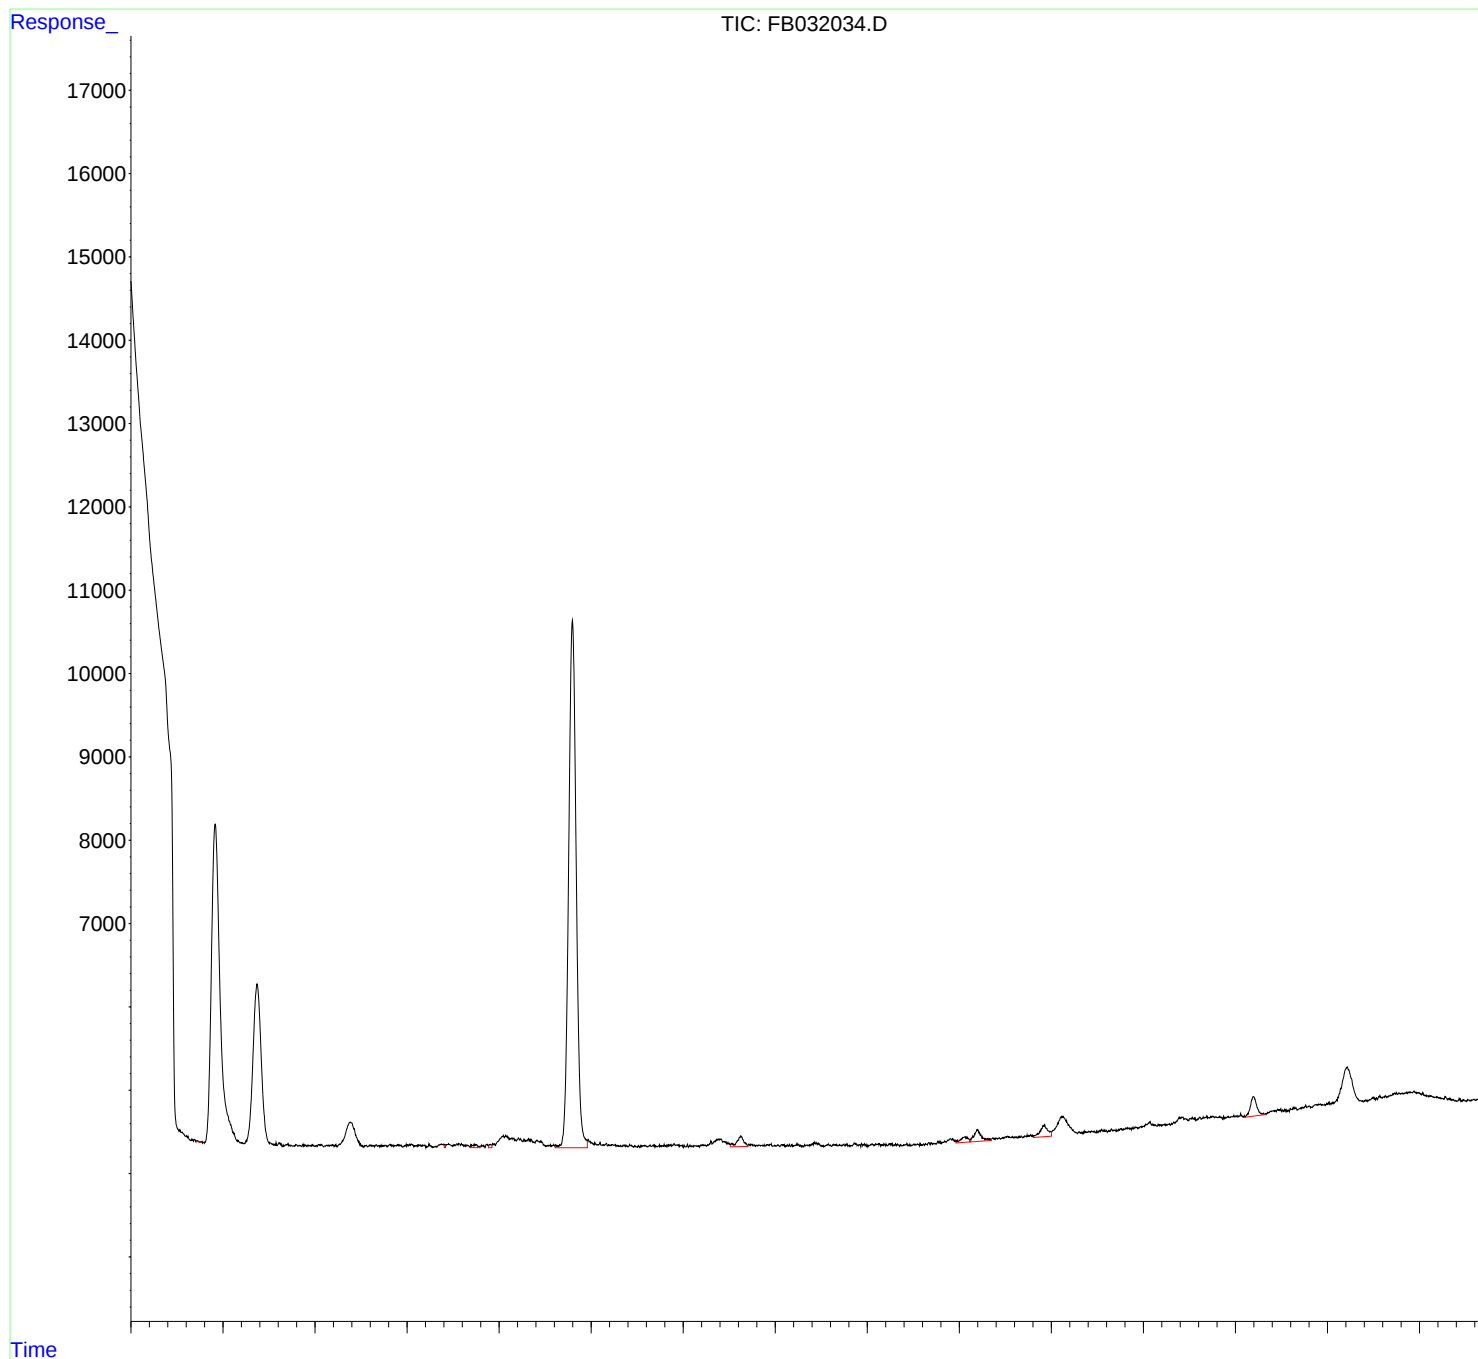


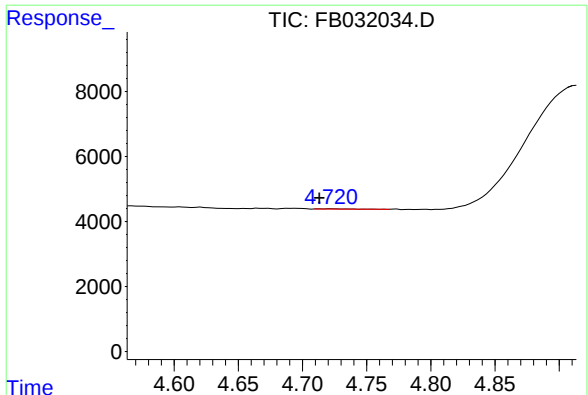

#1 2-Methylpentane


R.T.: 4.723 min
Delta R.T.: 0.010 min
Response: 149
Conc: 0.01 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0708S1

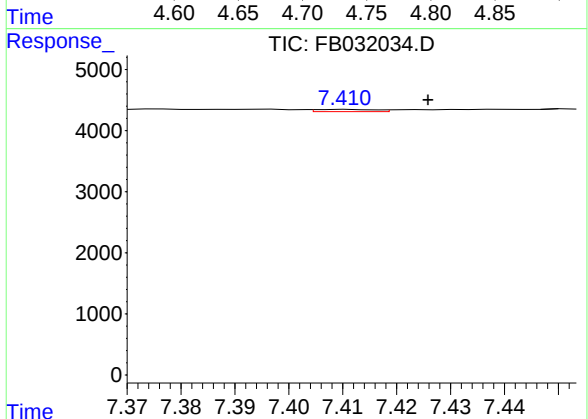


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.015 min
Response: 278
Conc: 0.01 ng/ml

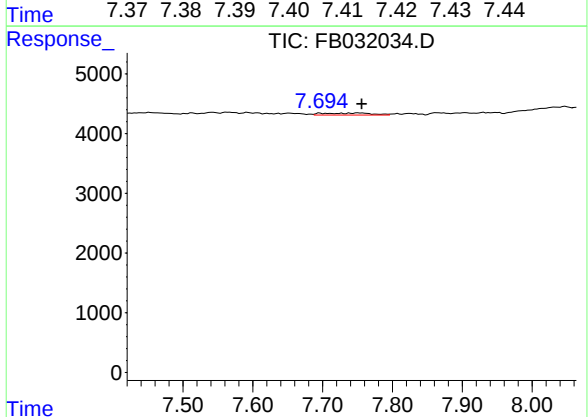


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.004 min
Response: 1617
Conc: 0.06 ng/ml

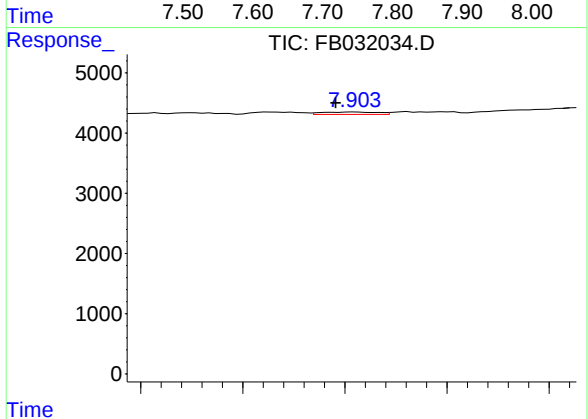

#4 Benzene


R.T.: 7.905 min
Delta R.T.: 0.009 min
Response: 744
Conc: 0.02 ng/ml

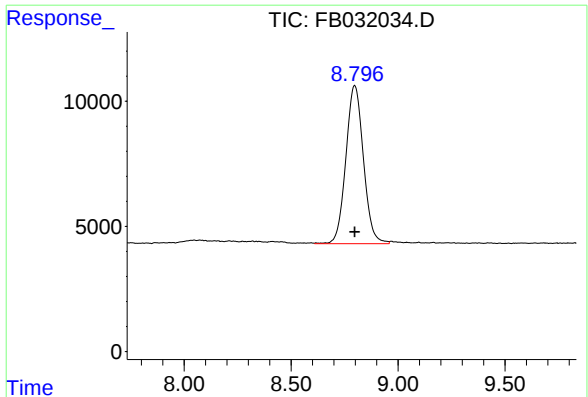

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 360801
Conc: 23.39 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0708S1

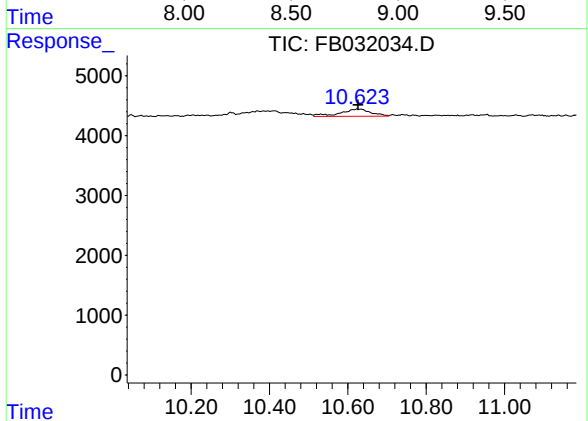


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.001 min
Response: 6564
Conc: 0.18 ng/ml

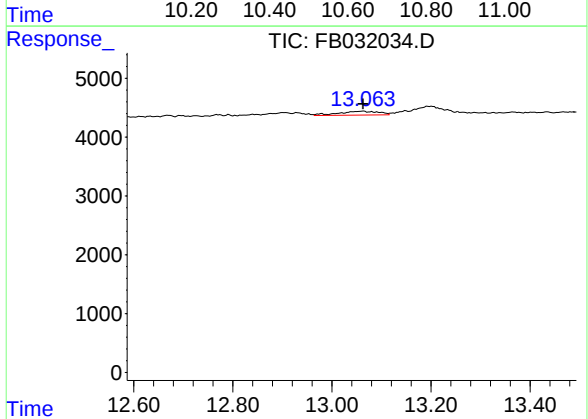


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: -0.001 min
Response: 3638
Conc: 0.12 ng/ml

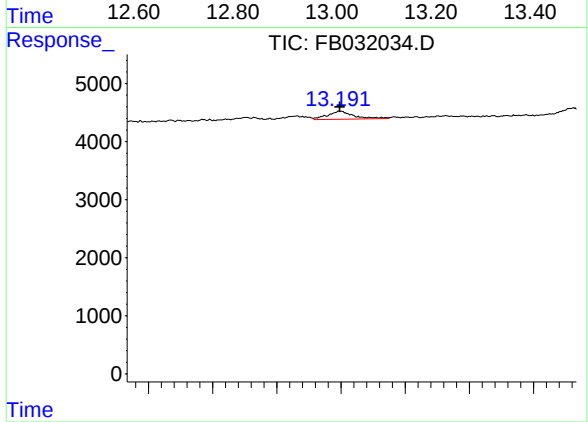

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: 0.003 min
Response: 7763
Conc: 0.24 ng/ml

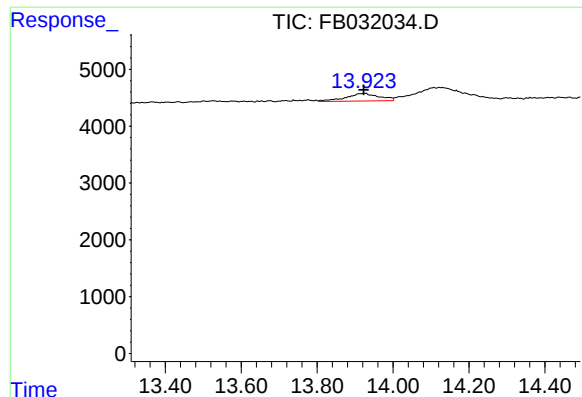

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: 0.002 min
Response: 8068
Conc: 0.26 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0708S1

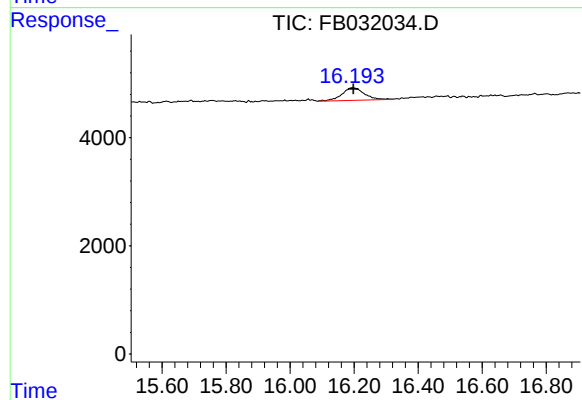

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: -0.002 min
Response: 11317
Conc: 0.43 ng/ml