

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070925\
 Data File : FB032036.D
 Signal(s) : FID2B.CH
 Acq On : 9 Jul 2025 10:13
 Operator : YP/AJ
 Sample : BSF0708S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0708S1

Integration File: SAMPLE.e
 Quant Time: Jul 10 01:21:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
 Quant Title :
 QLast Update : Mon Jun 23 13:56:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.798	274952	17.822 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.715	509642	20.033 ng/ml
2) t	2,2,4-Trimethylpentane	7.426	780165	28.929 ng/ml
3) t	n-Heptane	7.758	227783	9.129 ng/ml
4) t	Benzene	7.897	315484	9.279 ng/ml
6) t	Toluene	10.627	886182	24.783 ng/ml
7) t	Ethylbenzene	13.063	262621	8.317 ng/ml
8) t	m-Xylene	13.196	544412	16.598 ng/ml
9) t	O-Xylene	13.923	519211	16.729 ng/ml
10) t	1,2,4-Trimethylbenzene	16.198	428728	16.215 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070925\
Data File : FB032036.D
Signal(s) : FID2B.CH
Acq On : 9 Jul 2025 10:13
Operator : YP/AJ
Sample : BSF0708S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0708S1

Integration File: SAMPLE.e
Quant Time: Jul 10 01:21:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

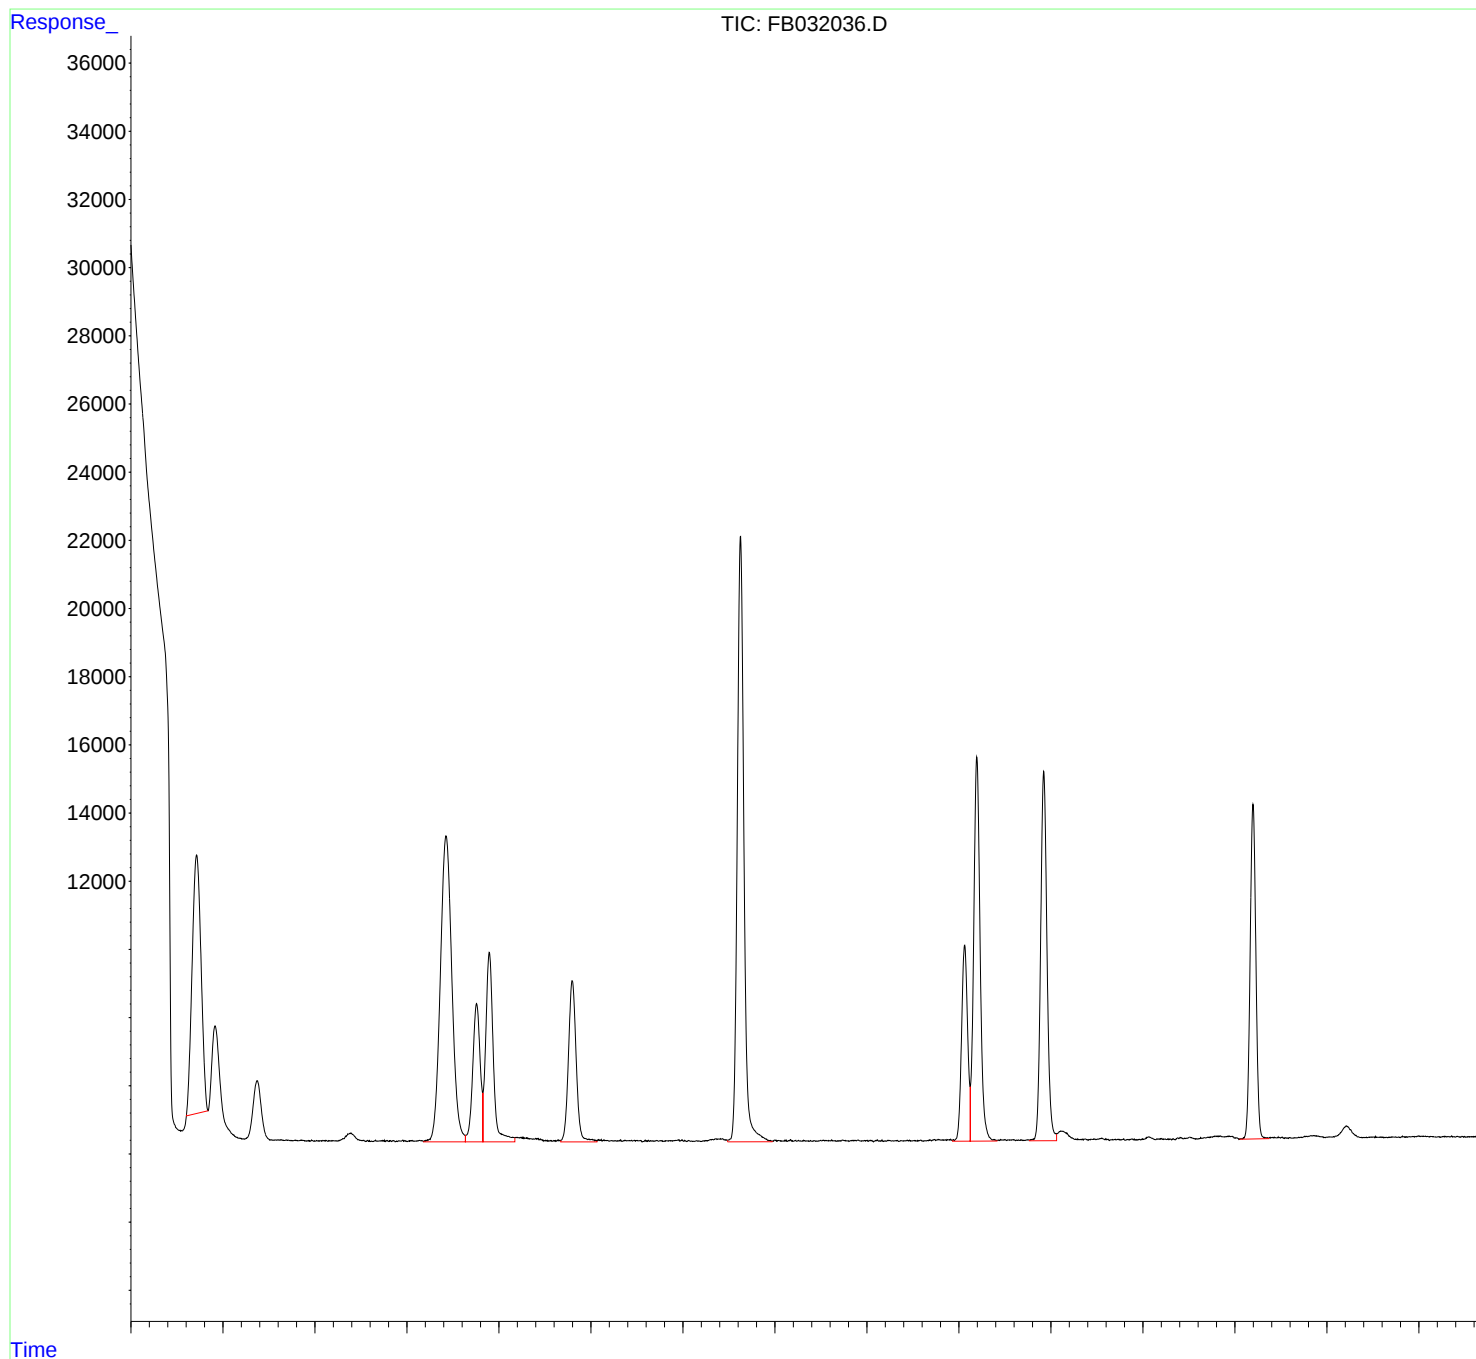


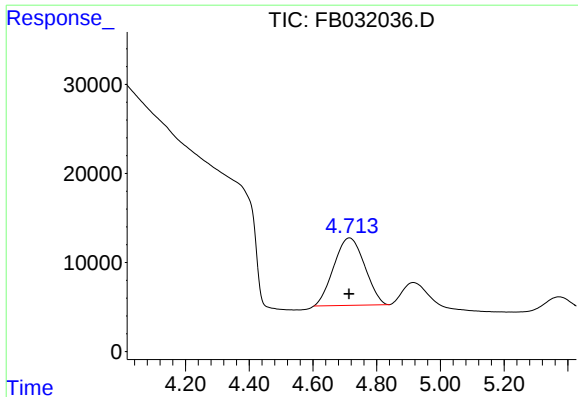

#1 2-Methylpentane


R.T.: 4.715 min
Delta R.T.: 0.002 min
Response: 509642
Conc: 20.03 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0708S1

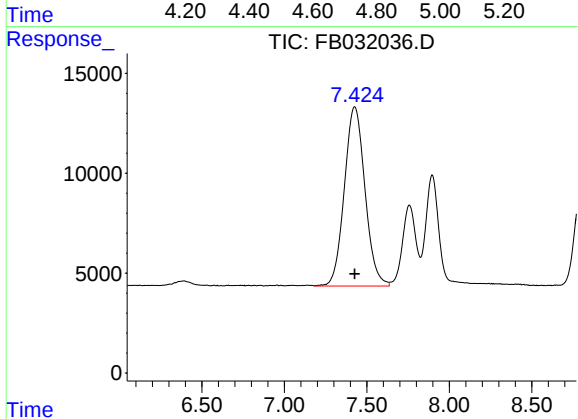


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: 0.000 min
Response: 780165
Conc: 28.93 ng/ml

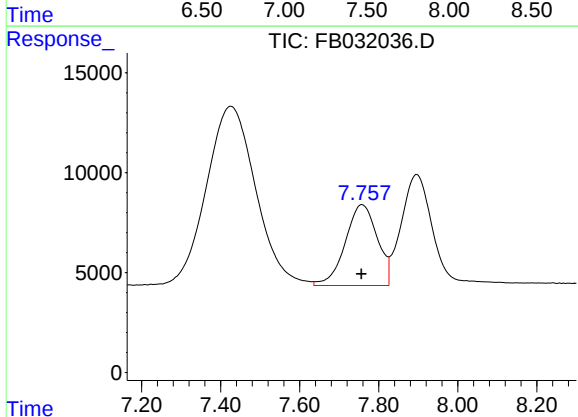


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.002 min
Response: 227783
Conc: 9.13 ng/ml

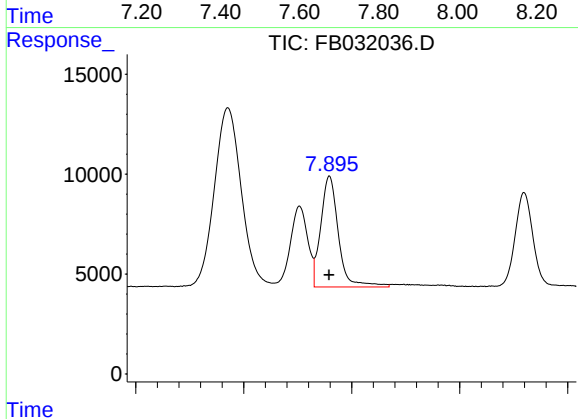

#4 Benzene


R.T.: 7.897 min
Delta R.T.: 0.000 min
Response: 315484
Conc: 9.28 ng/ml

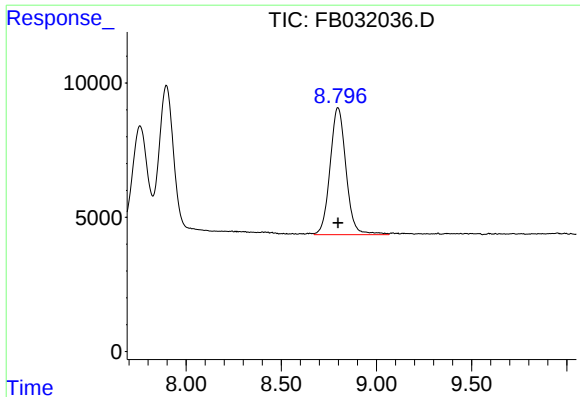

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 274952
Conc: 17.82 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0708S1

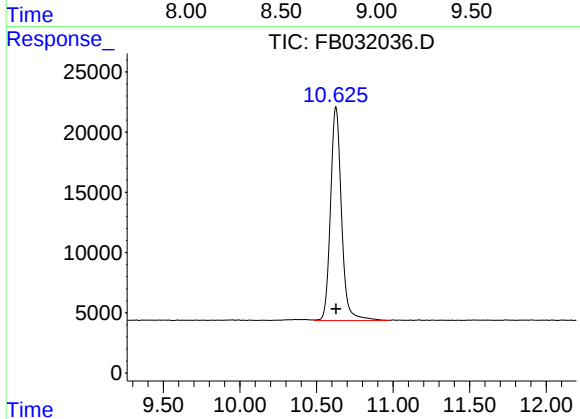


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.000 min
Response: 886182
Conc: 24.78 ng/ml

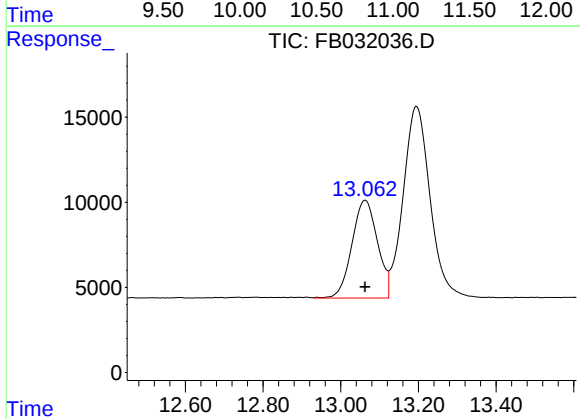


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.000 min
Response: 262621
Conc: 8.32 ng/ml

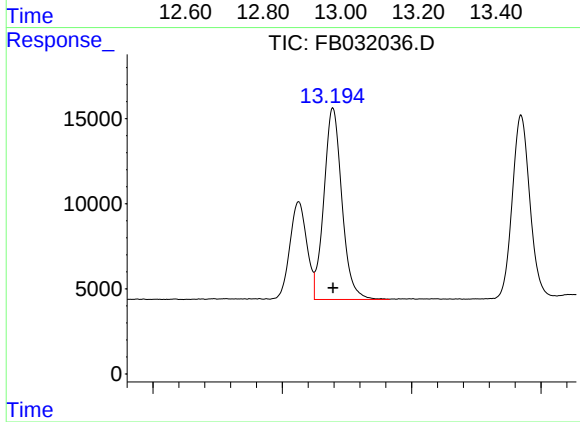

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: 0.000 min
Response: 544412
Conc: 16.60 ng/ml

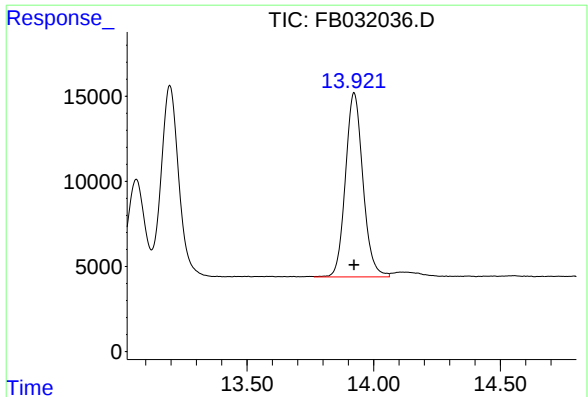

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: 0.000 min
Response: 519211
Conc: 16.73 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0708S1

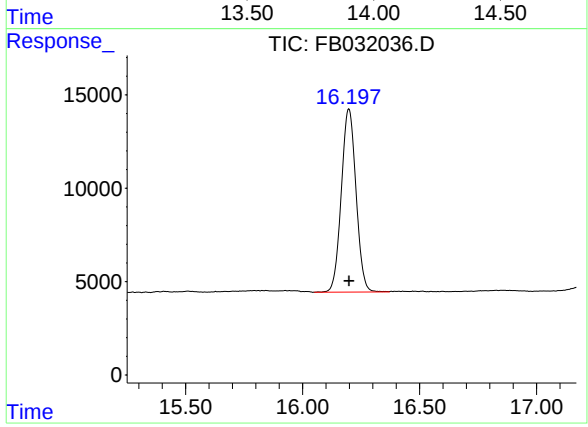

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.000 min
Response: 428728
Conc: 16.21 ng/ml