

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070925\
 Data File : FB032038.D
 Signal(s) : FID2B.CH
 Acq On : 9 Jul 2025 11:26
 Operator : YP/AJ
 Sample : Q2487-10
 Misc : 3.50G/5.00 ML DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 G4(6-12)

Integration File: SAMPLE.e
 Quant Time: Jul 10 01:22:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
 Quant Title :
 QLast Update : Mon Jun 23 13:56:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.797	302539	19.610 ng/ml
Target Compounds				
2) t	2,2,4-Trimethylpentane	7.429	279	0.010 ng/ml
3) t	n-Heptane	7.722	3031	0.121 ng/ml
4) t	Benzene	7.952	3901	0.115 ng/ml
6) t	Toluene	10.611	3778	0.106 ng/ml
7) t	Ethylbenzene	13.075	1685	0.053 ng/ml
8) t	m-Xylene	13.188	3855	0.118 ng/ml
9) t	O-Xylene	13.914	6273	0.202 ng/ml
10) t	1,2,4-Trimethylbenzene	16.202	5205	0.197 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070925\
Data File : FB032038.D
Signal(s) : FID2B.CH
Acq On : 9 Jul 2025 11:26
Operator : YP/AJ
Sample : Q2487-10
Misc : 3.50G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
G4(6-12)

Integration File: SAMPLE.e
Quant Time: Jul 10 01:22:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

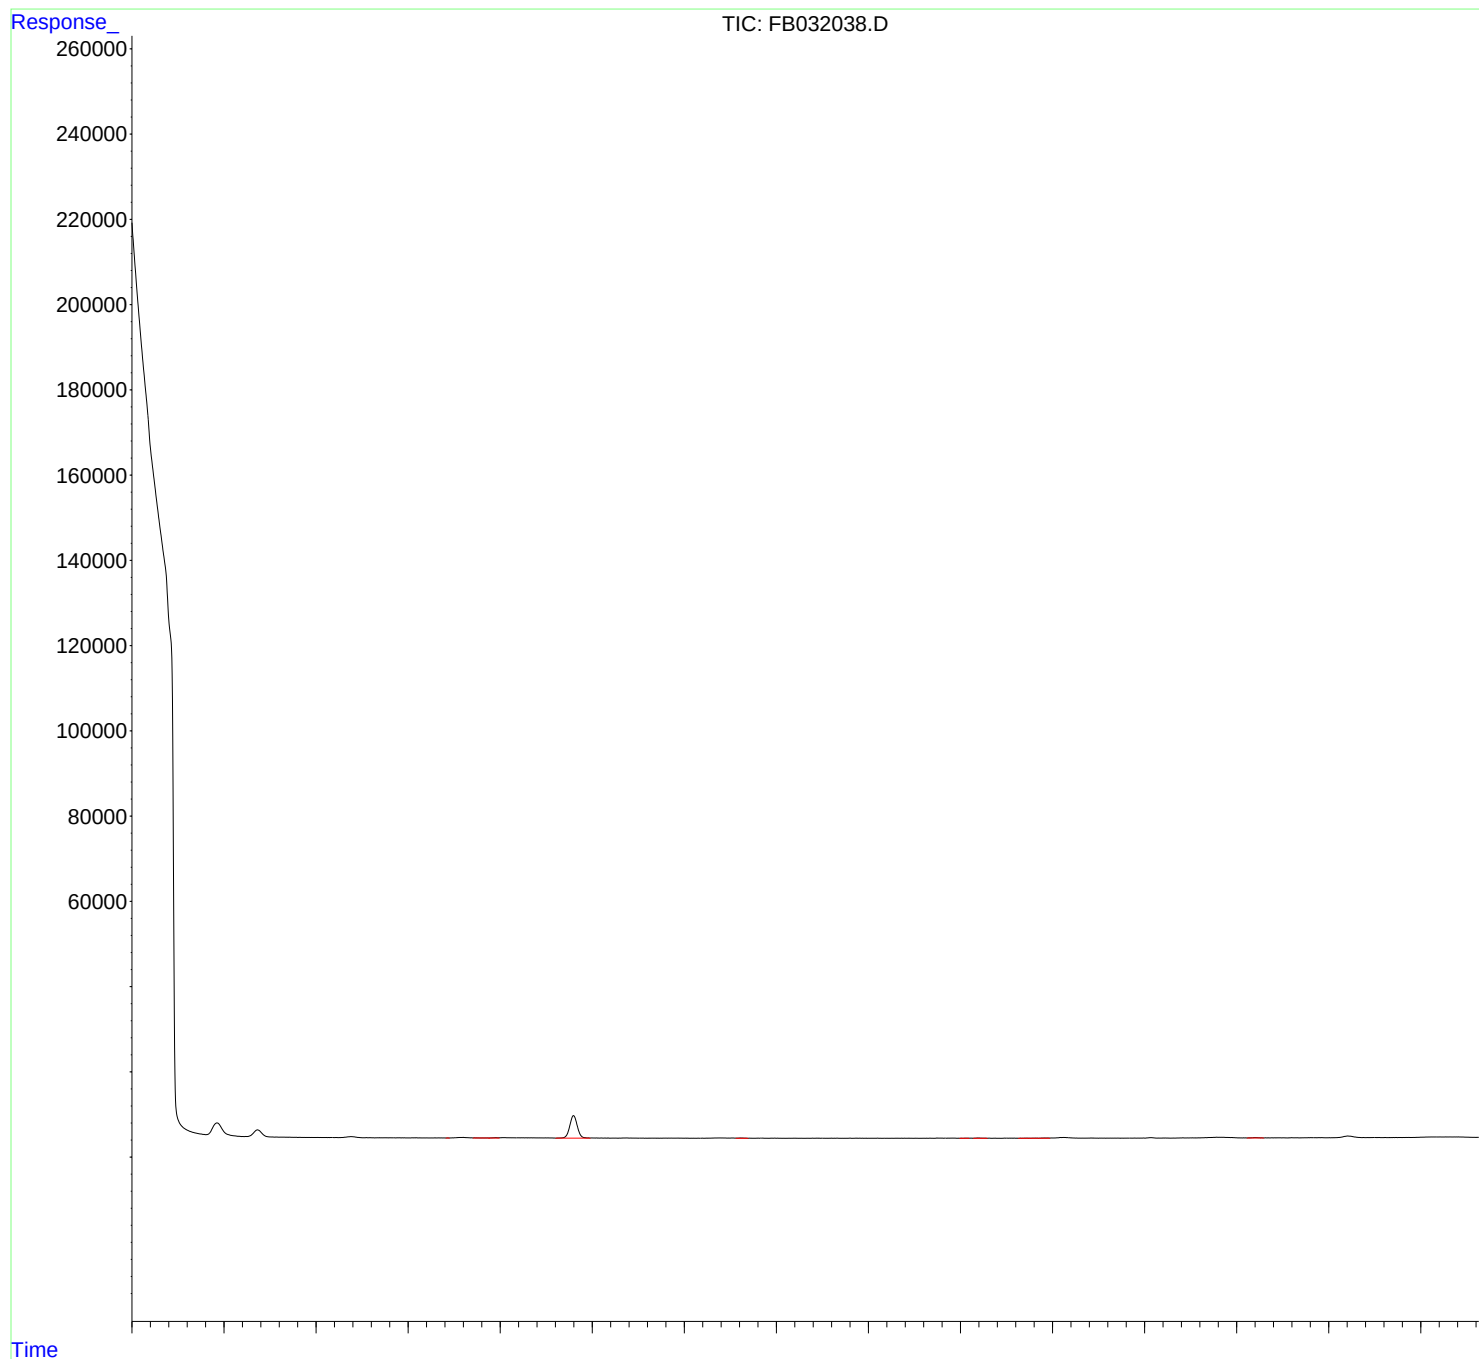


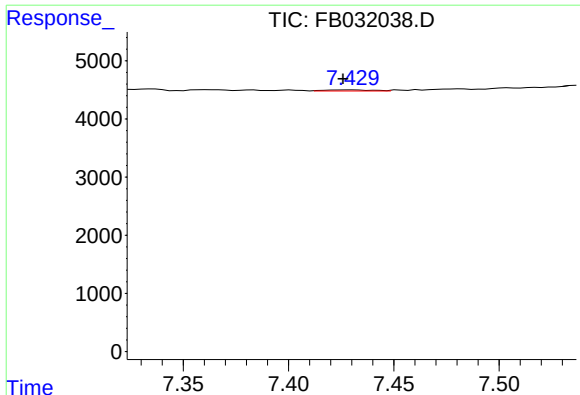

#2 2,2,4-Trimethylpentane


R.T.: 7.429 min
Delta R.T.: 0.003 min
Response: 279
Conc: 0.01 ng/ml

Instrument :
FID_B
ClientSampleId :
G4(6-12)

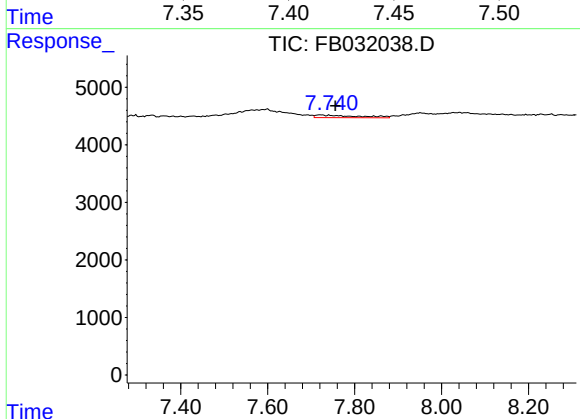


#3 n-Heptane

R.T.: 7.722 min
Delta R.T.: -0.034 min
Response: 3031
Conc: 0.12 ng/ml

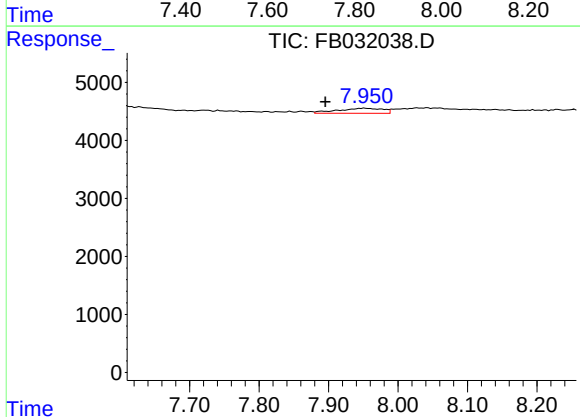


#4 Benzene

R.T.: 7.952 min
Delta R.T.: 0.057 min
Response: 3901
Conc: 0.11 ng/ml

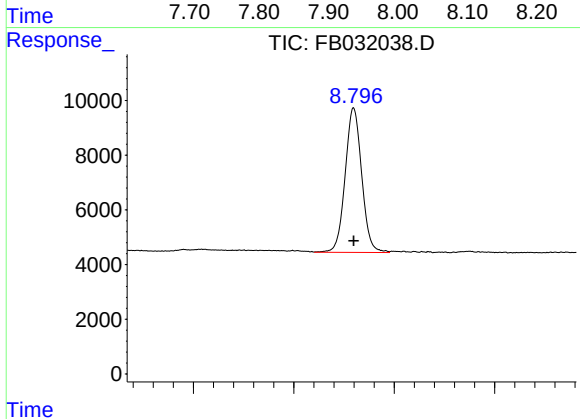

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 302539
Conc: 19.61 ng/ml

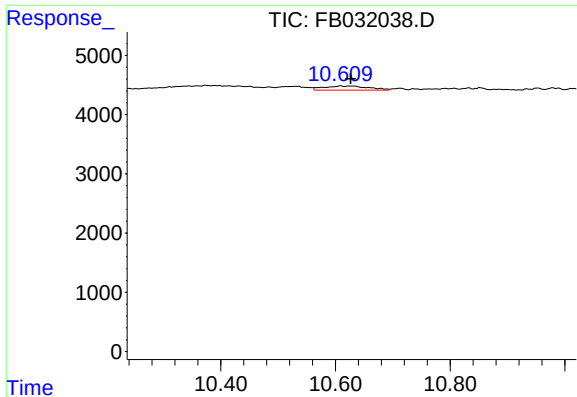

#6 Toluene


R.T.: 10.611 min
Delta R.T.: -0.016 min
Response: 3778
Conc: 0.11 ng/ml

Instrument :
FID_B
ClientSampleId :
G4(6-12)

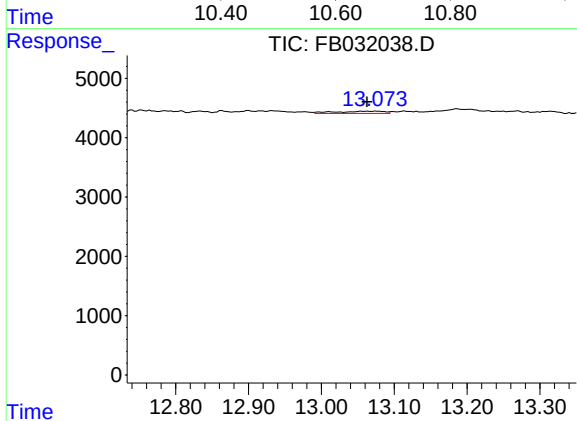


#7 Ethylbenzene

R.T.: 13.075 min
Delta R.T.: 0.012 min
Response: 1685
Conc: 0.05 ng/ml

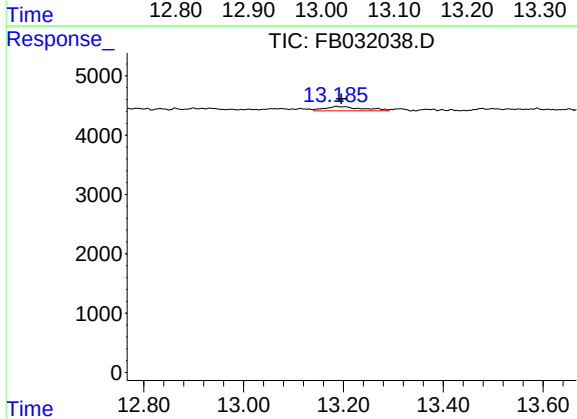


#8 m-Xylene

R.T.: 13.188 min
Delta R.T.: -0.007 min
Response: 3855
Conc: 0.12 ng/ml

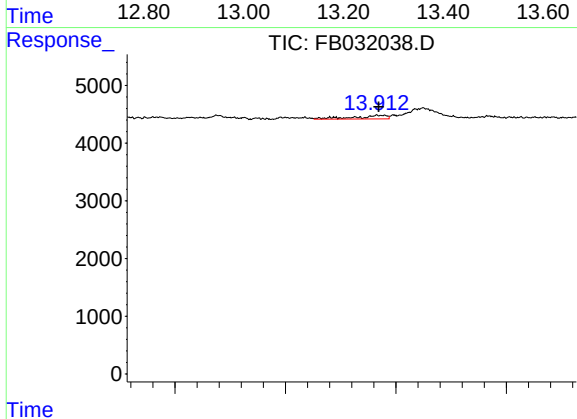

#9 o-Xylene

R.T.: 13.914 min
Delta R.T.: -0.009 min
Response: 6273
Conc: 0.20 ng/ml

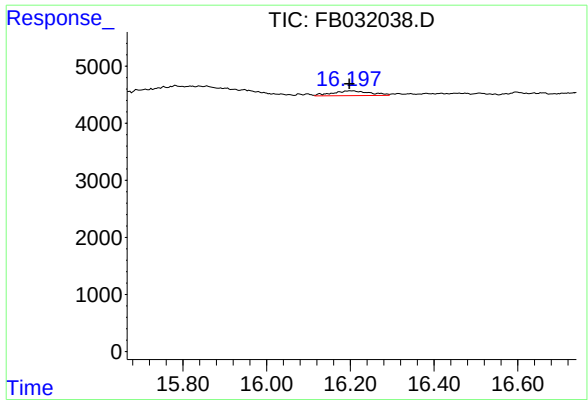

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: 0.004 min
Response: 5205
Conc: 0.20 ng/ml

Instrument :
FID_B
ClientSampleId :
G4(6-12)