

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070925\
 Data File : FB032039.D
 Signal(s) : FID2B.CH
 Acq On : 9 Jul 2025 11:53
 Operator : YP/AJ
 Sample : Q2487-11
 Misc : 4.50G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 G3(0-6)

Integration File: SAMPLE.e
 Quant Time: Jul 10 01:22:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
 Quant Title :
 QLast Update : Mon Jun 23 13:56:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.797	309780	20.079 ng/ml
Target Compounds				
2) t	2,2,4-Trimethylpentane	7.451	508	0.019 ng/ml
3) t	n-Heptane	7.749	1373	0.055 ng/ml
4) t	Benzene	7.866	902	0.027 ng/ml
6) t	Toluene	10.620	1775	0.050 ng/ml
7) t	Ethylbenzene	13.074	2207	0.070 ng/ml
8) t	m-Xylene	13.200	3948	0.120 ng/ml
9) t	O-Xylene	13.910	3800	0.122 ng/ml
10) t	1,2,4-Trimethylbenzene	16.195	4317	0.163 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070925\
Data File : FB032039.D
Signal(s) : FID2B.CH
Acq On : 9 Jul 2025 11:53
Operator : YP/AJ
Sample : Q2487-11
Misc : 4.50G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
G3(0-6)

Integration File: SAMPLE.e
Quant Time: Jul 10 01:22:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

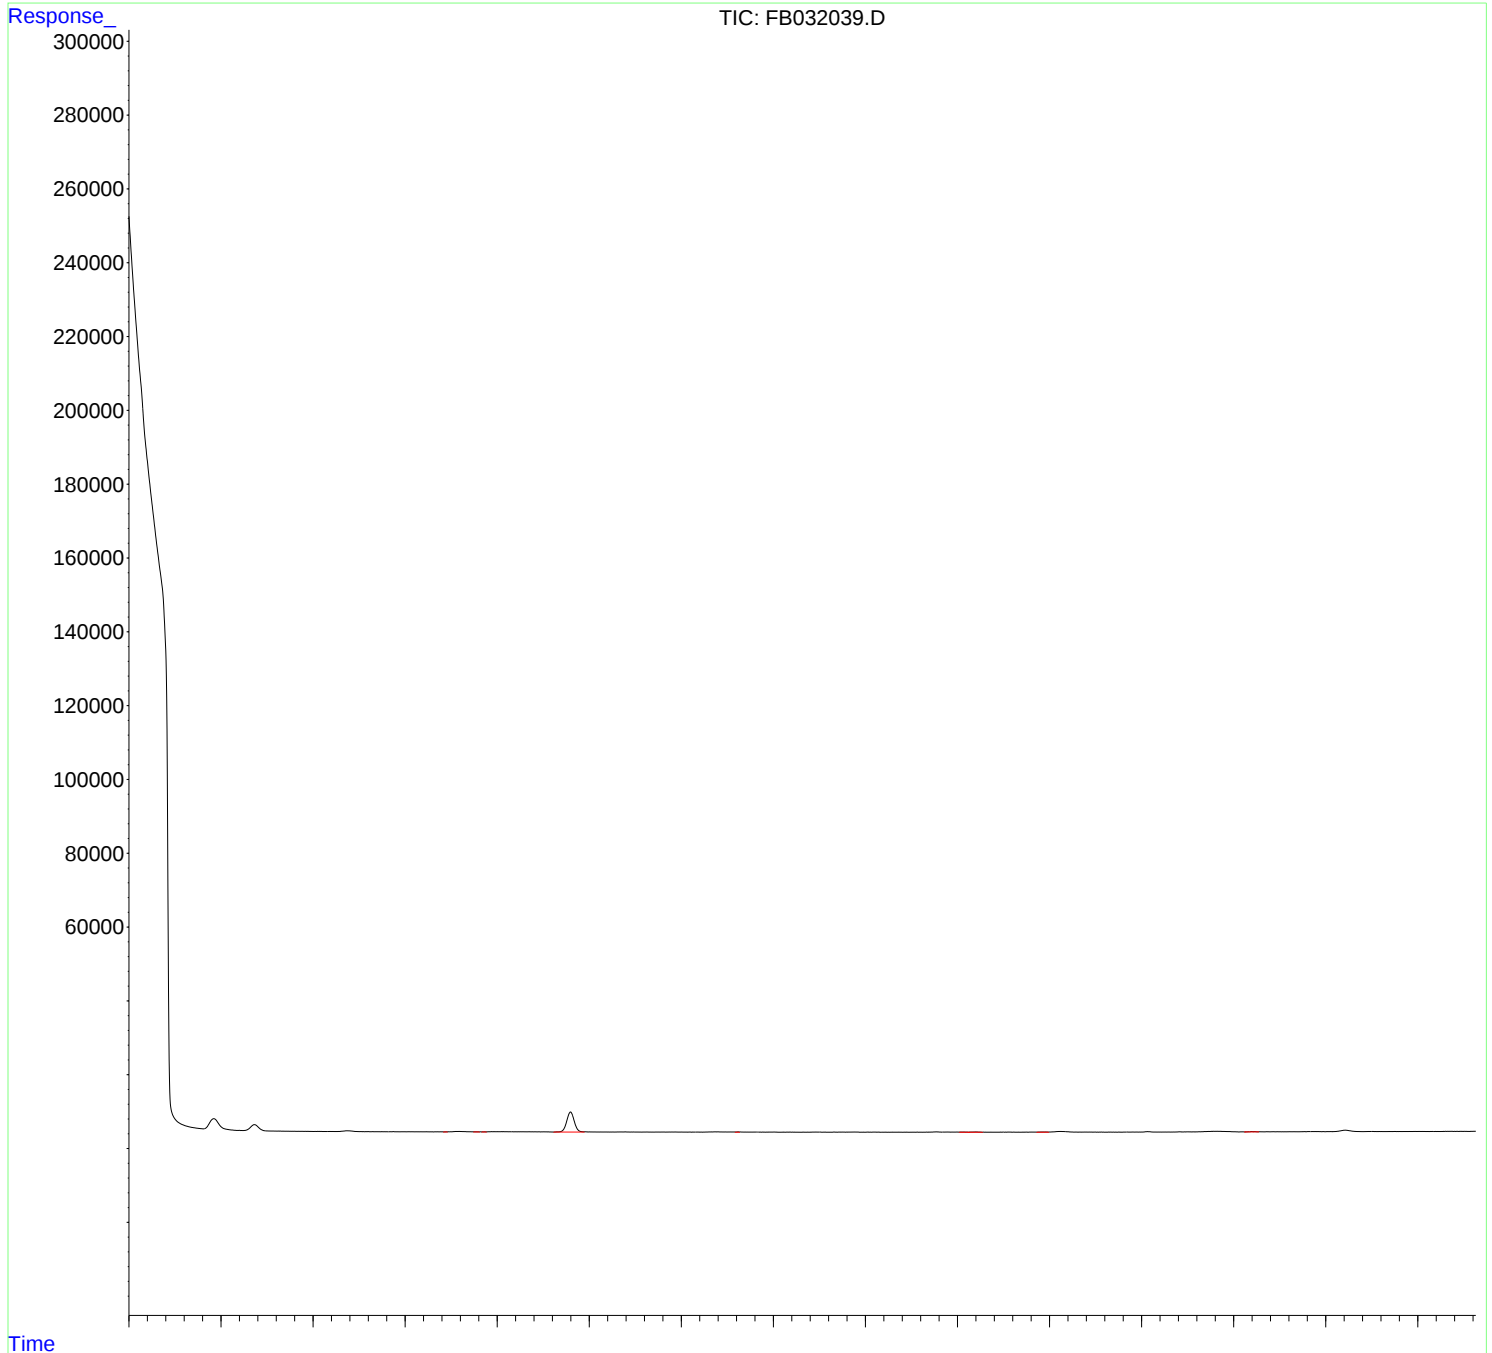


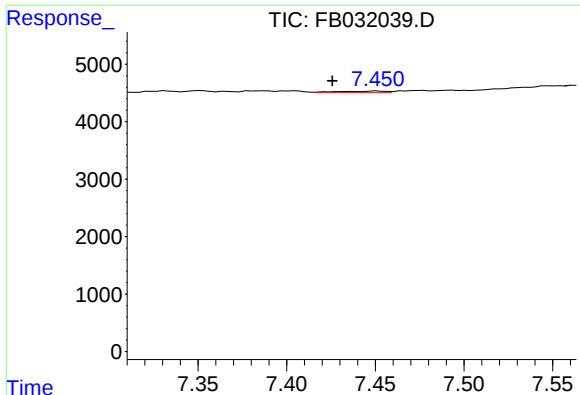

#2 2,2,4-Trimethylpentane


R.T.: 7.451 min
Delta R.T.: 0.025 min
Response: 508
Conc: 0.02 ng/ml

Instrument :
FID_B
ClientSampleId :
G3(0-6)

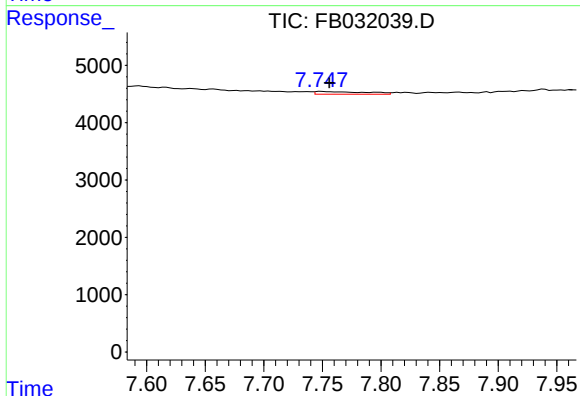


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.007 min
Response: 1373
Conc: 0.06 ng/ml

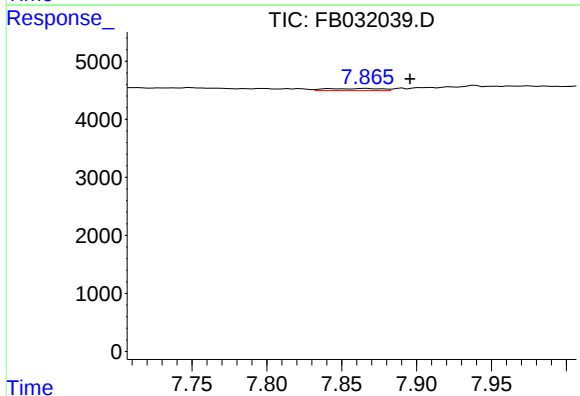


#4 Benzene

R.T.: 7.866 min
Delta R.T.: -0.029 min
Response: 902
Conc: 0.03 ng/ml

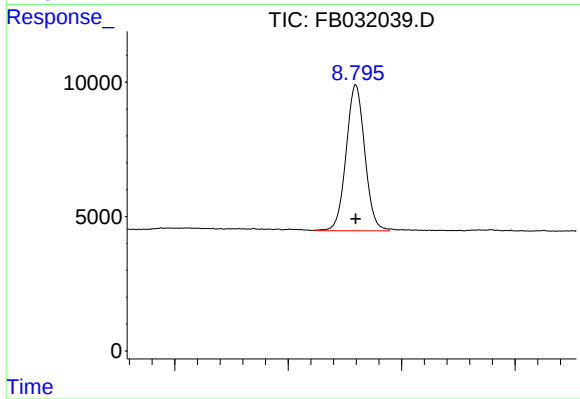

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 309780
Conc: 20.08 ng/ml

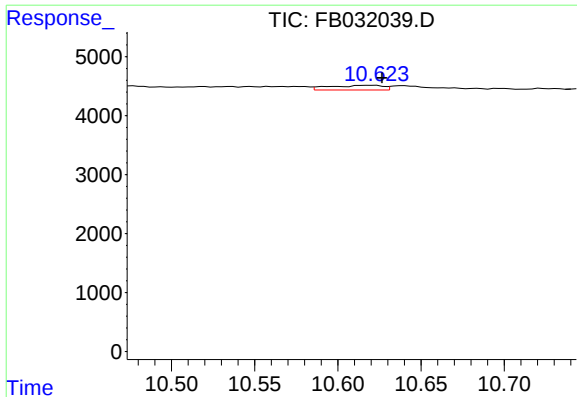

#6 Toluene


R.T.: 10.620 min
Delta R.T.: -0.006 min
Response: 1775
Conc: 0.05 ng/ml

Instrument :
FID_B
ClientSampleId :
G3(0-6)

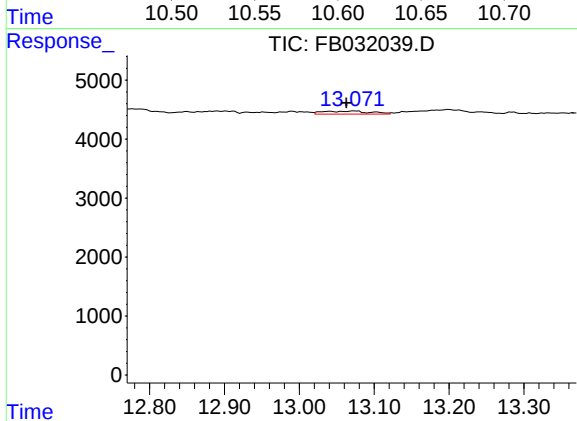


#7 Ethylbenzene

R.T.: 13.074 min
Delta R.T.: 0.011 min
Response: 2207
Conc: 0.07 ng/ml

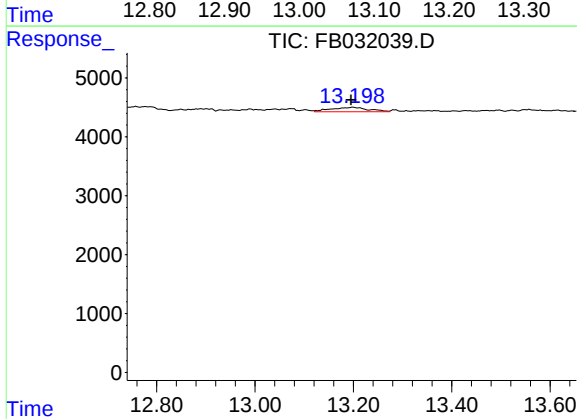


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: 0.004 min
Response: 3948
Conc: 0.12 ng/ml

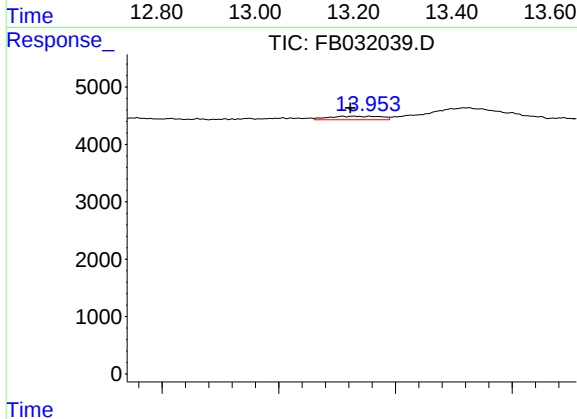

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: -0.013 min
Response: 3800
Conc: 0.12 ng/ml

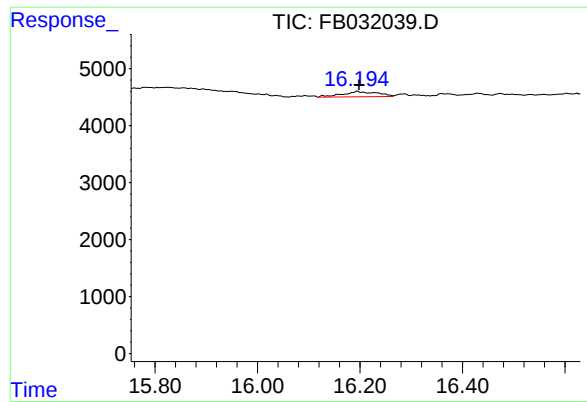

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: -0.002 min
Response: 4317
Conc: 0.16 ng/ml

Instrument :
FID_B
ClientSampleId :
G3(0-6)