

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070925\
Data File : FB032041.D
Signal(s) : FID2B.CH
Acq On : 9 Jul 2025 12:48
Operator : YP/AJ
Sample : Q2487-13
Misc : 4.15G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
G2(0-6)

Integration File: SAMPLE.e
Quant Time: Jul 10 01:22:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.803	15674	1.016 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.716	79	0.003 ng/ml
2) t	2,2,4-Trimethylpentane	7.431	503	0.019 ng/ml
3) t	n-Heptane	7.766	280	0.011 ng/ml
4) t	Benzene	7.887	629	0.019 ng/ml
6) t	Toluene	10.631	650	0.018 ng/ml
7) t	Ethylbenzene	13.064	515	0.016 ng/ml
8) t	m-Xylene	13.175	293	0.009 ng/ml
9) t	O-Xylene	13.956	744	0.024 ng/ml
10) t	1,2,4-Trimethylbenzene	16.210	432	0.016 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070925\
Data File : FB032041.D
Signal(s) : FID2B.CH
Acq On : 9 Jul 2025 12:48
Operator : YP/AJ
Sample : Q2487-13
Misc : 4.15G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
G2(0-6)

Integration File: SAMPLE.e
Quant Time: Jul 10 01:22:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

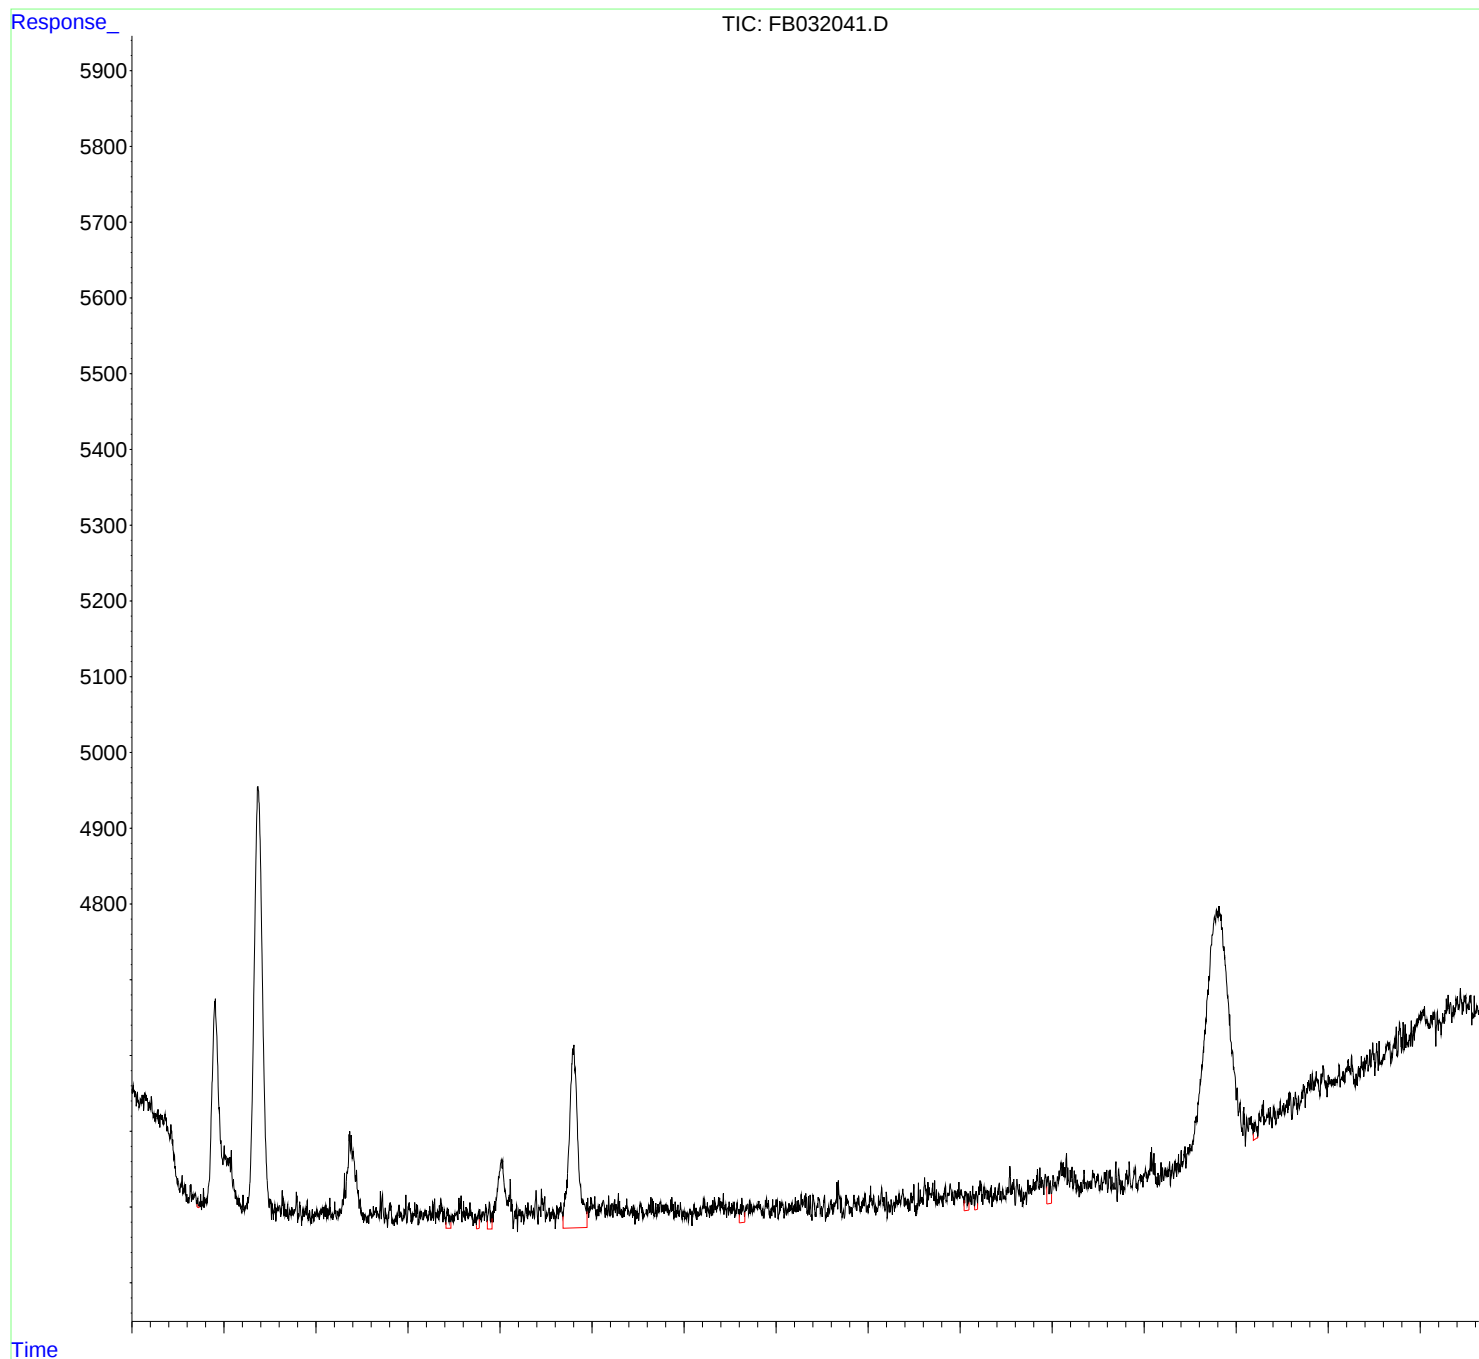


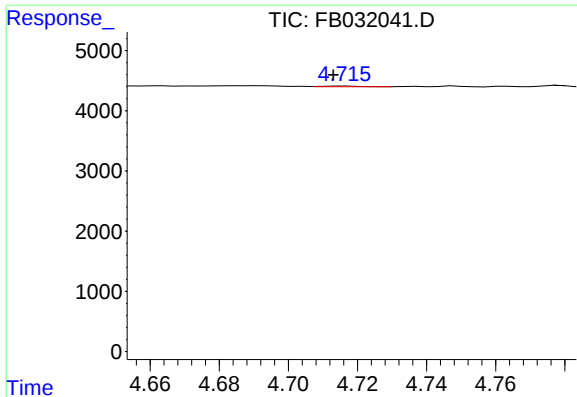

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: 0.003 min
Response: 79
Conc: 0.00 ng/ml

Instrument :
FID_B
ClientSampleId :
G2(0-6)

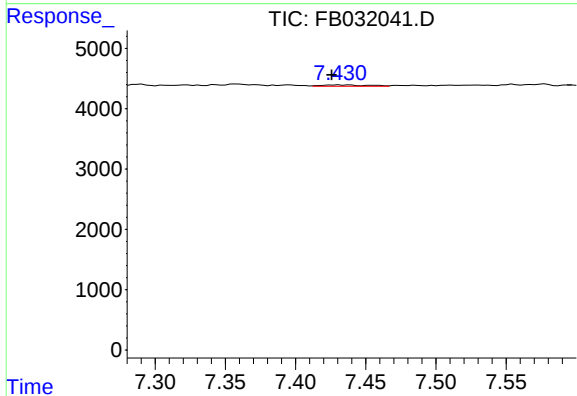


#2 2,2,4-Trimethylpentane

R.T.: 7.431 min
Delta R.T.: 0.005 min
Response: 503
Conc: 0.02 ng/ml

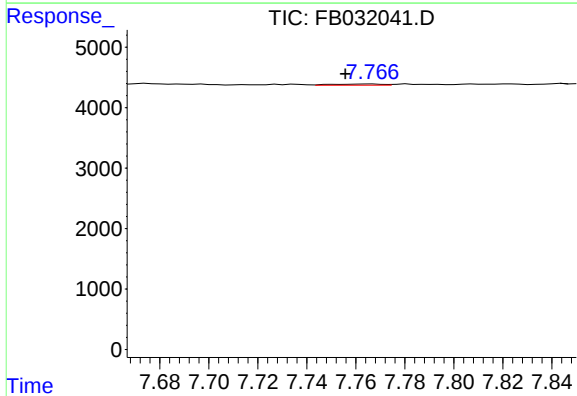


#3 n-Heptane

R.T.: 7.766 min
Delta R.T.: 0.010 min
Response: 280
Conc: 0.01 ng/ml

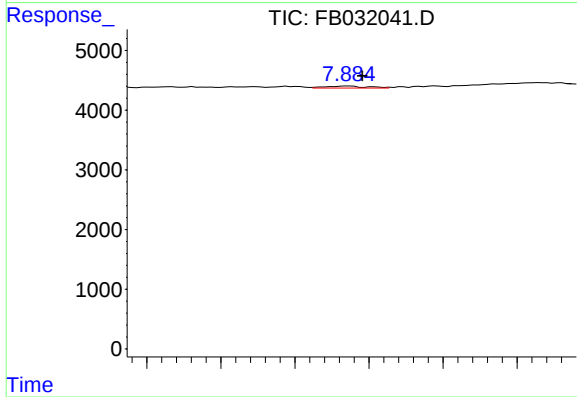

#4 Benzene

R.T.: 7.887 min
Delta R.T.: -0.009 min
Response: 629
Conc: 0.02 ng/ml

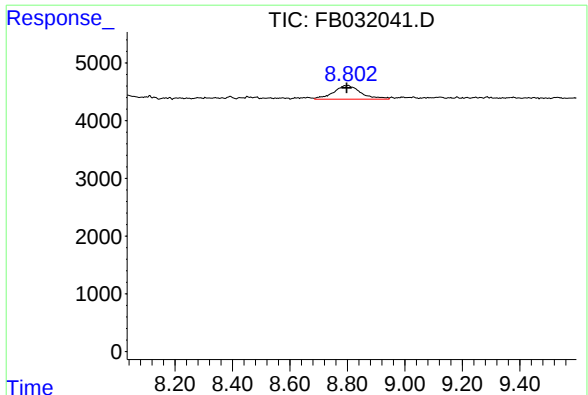

#5 AAA-TFT

R.T.: 8.803 min
Delta R.T.: 0.005 min
Response: 15674
Conc: 1.02 ng/ml

Instrument :
FID_B
ClientSampleId :
G2(0-6)

#6 Toluene


R.T.: 10.631 min
Delta R.T.: 0.004 min
Response: 650
Conc: 0.02 ng/ml

#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: 0.001 min
Response: 515
Conc: 0.02 ng/ml

#8 m-Xylene


R.T.: 13.175 min
Delta R.T.: -0.021 min
Response: 293
Conc: 0.01 ng/ml

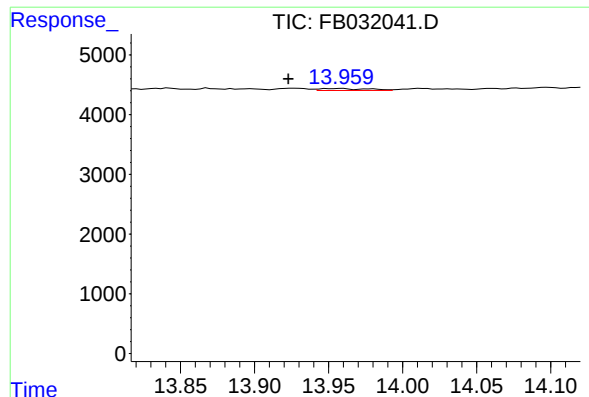

#9 O-Xylene

R.T.: 13.956 min
Delta R.T.: 0.033 min
Response: 744
Conc: 0.02 ng/ml

Instrument :
FID_B
ClientSampleId :
G2(0-6)

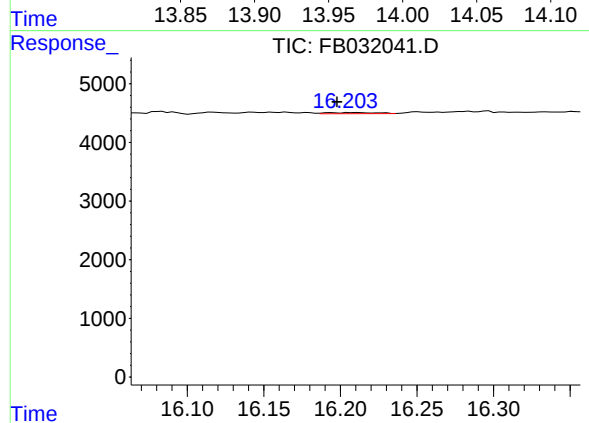

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.012 min
Response: 432
Conc: 0.02 ng/ml