

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070925\
 Data File : FB032048.D
 Signal(s) : FID2B.CH
 Acq On : 9 Jul 2025 17:37
 Operator : YP/AJ
 Sample : Q2514-07
 Misc : 4.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TP-36

Integration File: SAMPLE.e
 Quant Time: Jul 10 01:23:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
 Quant Title :
 QLast Update : Mon Jun 23 13:56:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.803	281701	18.259 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.718	269	0.011 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	132	0.005 ng/ml
3) t n-Heptane	7.779	404	0.016 ng/ml
4) t Benzene	7.892	831	0.024 ng/ml
6) t Toluene	10.634	3642	0.102 ng/ml
8) t m-Xylene	13.191	4150	0.127 ng/ml
9) t O-Xylene	13.912	3010	0.097 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	3240	0.123 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070925\
Data File : FB032048.D
Signal(s) : FID2B.CH
Acq On : 9 Jul 2025 17:37
Operator : YP/AJ
Sample : Q2514-07
Misc : 4.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-36

Integration File: SAMPLE.e
Quant Time: Jul 10 01:23:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

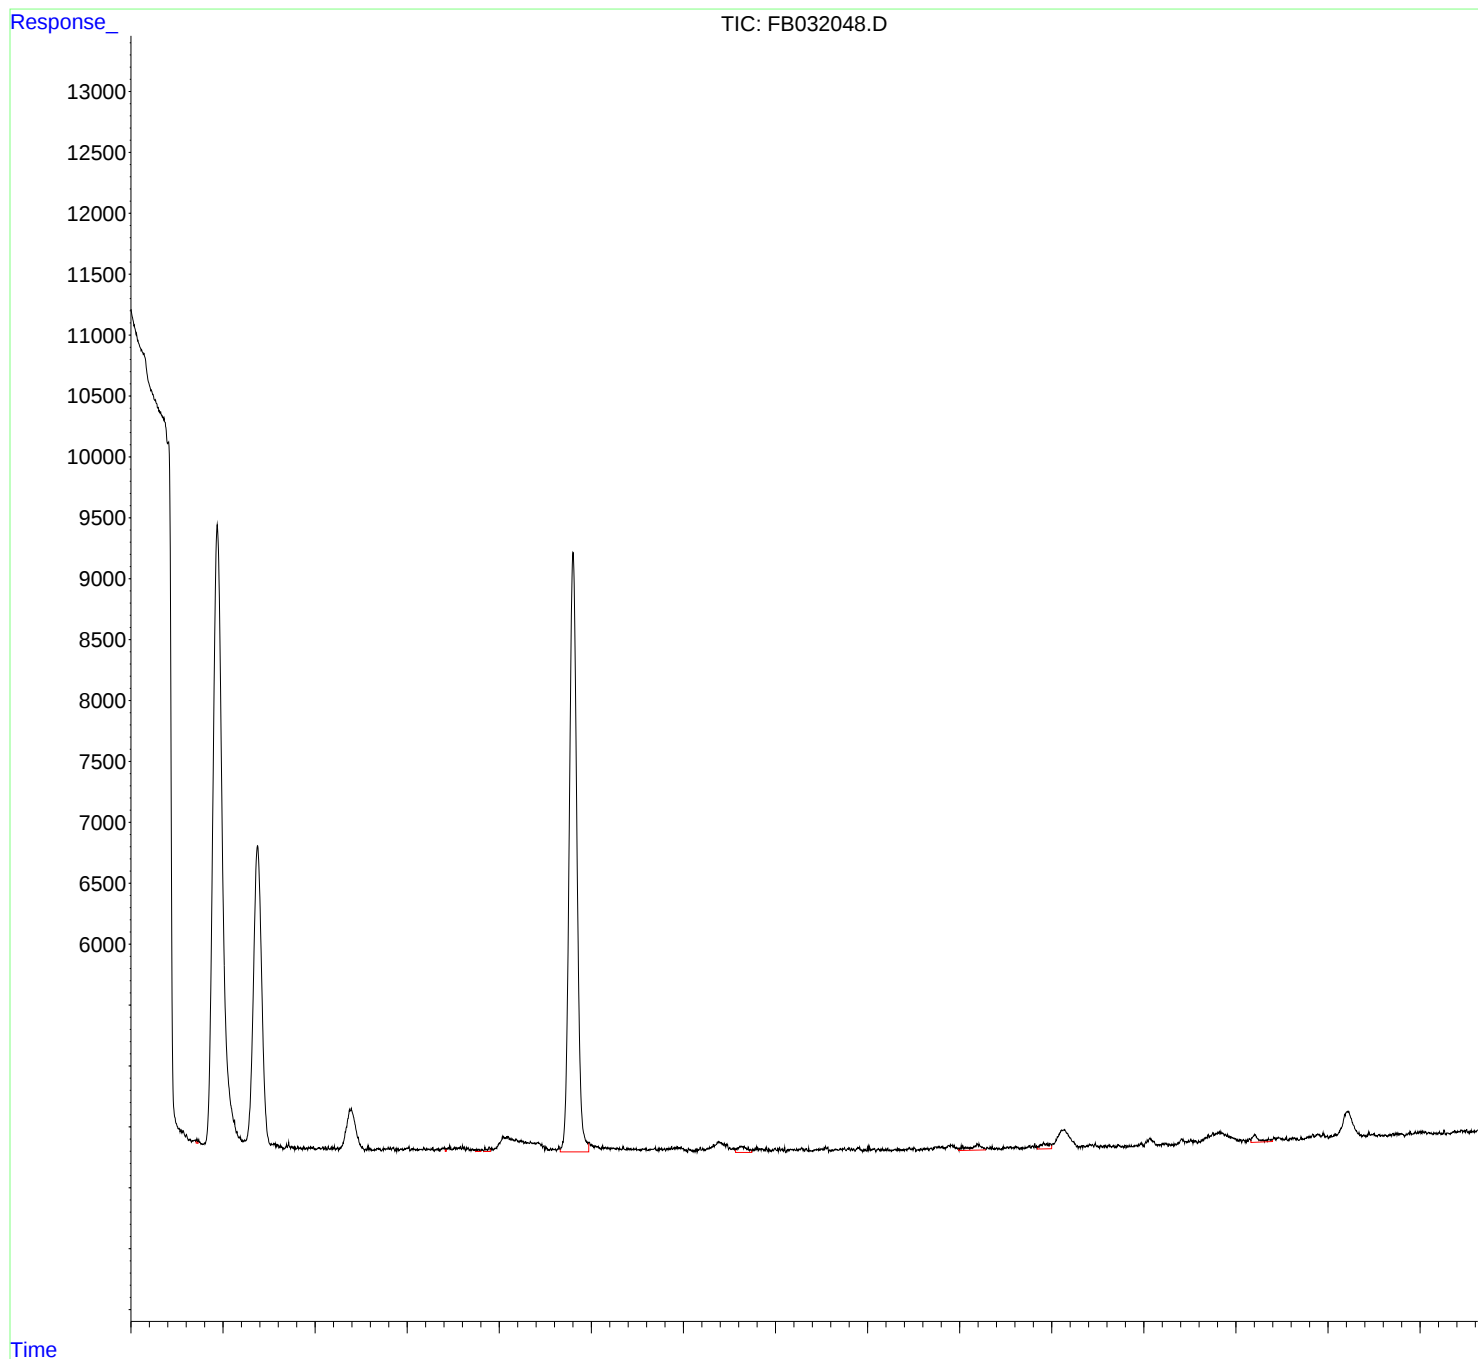


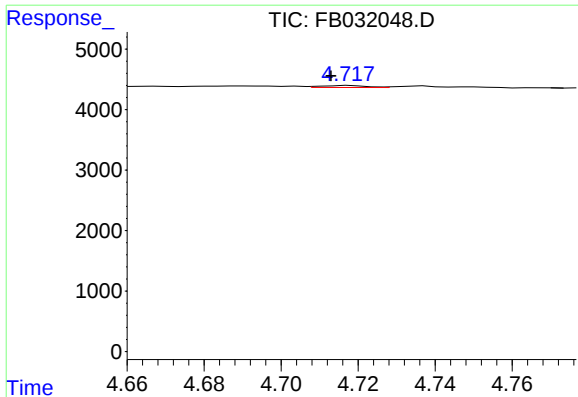

#1 2-Methylpentane


R.T.: 4.718 min
Delta R.T.: 0.005 min
Response: 269
Conc: 0.01 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-36

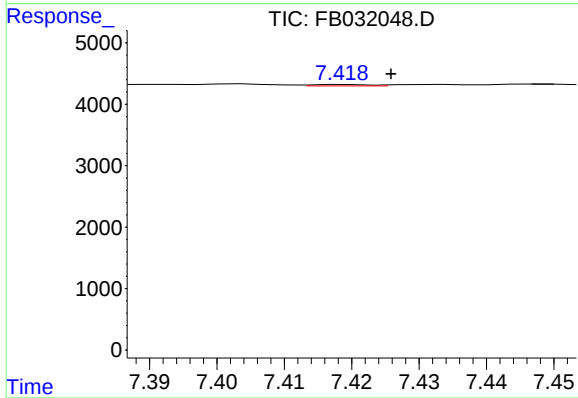


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: -0.007 min
Response: 132
Conc: 0.00 ng/ml

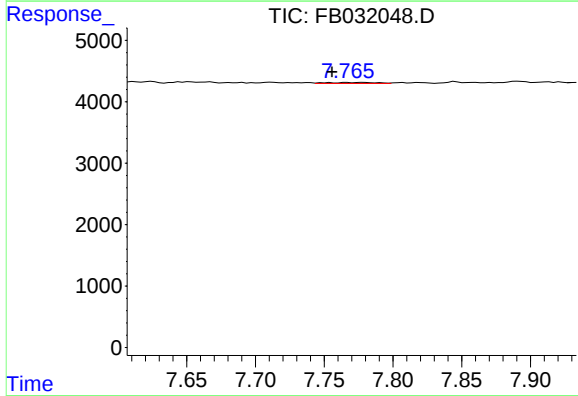


#3 n-Heptane

R.T.: 7.779 min
Delta R.T.: 0.023 min
Response: 404
Conc: 0.02 ng/ml

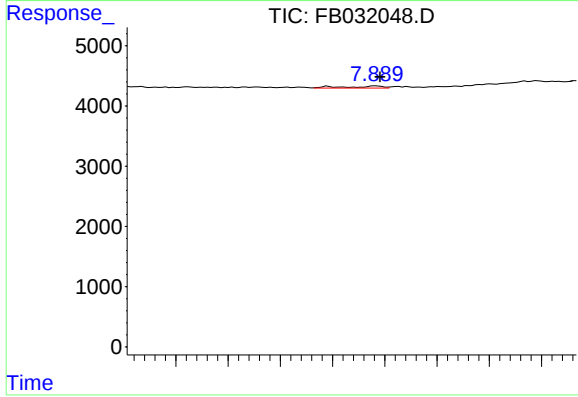

#4 Benzene


R.T.: 7.892 min
Delta R.T.: -0.004 min
Response: 831
Conc: 0.02 ng/ml

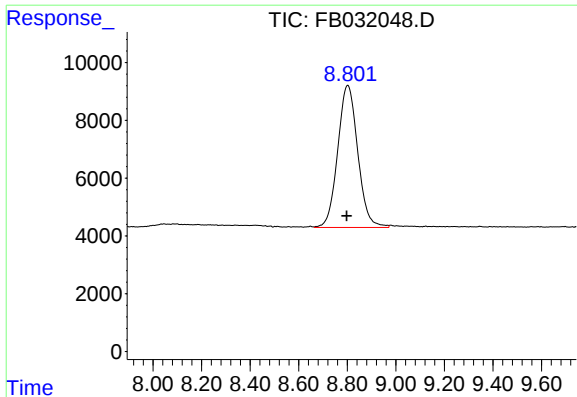

#5 AAA-TFT


R.T.: 8.803 min
Delta R.T.: 0.005 min
Response: 281701
Conc: 18.26 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-36

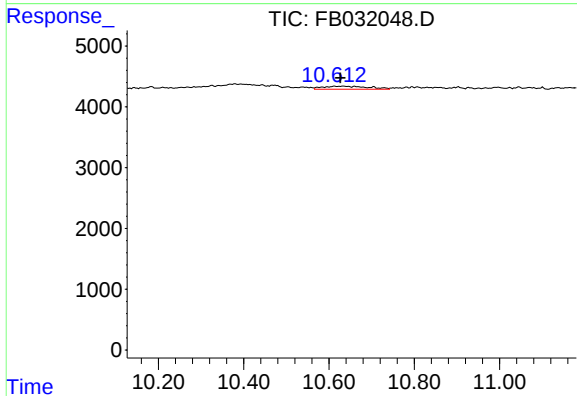


#6 Toluene

R.T.: 10.634 min
Delta R.T.: 0.008 min
Response: 3642
Conc: 0.10 ng/ml

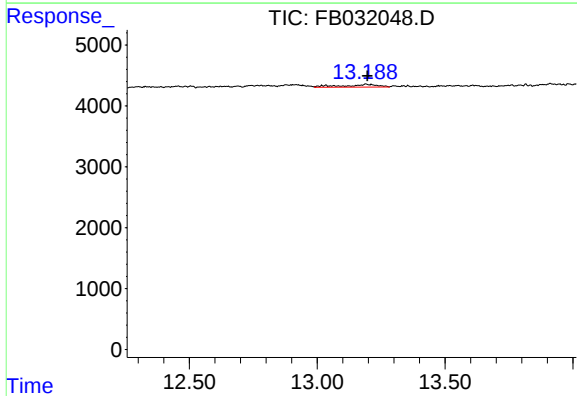


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: -0.004 min
Response: 4150
Conc: 0.13 ng/ml

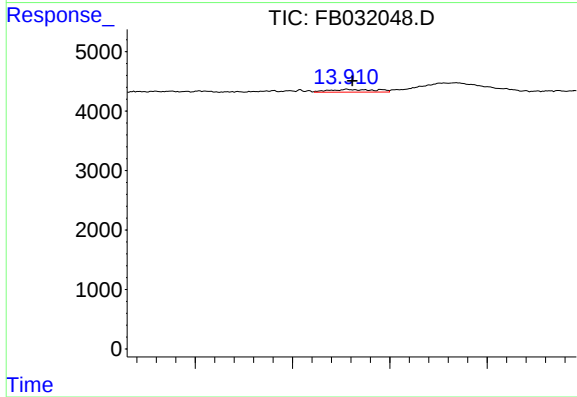

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.011 min
Response: 3010
Conc: 0.10 ng/ml

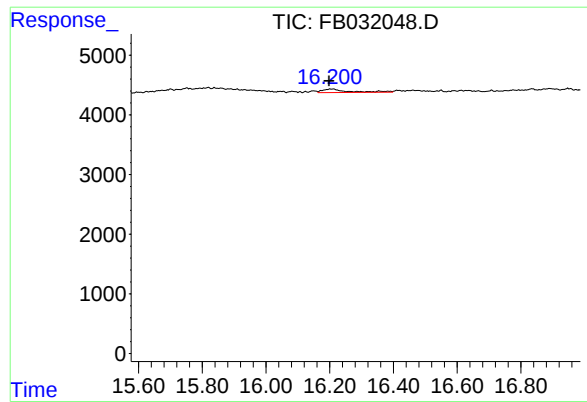

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.010 min
Response: 3240
Conc: 0.12 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-36