

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070925\
 Data File : FB032053.D
 Signal(s) : FID2B.CH
 Acq On : 9 Jul 2025 19:54
 Operator : YP/AJ
 Sample : Q2514-10
 Misc : 4.20G/5.00 ML DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TP-90

Integration File: SAMPLE.e
 Quant Time: Jul 10 01:24:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
 Quant Title :
 QLast Update : Mon Jun 23 13:56:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	278191	18.032 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	371	0.015 ng/ml
2) t 2,2,4-Trimethylpentane	7.465	841	0.031 ng/ml
3) t n-Heptane	7.731	813	0.033 ng/ml
6) t Toluene	10.636	2909	0.081 ng/ml
7) t Ethylbenzene	13.062	1620	0.051 ng/ml
8) t m-Xylene	13.177	2837	0.086 ng/ml
9) t O-Xylene	13.937	1647	0.053 ng/ml
10) t 1,2,4-Trimethylbenzene	16.222	2168	0.082 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070925\
Data File : FB032053.D
Signal(s) : FID2B.CH
Acq On : 9 Jul 2025 19:54
Operator : YP/AJ
Sample : Q2514-10
Misc : 4.20G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-90

Integration File: SAMPLE.e
Quant Time: Jul 10 01:24:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

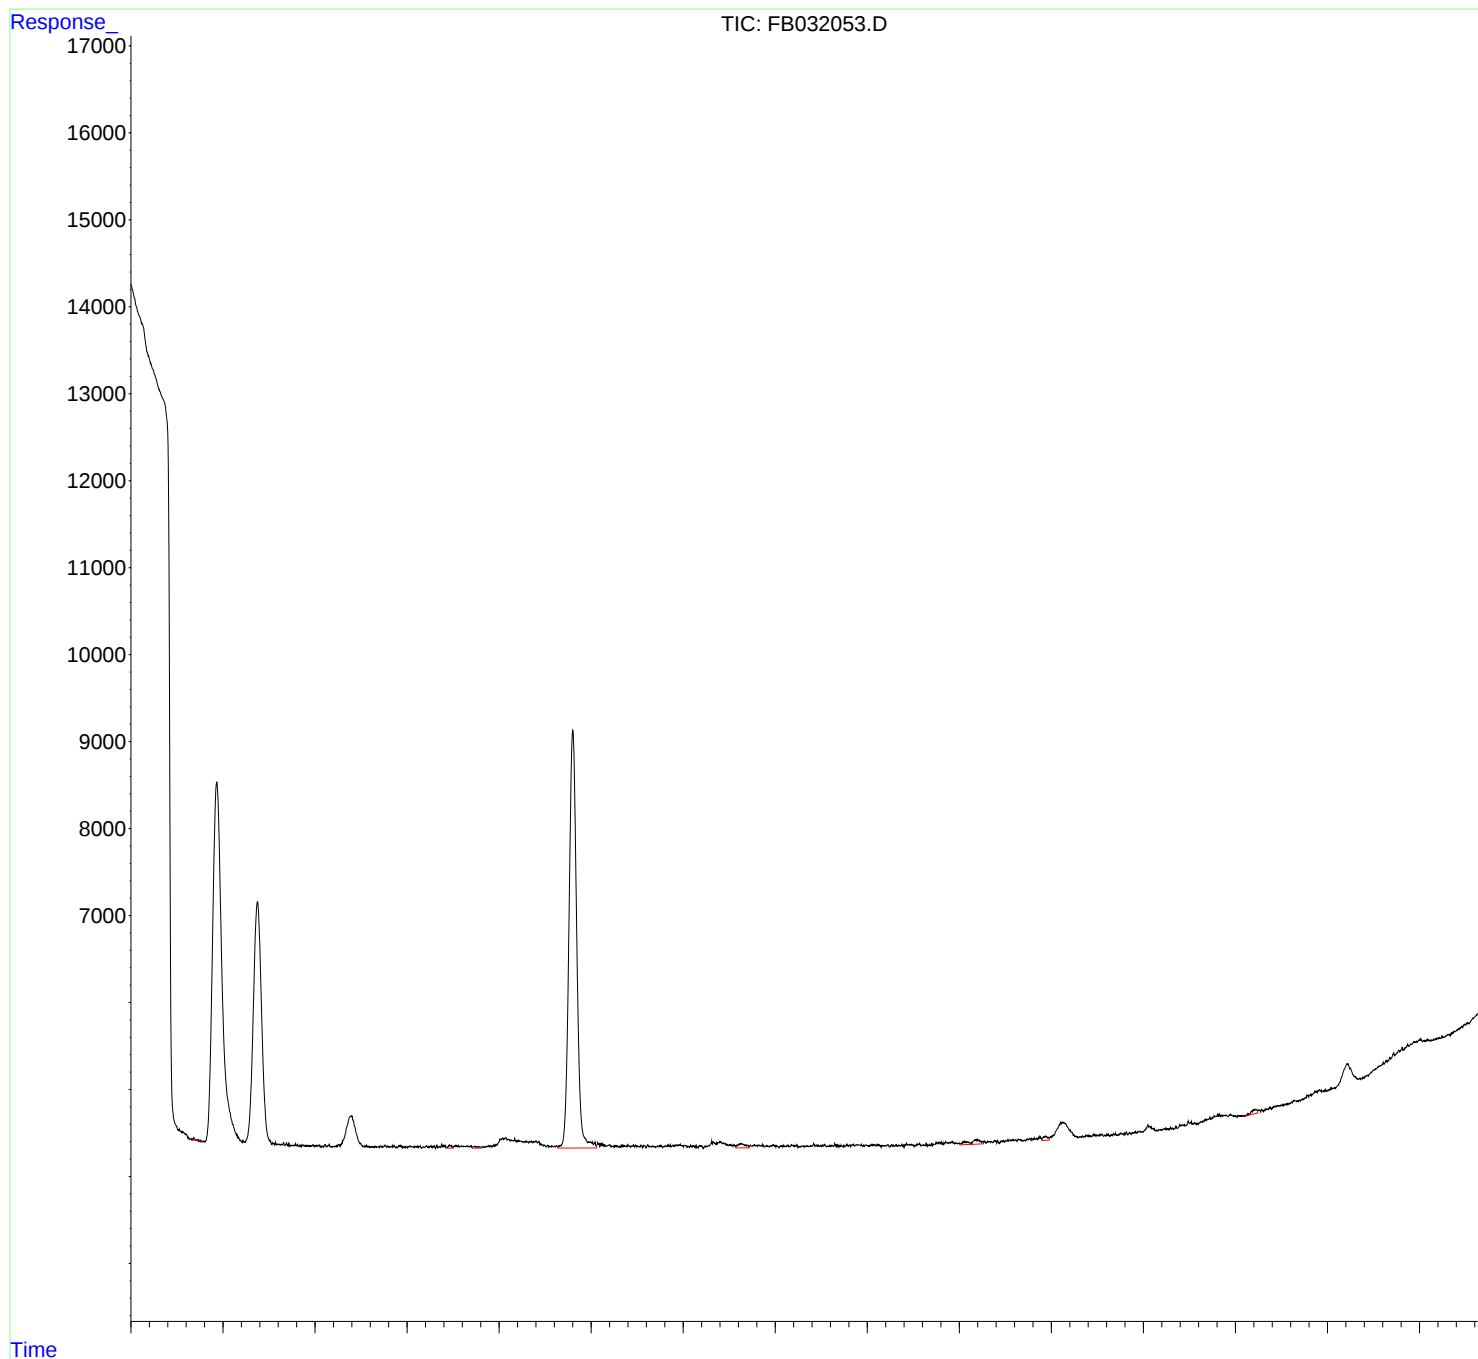


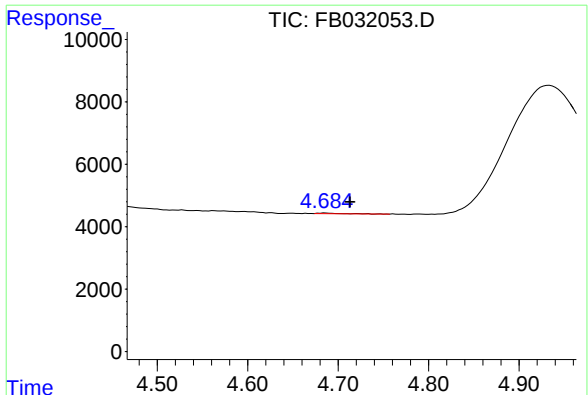

#1 2-Methylpentane


R.T.: 4.686 min
Delta R.T.: -0.027 min
Response: 371
Conc: 0.01 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-90

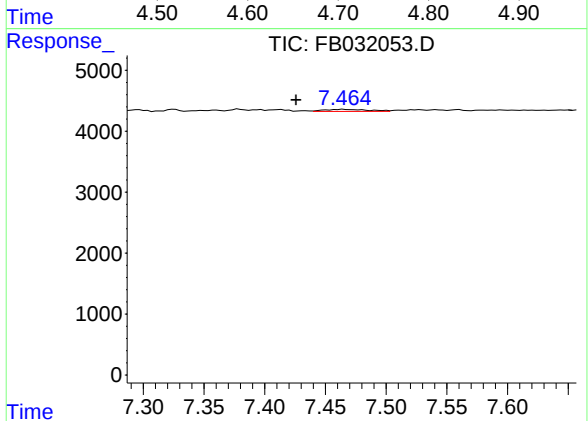


#2 2,2,4-Trimethylpentane

R.T.: 7.465 min
Delta R.T.: 0.040 min
Response: 841
Conc: 0.03 ng/ml

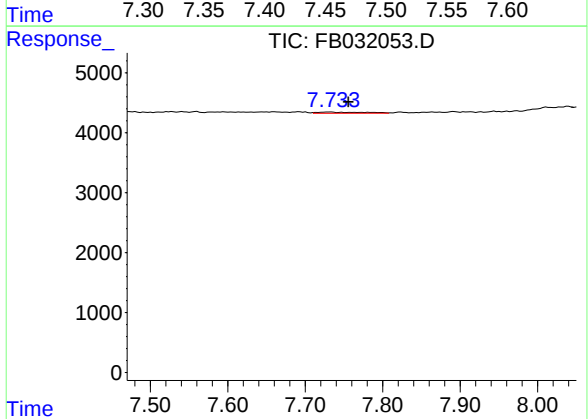


#3 n-Heptane

R.T.: 7.731 min
Delta R.T.: -0.025 min
Response: 813
Conc: 0.03 ng/ml

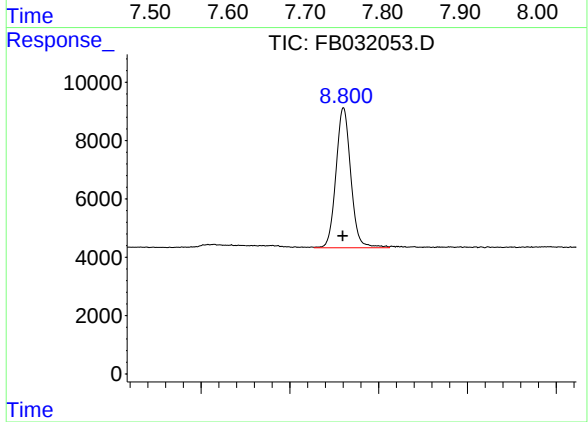

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.004 min
Response: 278191
Conc: 18.03 ng/ml

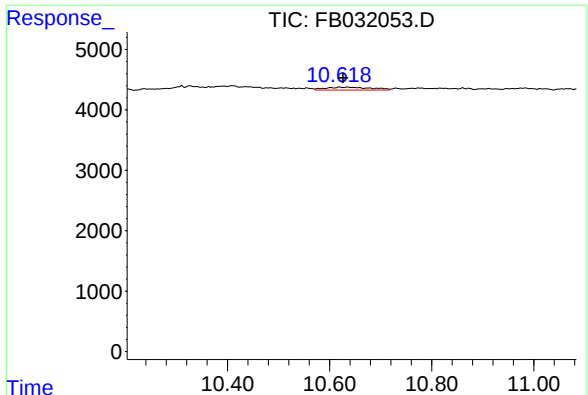

#6 Toluene


R.T.: 10.636 min
Delta R.T.: 0.009 min
Response: 2909
Conc: 0.08 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-90

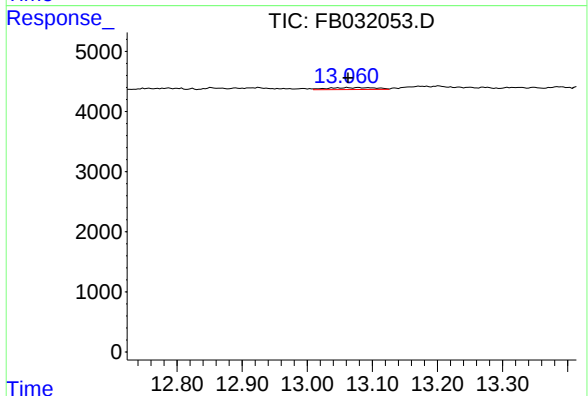


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: 0.000 min
Response: 1620
Conc: 0.05 ng/ml

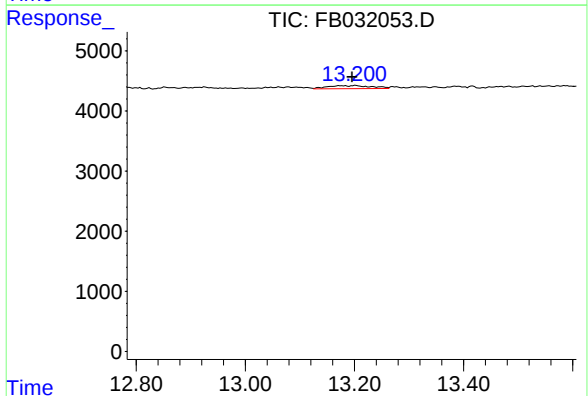


#8 m-Xylene

R.T.: 13.177 min
Delta R.T.: -0.019 min
Response: 2837
Conc: 0.09 ng/ml

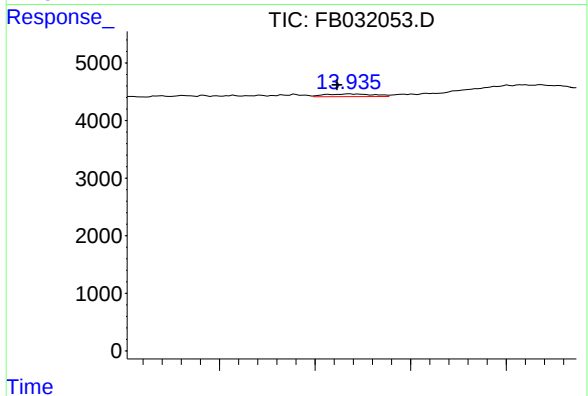

#9 O-Xylene

R.T.: 13.937 min
Delta R.T.: 0.015 min
Response: 1647
Conc: 0.05 ng/ml

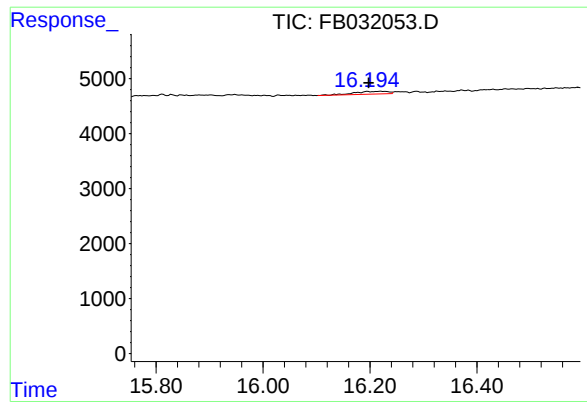

#10 1,2,4-Trimethylbenzene

R.T.: 16.222 min
Delta R.T.: 0.024 min
Response: 2168
Conc: 0.08 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-90