

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071019\
 Data File : FB021659.D
 Signal(s) : FID2B.CH
 Acq On : 10 Jul 2019 9:47
 Operator : MJ/SJ
 Sample : BSF0710S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 11 01:45:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.993	283552	20.508 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.865	953049	27.918 ng/ml
2) t 2,2,4-Trimethylpentane	7.613	929639	30.083 ng/ml
3) t n-Heptane	7.952	290835	9.937 ng/ml
4) t Benzene	8.087	337057	10.042 ng/ml
6) t Toluene	10.834	693432	30.357 ng/ml
7) t Ethylbenzene	13.279	233648	9.870 ng/ml
8) t m-Xylene	13.412	500284	19.738 ng/ml
9) t O-Xylene	14.141	524382	19.994 ng/ml
10) t 1,2,4-Trimethylbenzene	16.420	540694	20.579 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071019\
Data File : FB021659.D
Signal(s) : FID2B.CH
Acq On : 10 Jul 2019 9:47
Operator : MJ/SJ
Sample : BSF0710S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 11 01:45:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

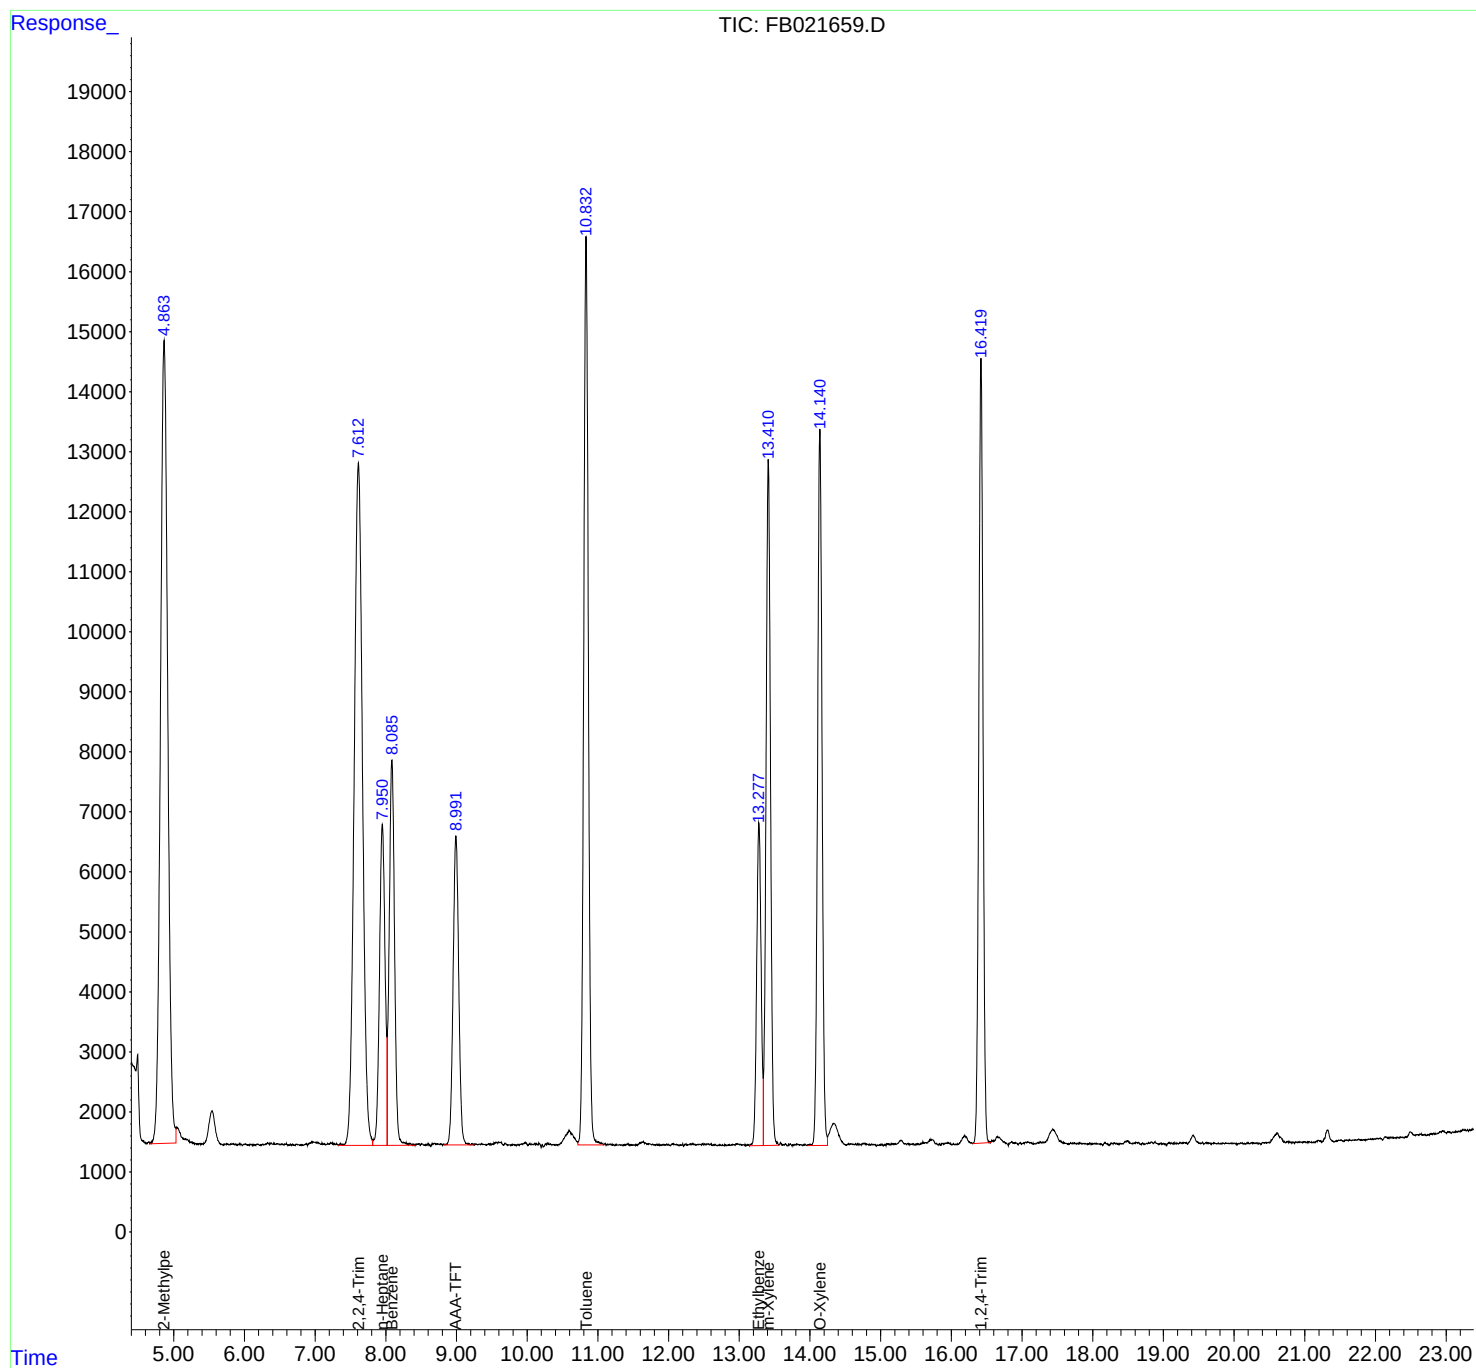

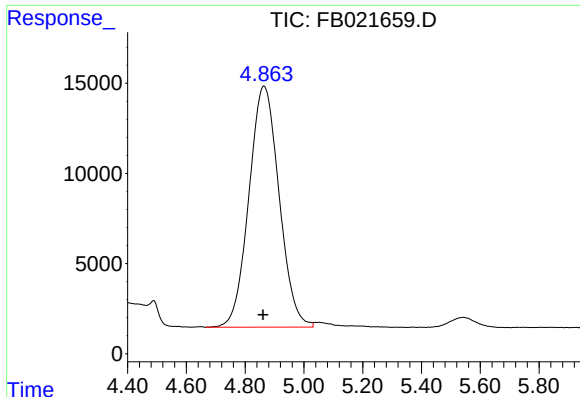


#1 2-Methylpentane

R.T.: 4.865 min
Delta R.T.: 0.004 min
Response: 953049
Conc: 27.92 ng/ml

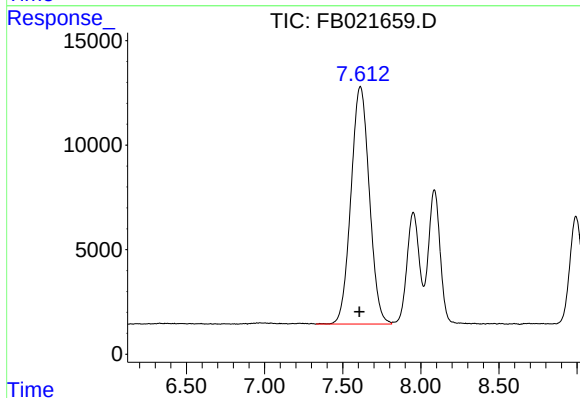


#2 2,2,4-Trimethylpentane

R.T.: 7.613 min
Delta R.T.: 0.005 min
Response: 929639
Conc: 30.08 ng/ml

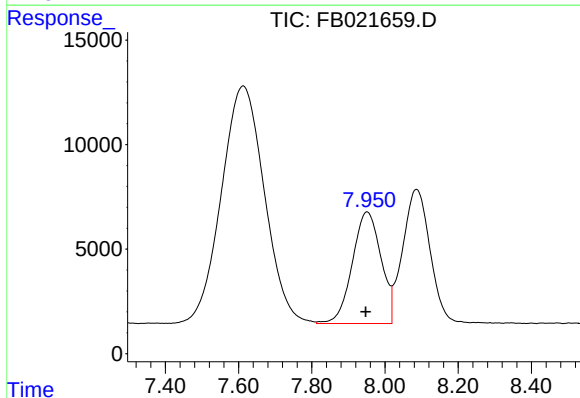


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: 0.004 min
Response: 290835
Conc: 9.94 ng/ml

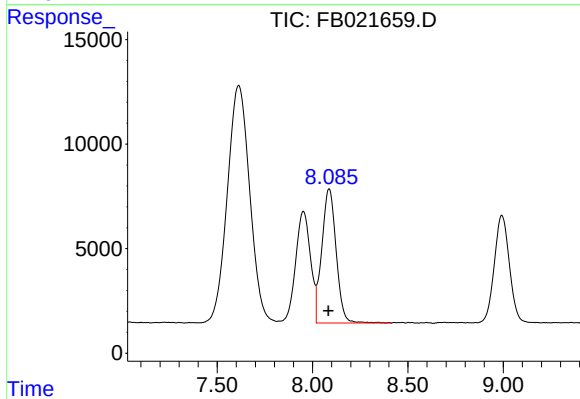


#4 Benzene

R.T.: 8.087 min
Delta R.T.: 0.005 min
Response: 337057
Conc: 10.04 ng/ml

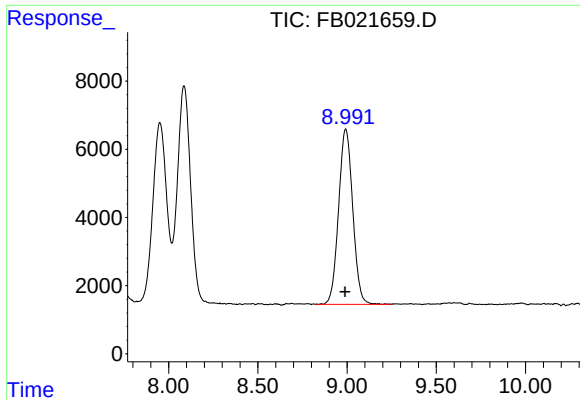


#5 AAA-TFT

R.T.: 8.993 min
 Delta R.T.: 0.004 min
 Response: 283552
 Conc: 20.51 ng/ml

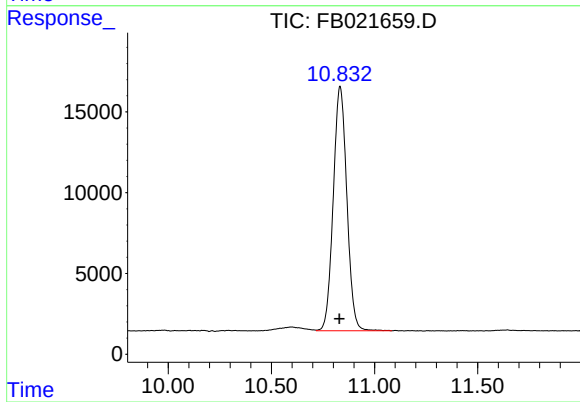


#6 Toluene

R.T.: 10.834 min
 Delta R.T.: 0.004 min
 Response: 693432
 Conc: 30.36 ng/ml

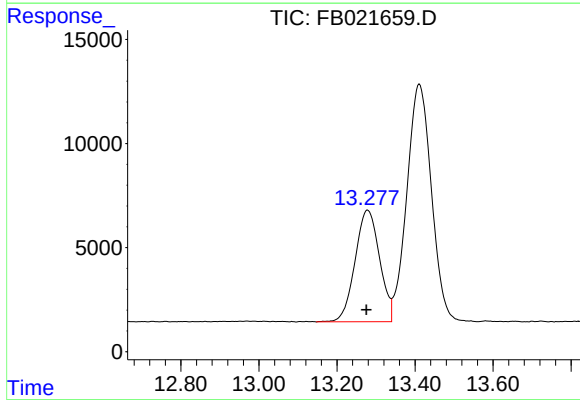


#7 Ethylbenzene

R.T.: 13.279 min
 Delta R.T.: 0.004 min
 Response: 233648
 Conc: 9.87 ng/ml

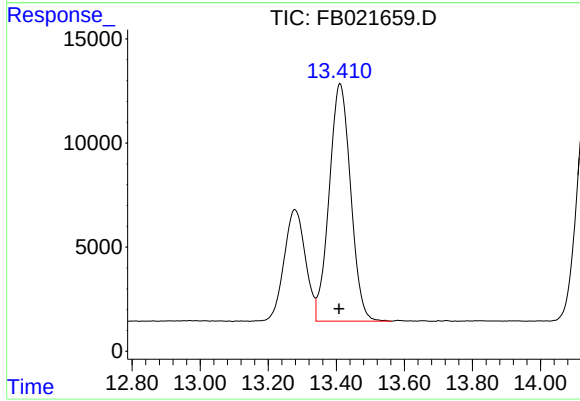

#8 m-Xylene

R.T.: 13.412 min
 Delta R.T.: 0.004 min
 Response: 500284
 Conc: 19.74 ng/ml

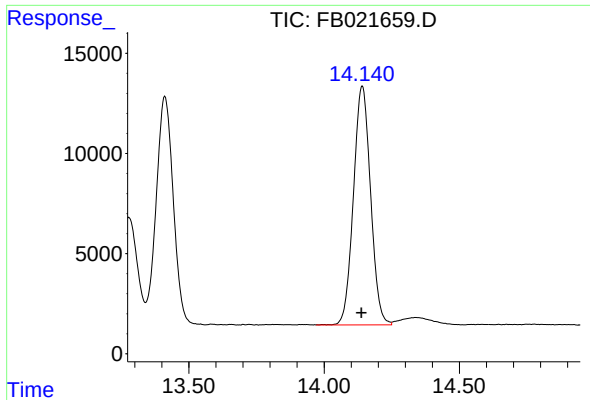


#9 O-Xylene

R.T.: 14.141 min

Delta R.T.: 0.004 min

Response: 524382

Conc: 19.99 ng/ml

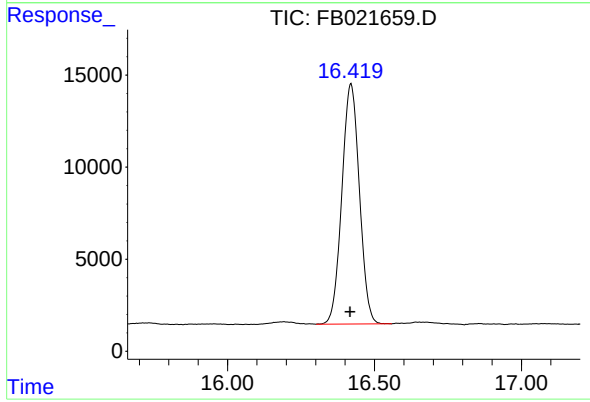

#10 1,2,4-Trimethylbenzene

R.T.: 16.420 min

Delta R.T.: 0.003 min

Response: 540694

Conc: 20.58 ng/ml