

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071020\
 Data File : FB024582.D
 Signal(s) : FID2B.CH
 Acq On : 10 Jul 2020 12:13
 Operator : DD/AJ
 Sample : L3216-03
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 11 00:03:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
 Quant Title :
 QLast Update : Thu Jul 09 10:49:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	425929	18.490 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.692	58770	1.986 ng/ml
2) t 2,2,4-Trimethylpentane	7.407	51448	1.643 ng/mlm
3) t n-Heptane	7.761	14999	0.482 ng/ml
4) t Benzene	7.896	18494	0.485 ng/ml
6) t Toluene	10.632	61772	1.689 ng/ml
7) t Ethylbenzene	13.073	20278	0.594 ng/ml
8) t m-Xylene	13.205	40836	1.210 ng/ml
9) t O-Xylene	13.933	38960	1.185 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	30640	1.136 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071020\
Data File : FB024582.D
Signal(s) : FID2B.CH
Acq On : 10 Jul 2020 12:13
Operator : DD/AJ
Sample : L3216-03
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 11 00:03:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

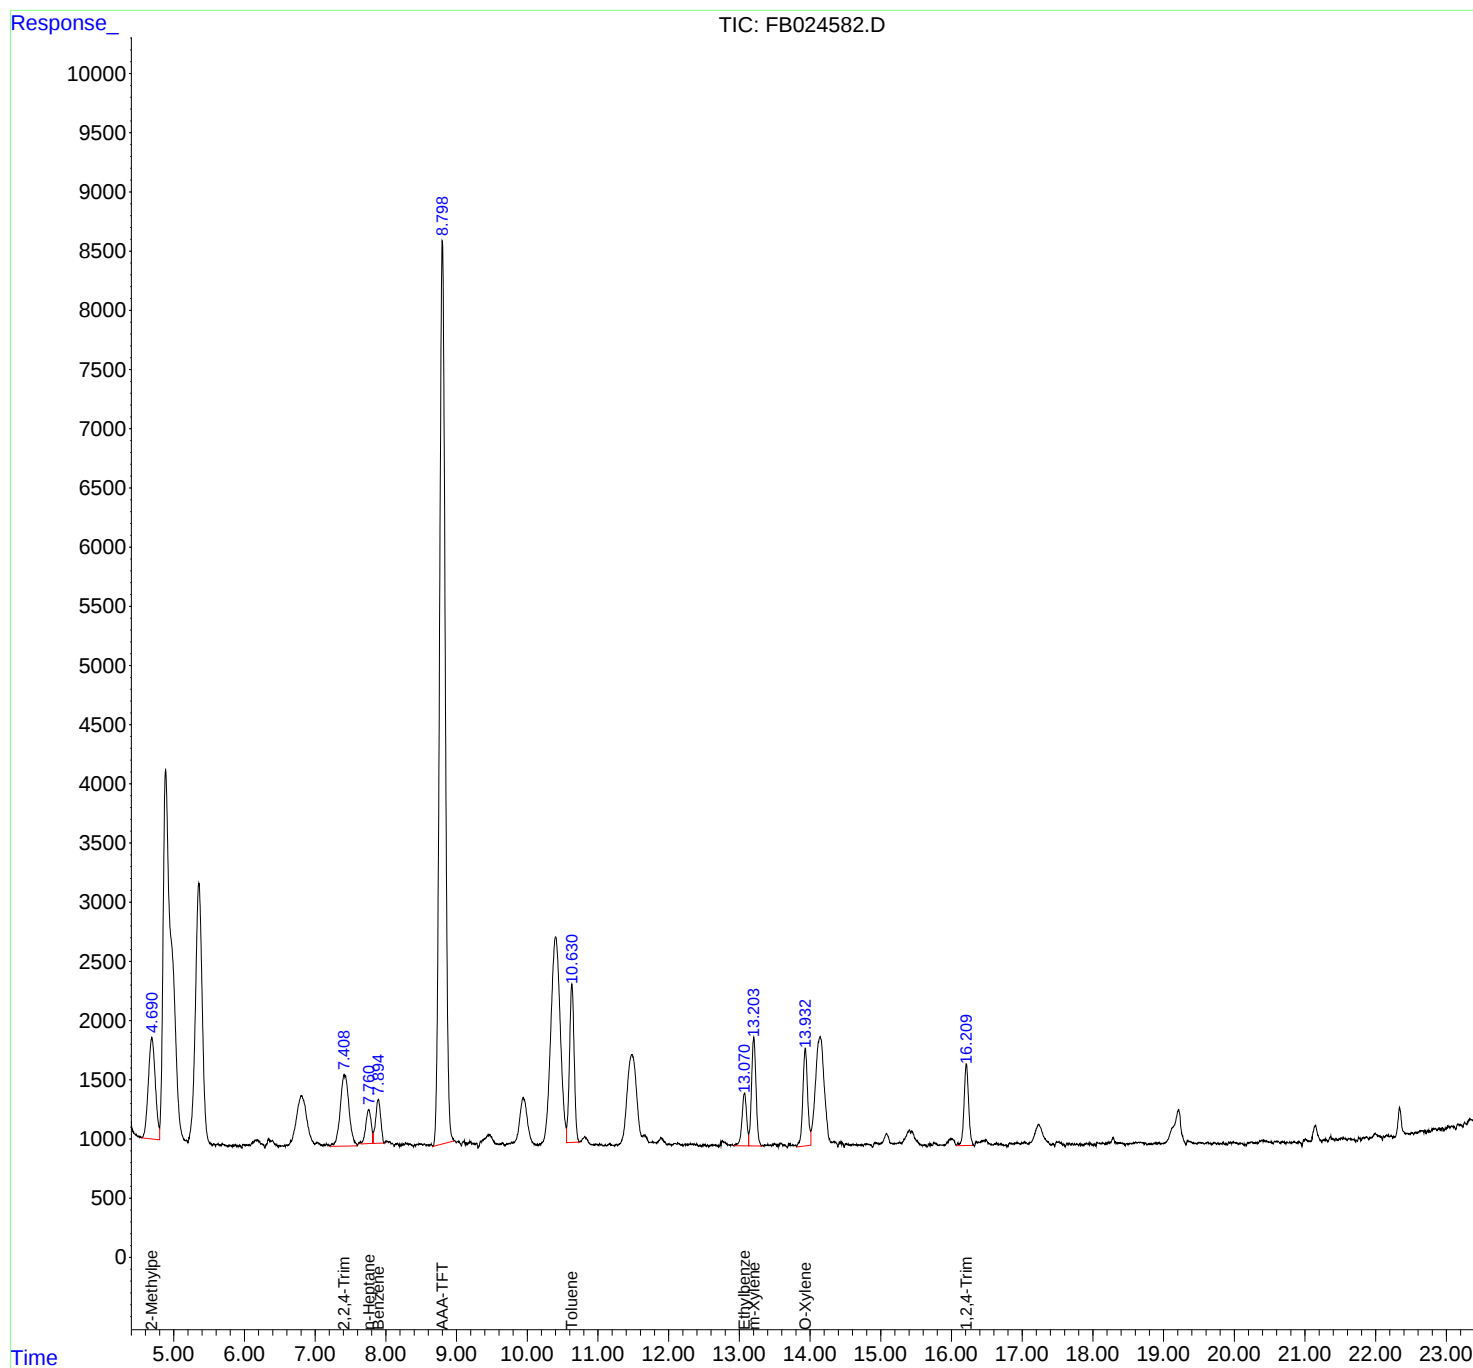

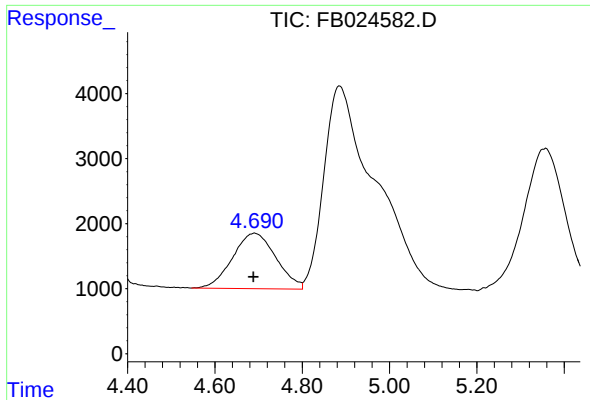


#1 2-Methylpentane

R.T.: 4.692 min
Delta R.T.: 0.004 min
Response: 58770
Conc: 1.99 ng/ml

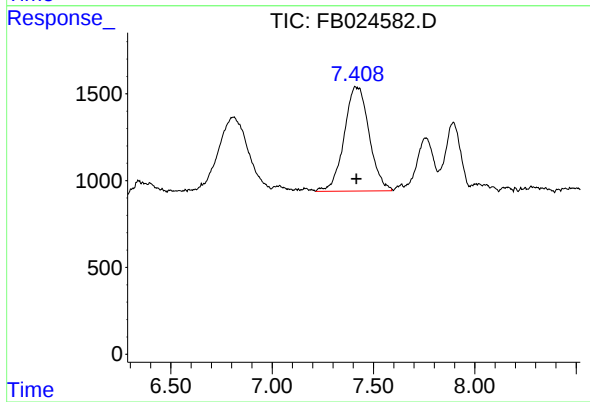


#2 2,2,4-Trimethylpentane

R.T.: 7.407 min
Delta R.T.: -0.009 min
Response: 51448
Conc: 1.64 ng/ml m

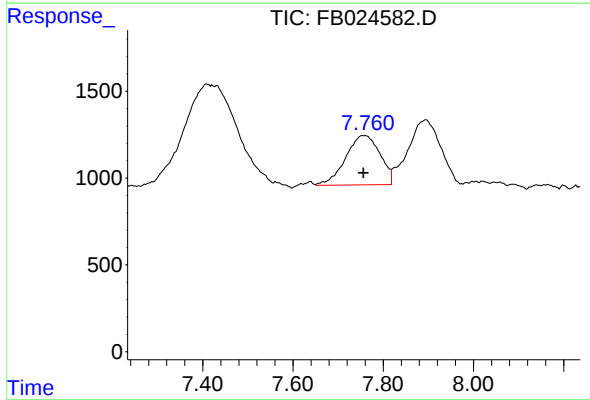


#3 n-Heptane

R.T.: 7.761 min
Delta R.T.: 0.006 min
Response: 14999
Conc: 0.48 ng/ml

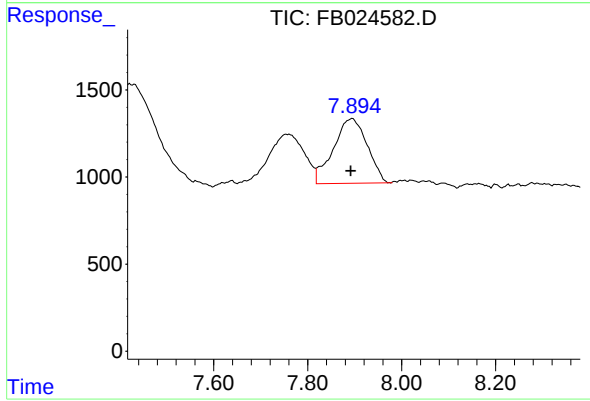


#4 Benzene

R.T.: 7.896 min
Delta R.T.: 0.004 min
Response: 18494
Conc: 0.49 ng/ml

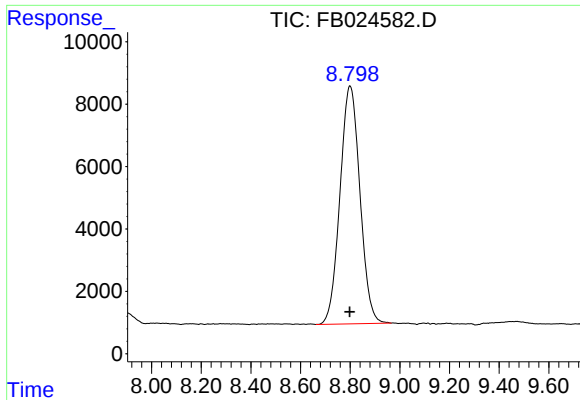


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.002 min
Response: 425929
Conc: 18.49 ng/ml

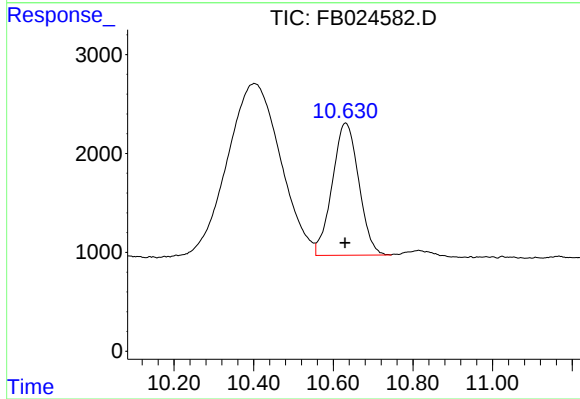


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.003 min
Response: 61772
Conc: 1.69 ng/ml

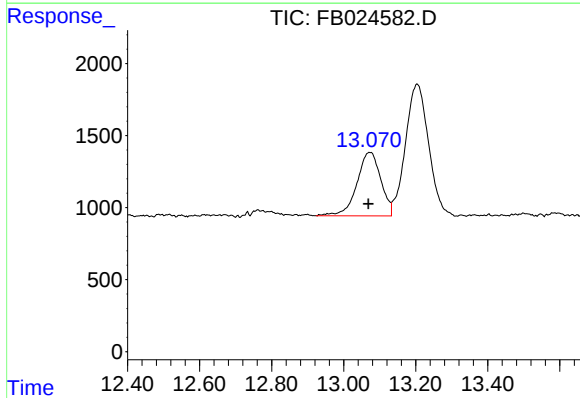


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.005 min
Response: 20278
Conc: 0.59 ng/ml

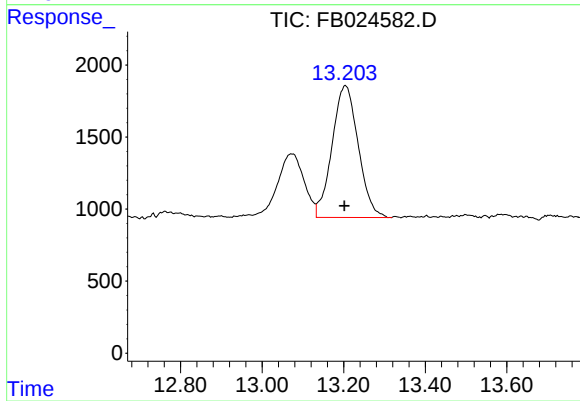


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.003 min
Response: 40836
Conc: 1.21 ng/ml

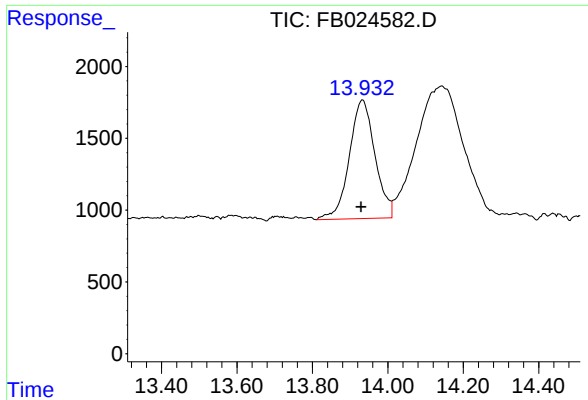

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.004 min
Response: 38960
Conc: 1.19 ng/ml

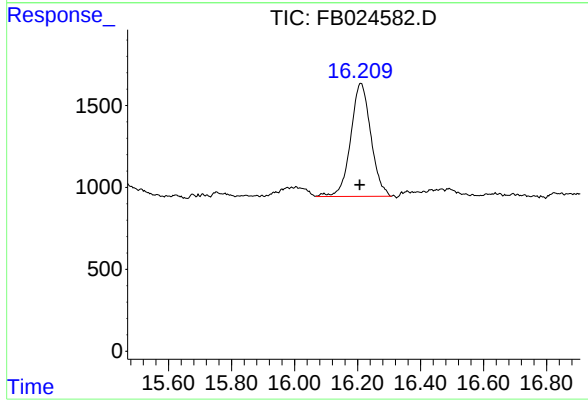

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.004 min
Response: 30640
Conc: 1.14 ng/ml