

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071122\
 Data File : FB027651.D
 Signal(s) : FID2B.CH
 Acq On : 11 Jul 2022 14:42
 Operator : AJ/MA
 Sample : 100 GRO STD
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 100 GRO STD

Integration File: Calibration.e
 Quant Time: Jul 11 14:57:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
 Quant Title :
 QLast Update : Mon Jul 11 14:21:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	1123557	95.711 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	2897564	134.800 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	2958667	140.832 ng/ml
3) t n-Heptane	7.747	1033596	50.345 ng/ml
4) t Benzene	7.884	1182224	50.474 ng/ml
6) t Toluene	10.619	3357853	150.468 ng/ml
7) t Ethylbenzene	13.056	1021663	48.456 ng/ml
8) t m-Xylene	13.188	2014241	95.295 ng/ml
9) t O-Xylene	13.916	1930623	93.036 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	1850215	86.655 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071122\
Data File : FB027651.D
Signal(s) : FID2B.CH
Acq On : 11 Jul 2022 14:42
Operator : AJ/MA
Sample : 100 GRO STD
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
100 GRO STD

Integration File: Calibration.e
Quant Time: Jul 11 14:57:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071122.M
Quant Title :
QLast Update : Mon Jul 11 14:21:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

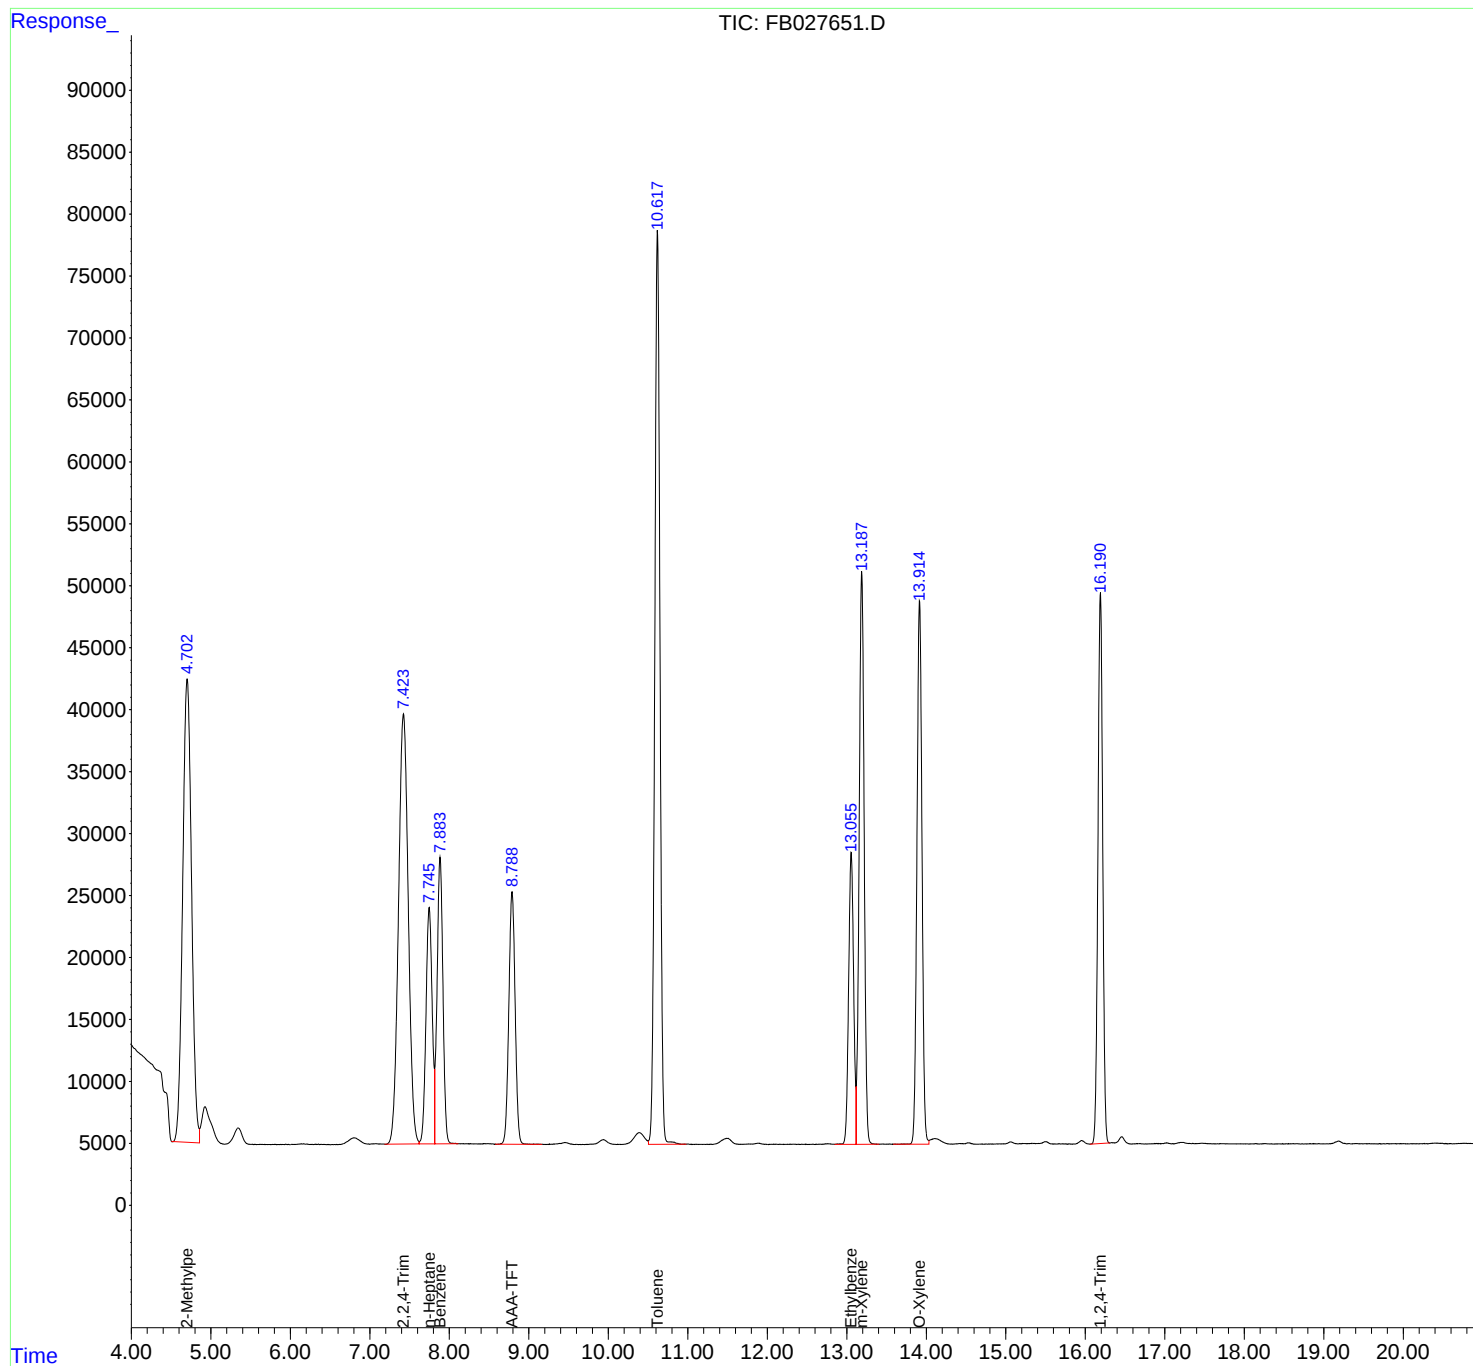


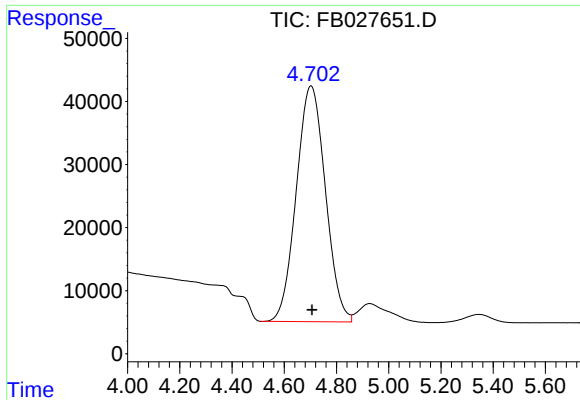

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: -0.004 min
Response: 2897564
Conc: 134.80 ng/ml

Instrument :
FID_B
ClientSampleId :
100 GRO STD

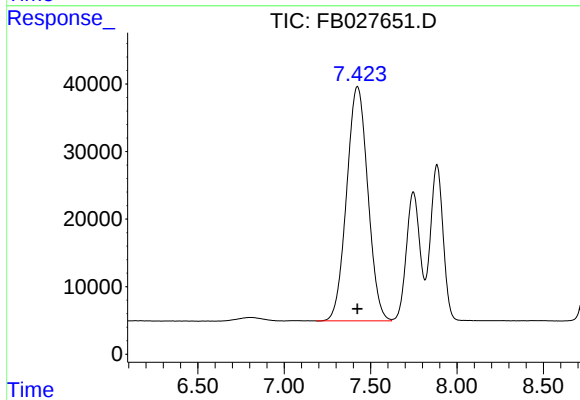


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 2958667
Conc: 140.83 ng/ml

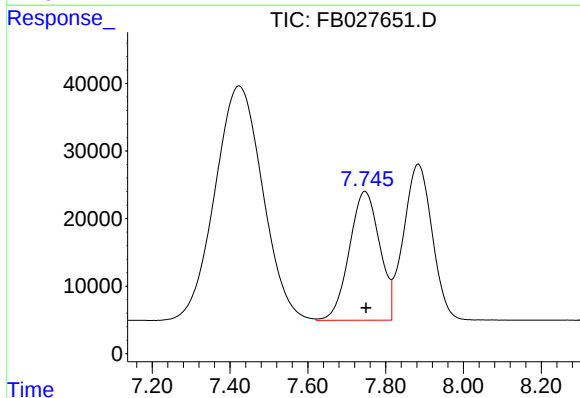


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.003 min
Response: 1033596
Conc: 50.34 ng/ml

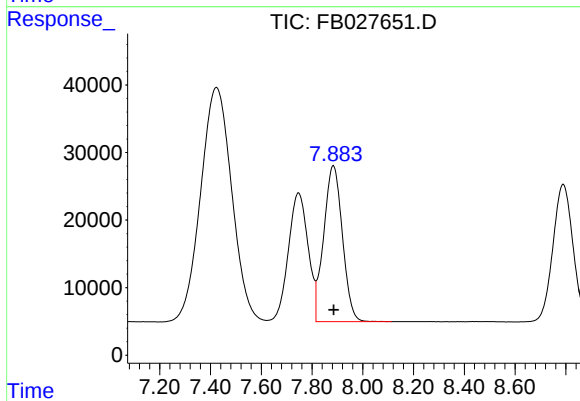

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.002 min
Response: 1182224
Conc: 50.47 ng/ml

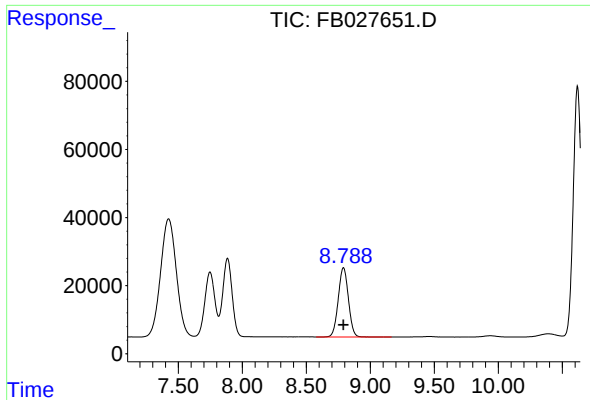

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 1123557
Conc: 95.71 ng/ml

Instrument :
FID_B
ClientSampleId :
100 GRO STD

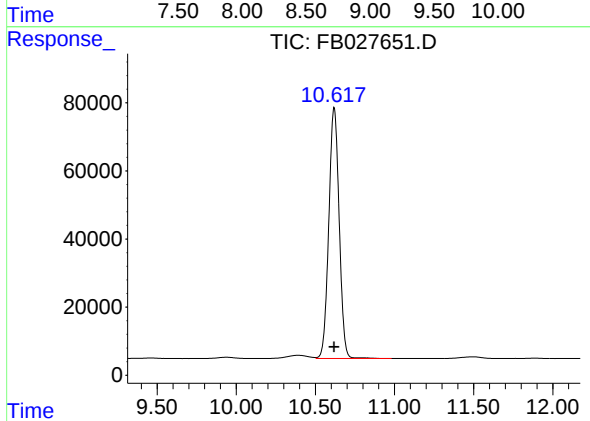


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.000 min
Response: 3357853
Conc: 150.47 ng/ml

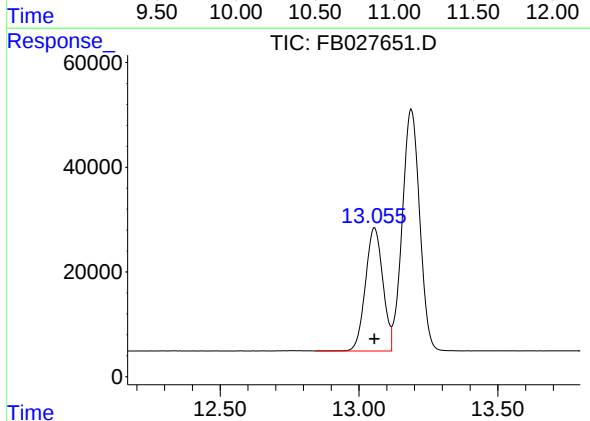


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 1021663
Conc: 48.46 ng/ml

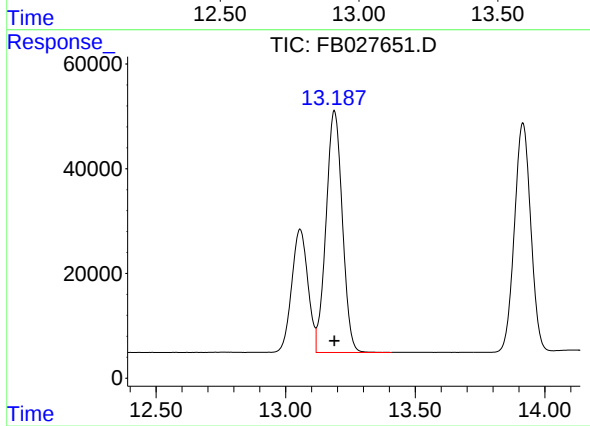

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: 0.000 min
Response: 2014241
Conc: 95.30 ng/ml

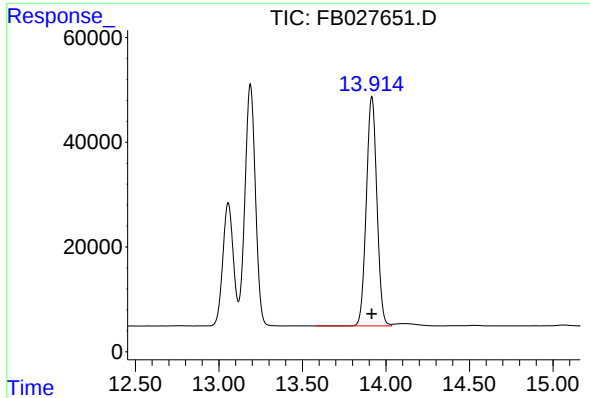

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 1930623
Conc: 93.04 ng/ml

Instrument :
FID_B
ClientSampleId :
100 GRO STD

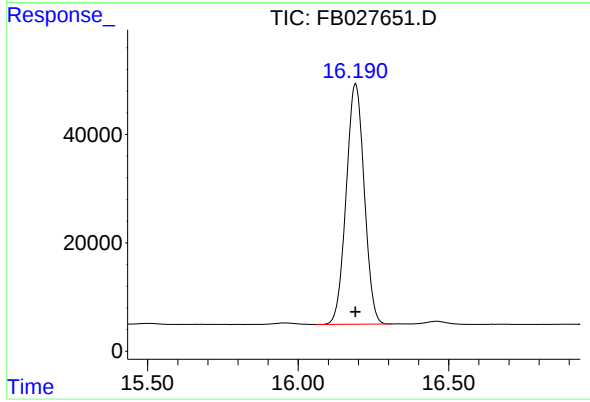

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 1850215
Conc: 86.66 ng/ml