

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071123\
 Data File : FB030153.D
 Signal(s) : FID2B.CH
 Acq On : 11 Jul 2023 13:17
 Operator : YP/AJ
 Sample : 03572-01
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jul 12 03:10:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
 Quant Title :
 QLast Update : Mon Jun 26 14:31:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	254373	19.357 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	48586	2.584 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	51530	2.451 ng/ml
3) t n-Heptane	7.750	17863	0.875 ng/ml
4) t Benzene	7.891	20477	0.836 ng/ml
6) t Toluene	10.620	61750	2.602 ng/ml
7) t Ethylbenzene	13.056	18704	0.831 ng/ml
8) t m-Xylene	13.189	39498	1.737 ng/ml
9) t O-Xylene	13.913	40975	1.807 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	43721	1.912 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071123\
Data File : FB030153.D
Signal(s) : FID2B.CH
Acq On : 11 Jul 2023 13:17
Operator : YP/AJ
Sample : 03572-01
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 12 03:10:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
Quant Title :
QLast Update : Mon Jun 26 14:31:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

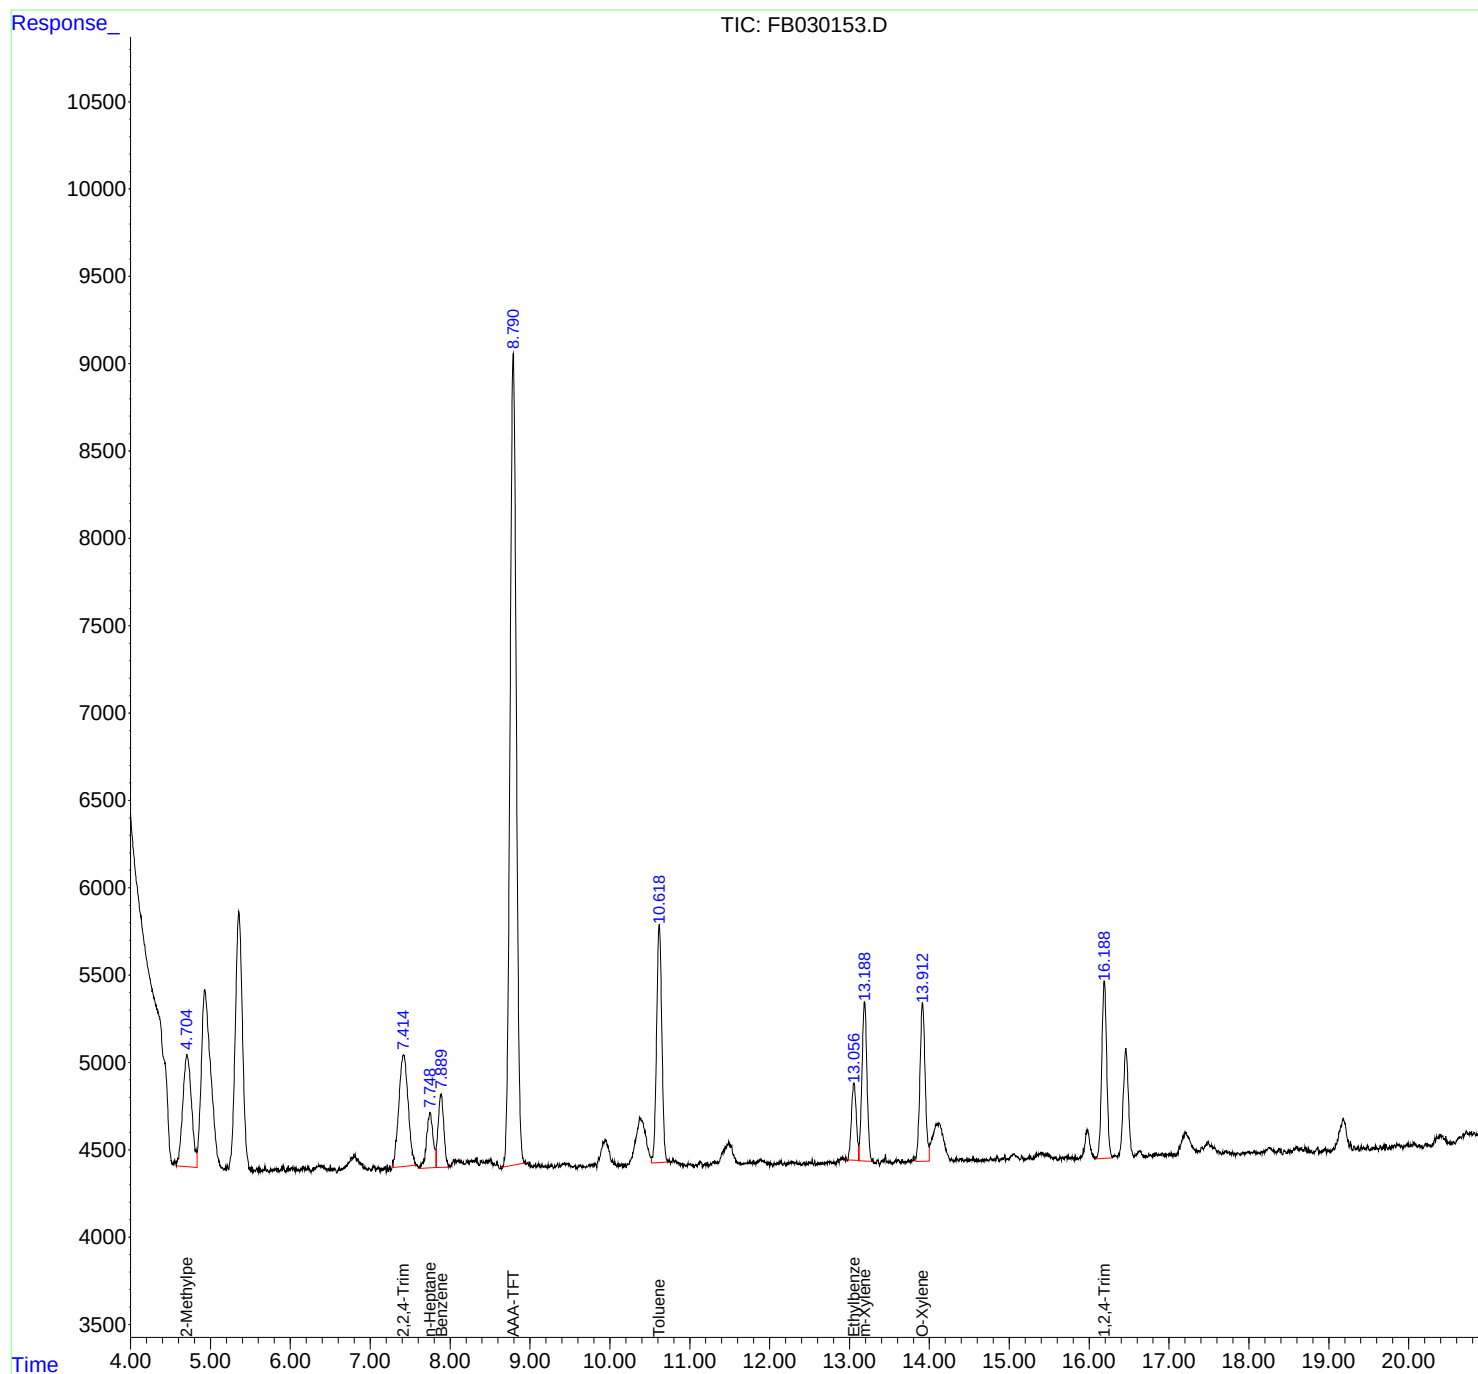


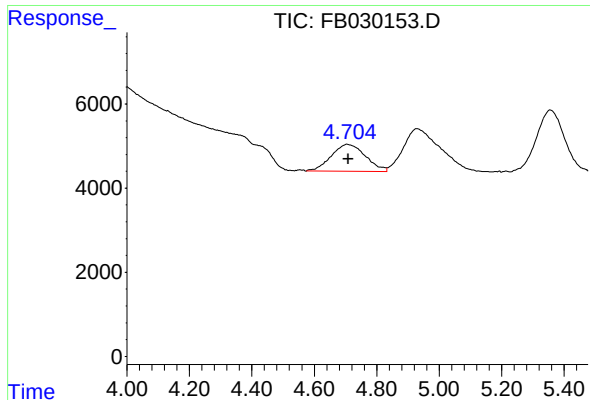

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: -0.003 min
Response: 48586
Conc: 2.58 ng/ml

Instrument :
FID_B
ClientSampleId :

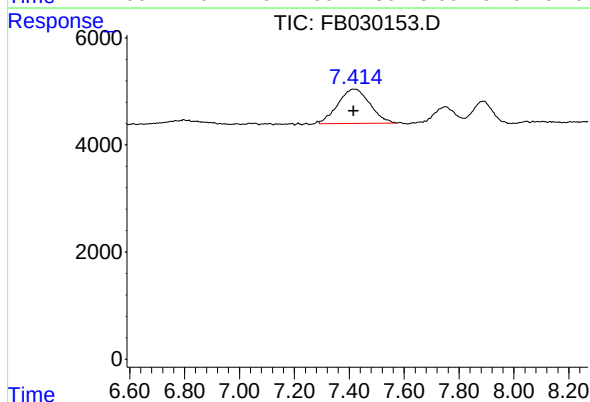


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 51530
Conc: 2.45 ng/ml

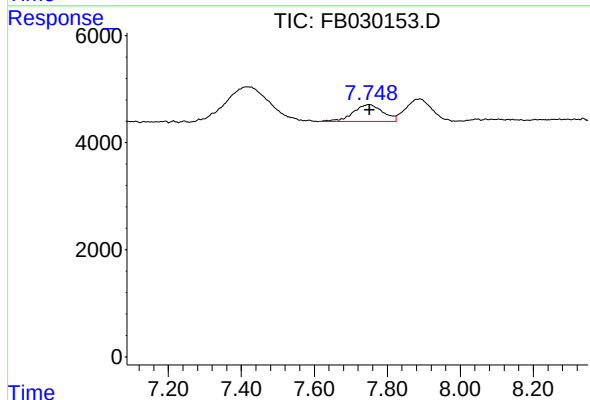


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.001 min
Response: 17863
Conc: 0.88 ng/ml

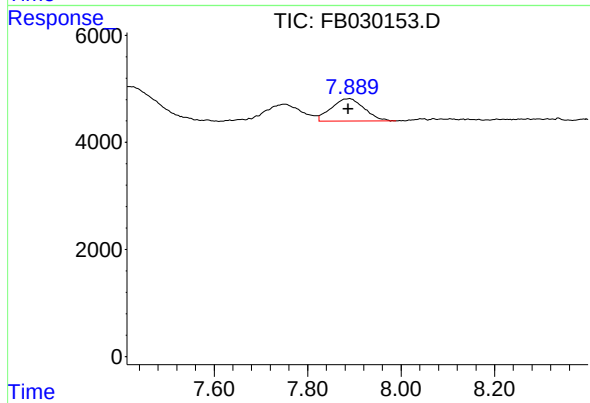

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.004 min
Response: 20477
Conc: 0.84 ng/ml

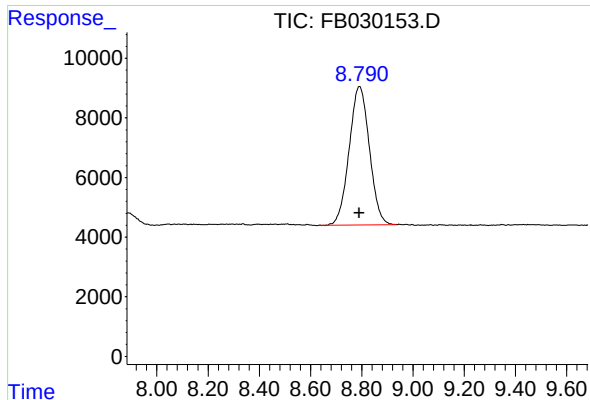

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 254373
Conc: 19.36 ng/ml

Instrument :
FID_B
ClientSampleId :

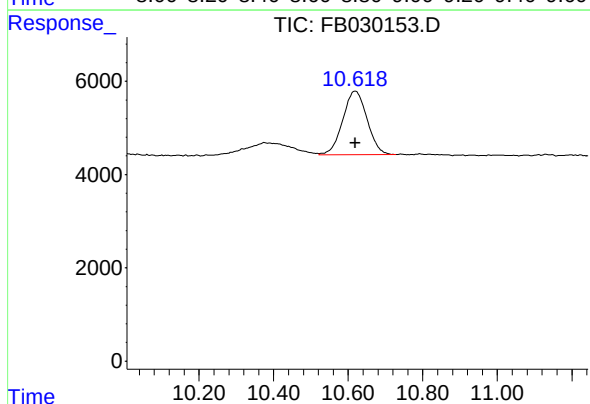


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.000 min
Response: 61750
Conc: 2.60 ng/ml

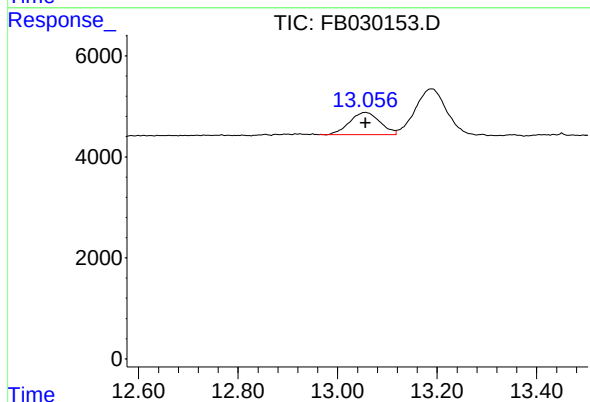


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 18704
Conc: 0.83 ng/ml

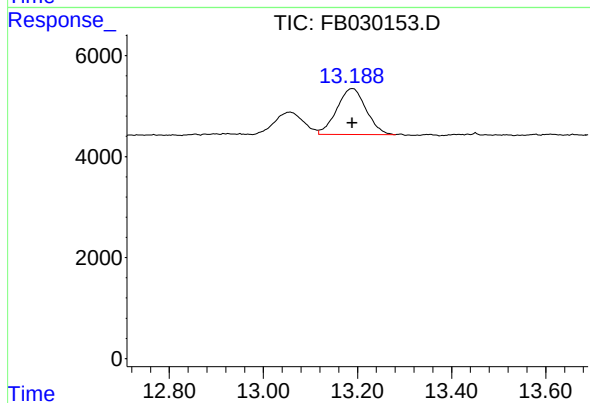

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 39498
Conc: 1.74 ng/ml

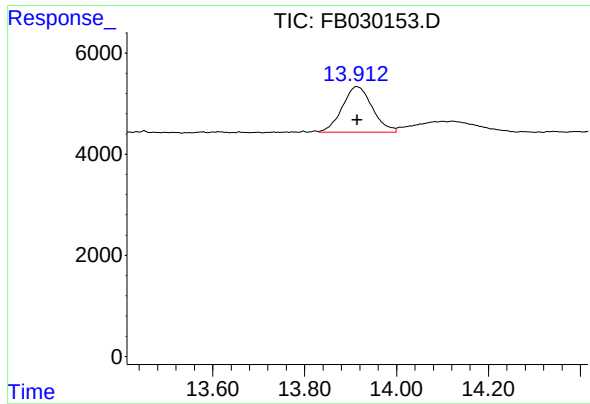

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.002 min
Response: 40975
Conc: 1.81 ng/ml

Instrument :
FID_B
ClientSampleId :

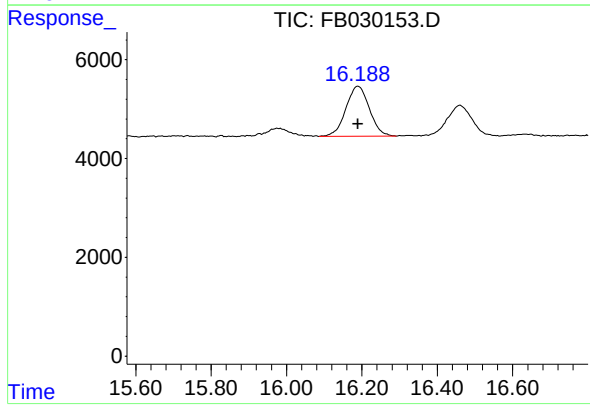

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: 0.000 min
Response: 43721
Conc: 1.91 ng/ml