

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071123\
 Data File : FB030155.D
 Signal(s) : FID2B.CH
 Acq On : 11 Jul 2023 14:34
 Operator : YP/AJ
 Sample : 03572-02
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jul 12 03:10:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
 Quant Title :
 QLast Update : Mon Jun 26 14:31:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	279185	21.245 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	138555	7.370 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	157873	7.508 ng/ml
3) t n-Heptane	7.751	53572	2.625 ng/ml
4) t Benzene	7.888	64762	2.643 ng/ml
6) t Toluene	10.620	183426	7.730 ng/ml
7) t Ethylbenzene	13.056	57403	2.551 ng/ml
8) t m-Xylene	13.190	113228	4.979 ng/ml
9) t O-Xylene	13.916	112078	4.943 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	108664	4.751 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071123\
Data File : FB030155.D
Signal(s) : FID2B.CH
Acq On : 11 Jul 2023 14:34
Operator : YP/AJ
Sample : 03572-02
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 12 03:10:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
Quant Title :
QLast Update : Mon Jun 26 14:31:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

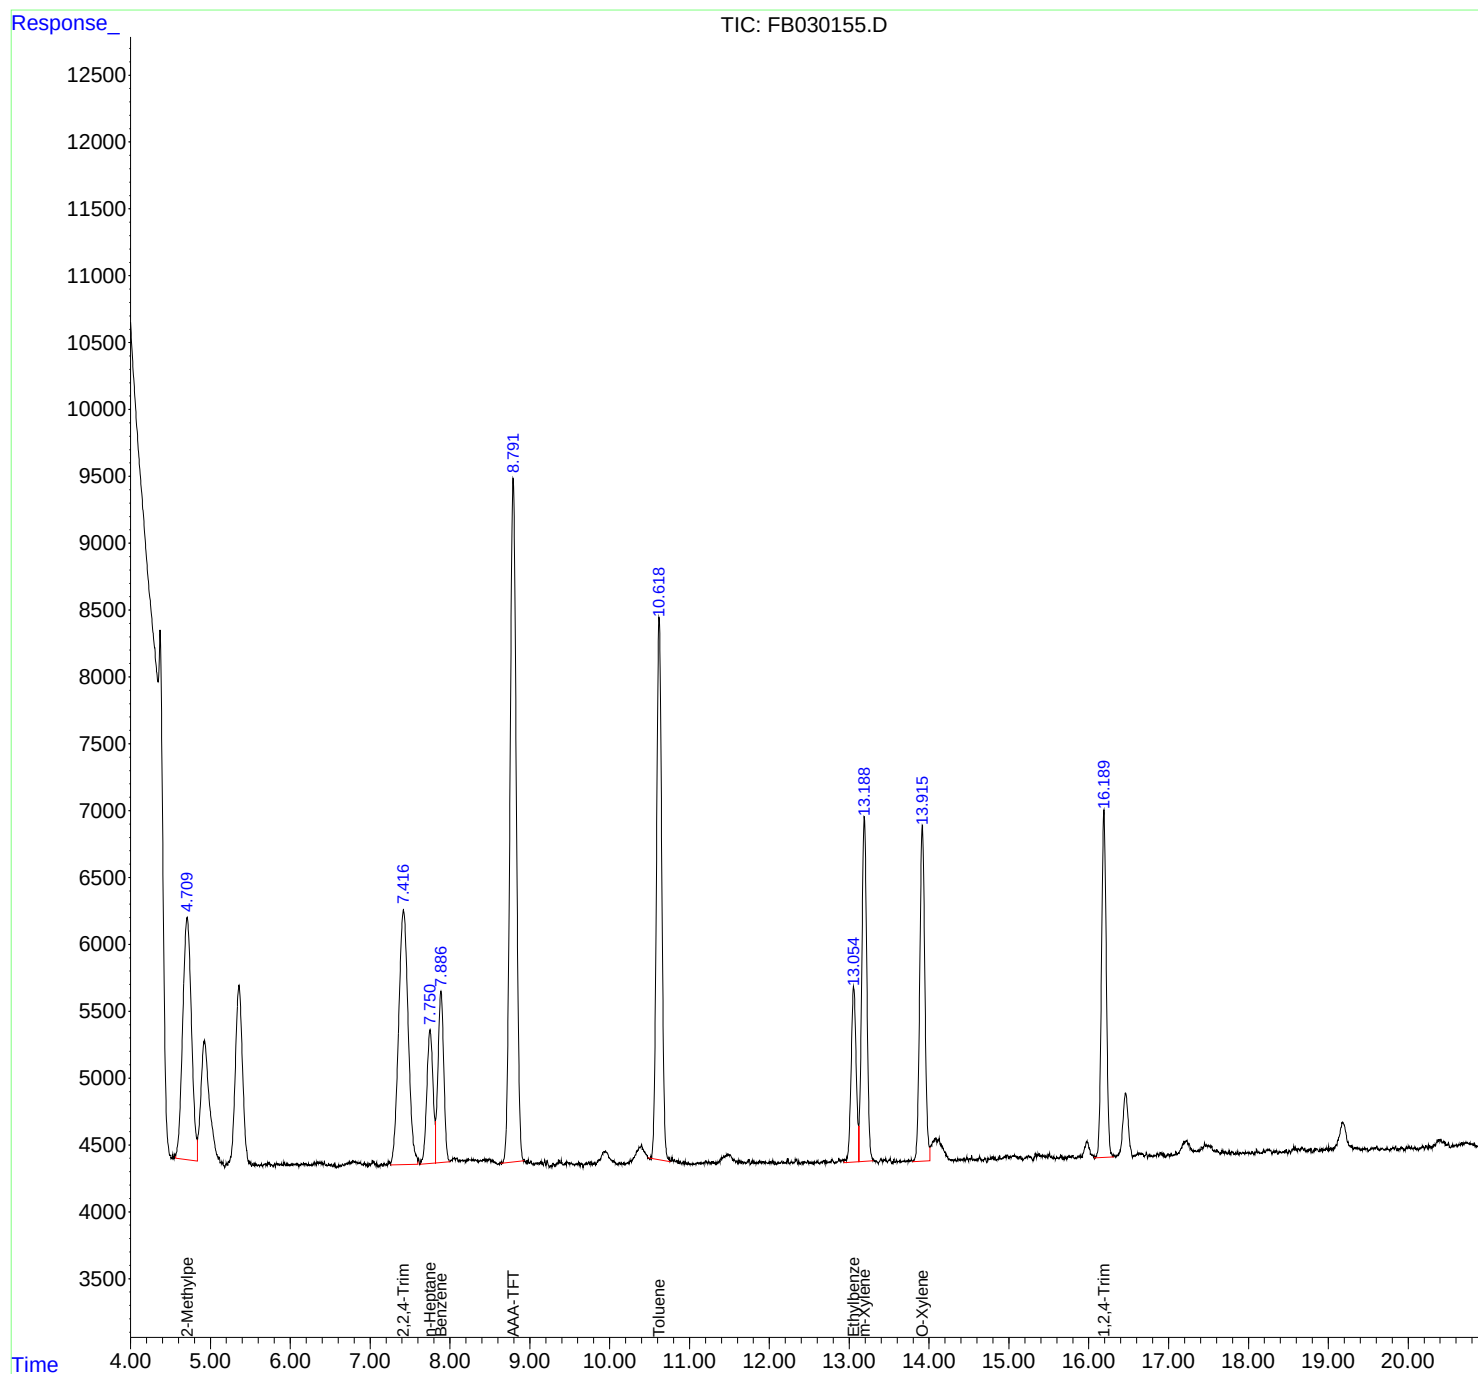


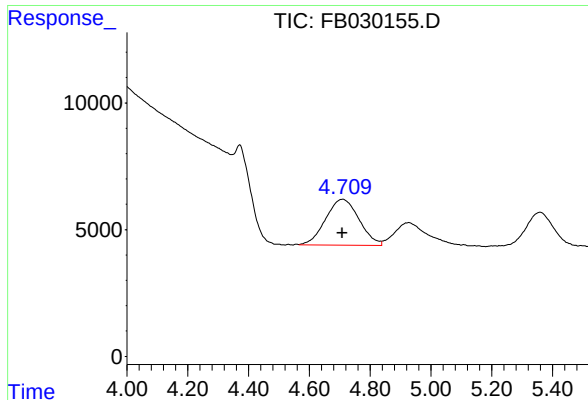

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.001 min
Response: 138555
Conc: 7.37 ng/ml

Instrument :
FID_B
ClientSampleId :

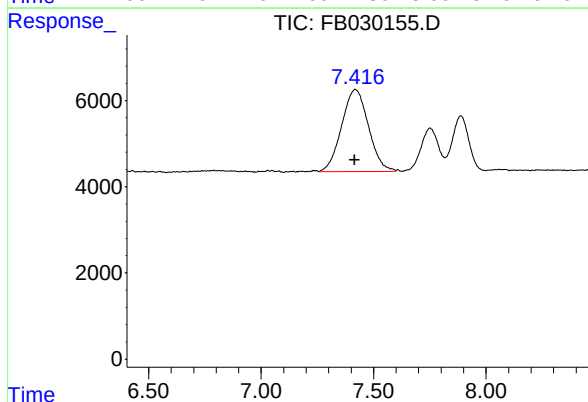


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.002 min
Response: 157873
Conc: 7.51 ng/ml

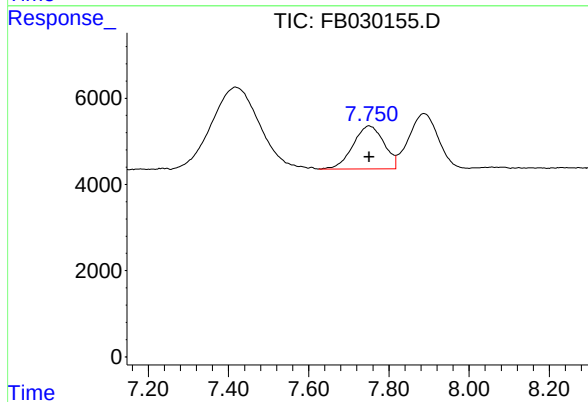


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 53572
Conc: 2.63 ng/ml

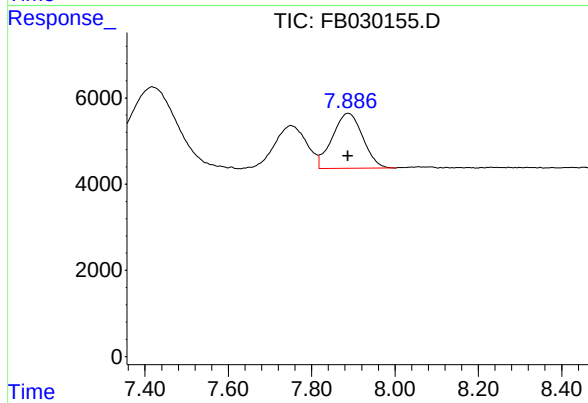

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.001 min
Response: 64762
Conc: 2.64 ng/ml

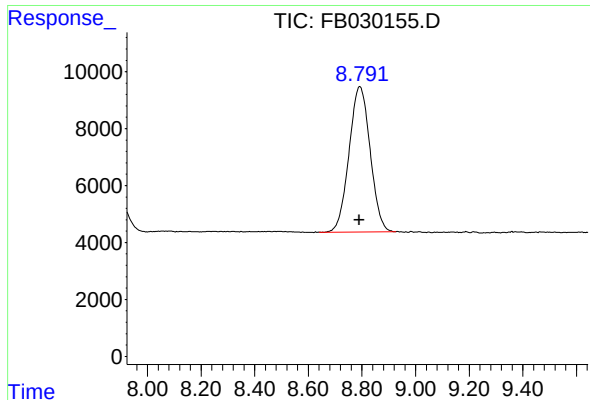

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.001 min
Response: 279185
Conc: 21.24 ng/ml

Instrument :
FID_B
ClientSampleId :

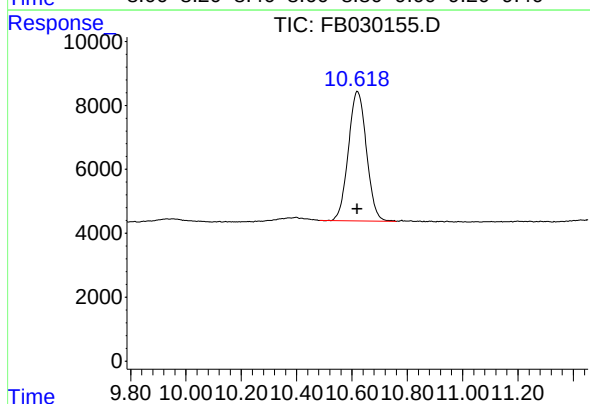


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.000 min
Response: 183426
Conc: 7.73 ng/ml

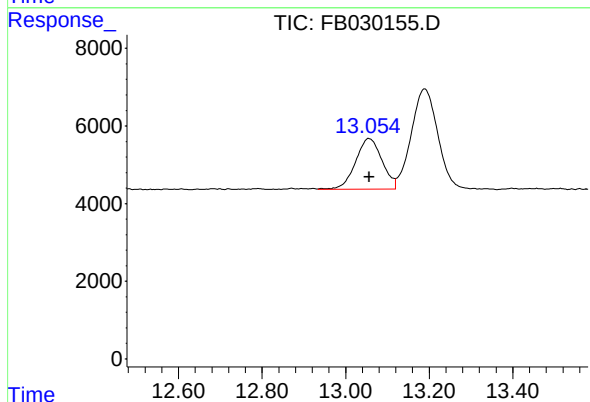


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 57403
Conc: 2.55 ng/ml

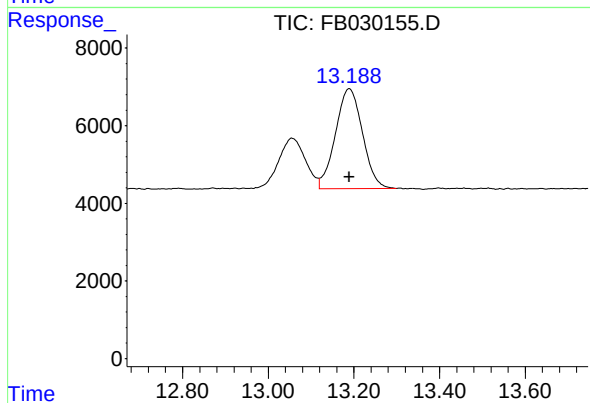

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.000 min
Response: 113228
Conc: 4.98 ng/ml

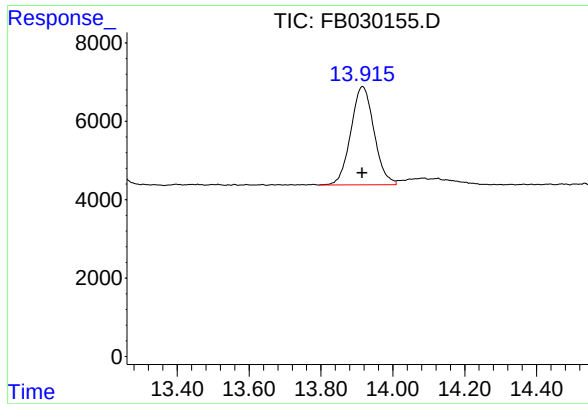

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.001 min
Response: 112078
Conc: 4.94 ng/ml

Instrument :
FID_B
ClientSampleId :

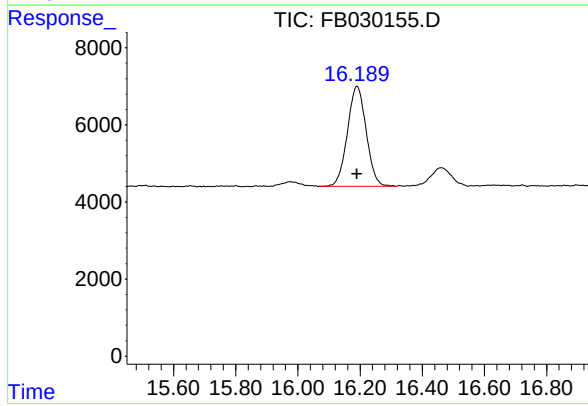

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 108664
Conc: 4.75 ng/ml