

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071123\
 Data File : FB030159.D
 Signal(s) : FID2B.CH
 Acq On : 11 Jul 2023 17:49
 Operator : YP/AJ
 Sample : BSF0711W1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jul 12 03:10:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
 Quant Title :
 QLast Update : Mon Jun 26 14:31:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	271226	20.639 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	527488	28.059 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	595248	28.307 ng/ml
3) t n-Heptane	7.753	204066	10.001 ng/ml
4) t Benzene	7.889	249117	10.165 ng/ml
6) t Toluene	10.622	718221	30.269 ng/ml
7) t Ethylbenzene	13.058	224260	9.965 ng/ml
8) t m-Xylene	13.191	436807	19.207 ng/ml
9) t O-Xylene	13.917	424358	18.717 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	391100	17.101 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071123\
Data File : FB030159.D
Signal(s) : FID2B.CH
Acq On : 11 Jul 2023 17:49
Operator : YP/AJ
Sample : BSF0711W1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 12 03:10:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
Quant Title :
QLast Update : Mon Jun 26 14:31:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

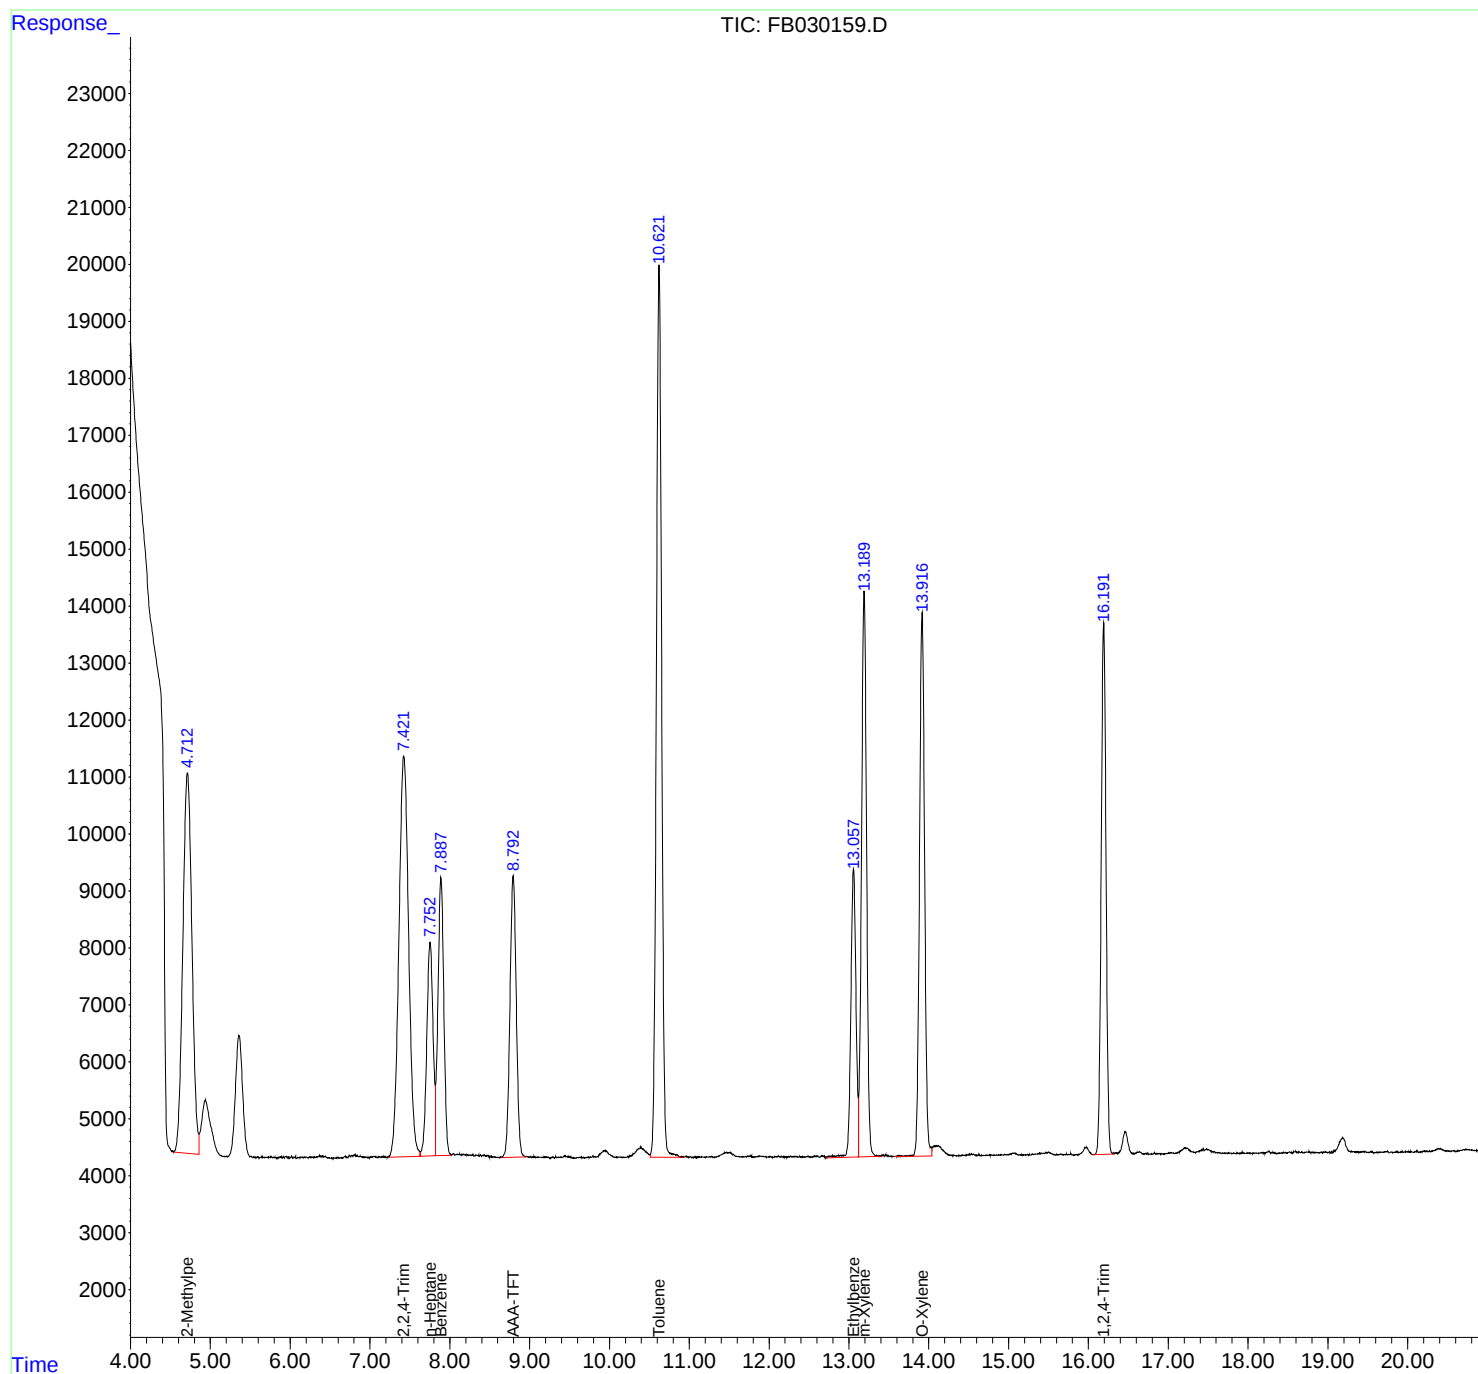

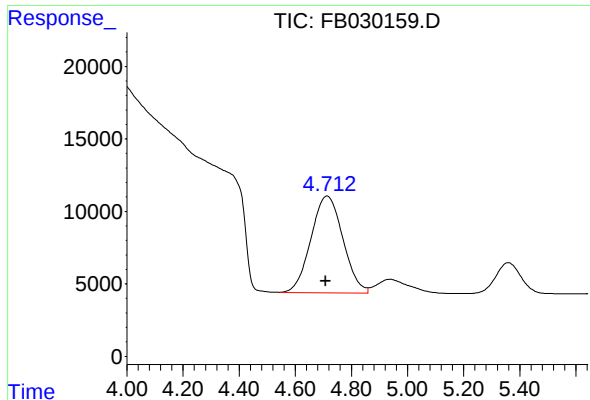


#1 2-Methylpentane

R.T.: 4.713 min
Delta R.T.: 0.005 min
Response: 527488
Conc: 28.06 ng/ml

Instrument :


FID_B

ClientSampleId :

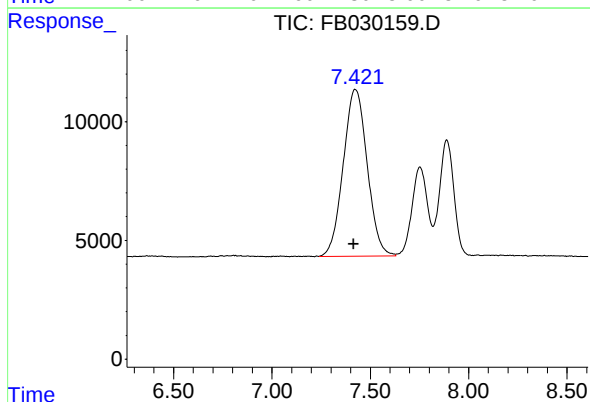


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.007 min
Response: 595248
Conc: 28.31 ng/ml

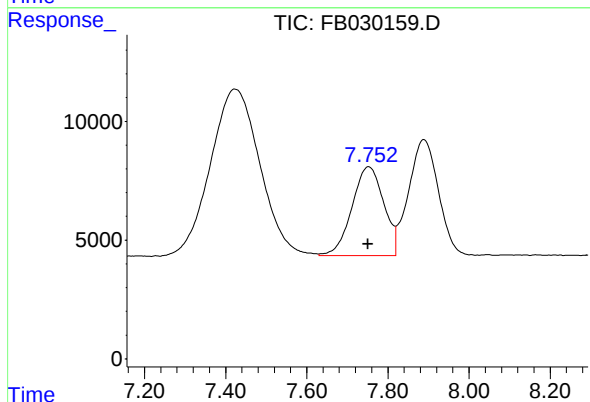


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.002 min
Response: 204066
Conc: 10.00 ng/ml

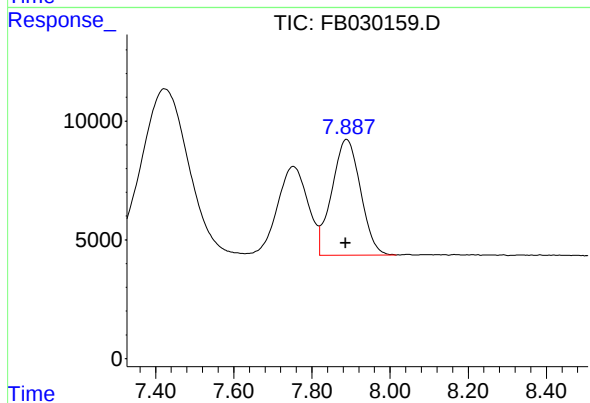

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.002 min
Response: 249117
Conc: 10.17 ng/ml

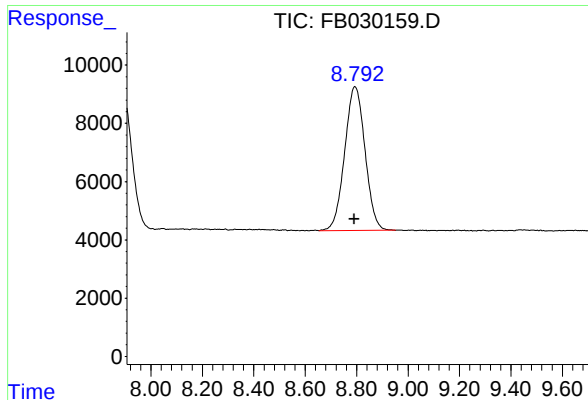

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.003 min
Response: 271226
Conc: 20.64 ng/ml

Instrument :
FID_B
ClientSampleId :

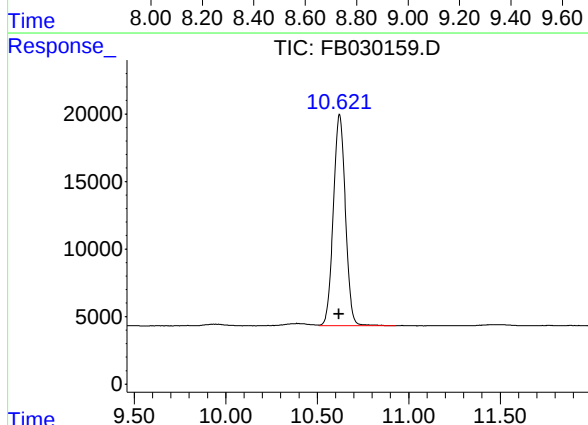


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.003 min
Response: 718221
Conc: 30.27 ng/ml

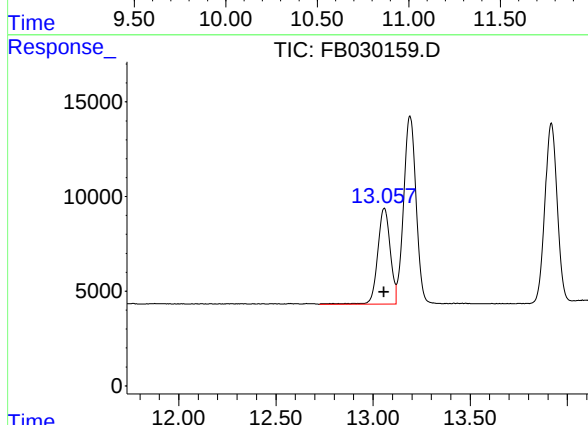


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.002 min
Response: 224260
Conc: 9.97 ng/ml

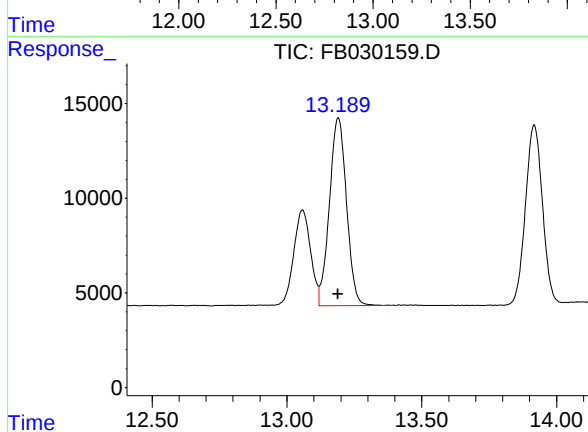

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.002 min
Response: 436807
Conc: 19.21 ng/ml

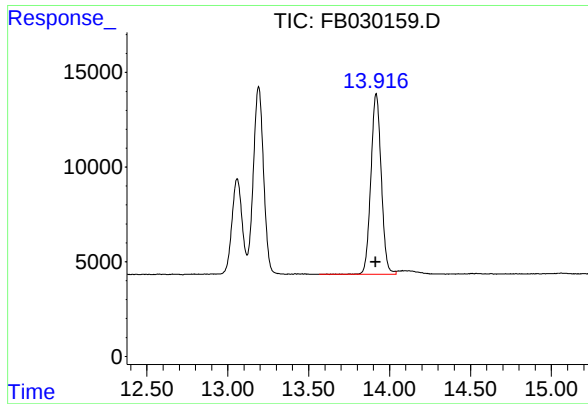

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.002 min
Response: 424358
Conc: 18.72 ng/ml

Instrument :
FID_B
ClientSampleId :

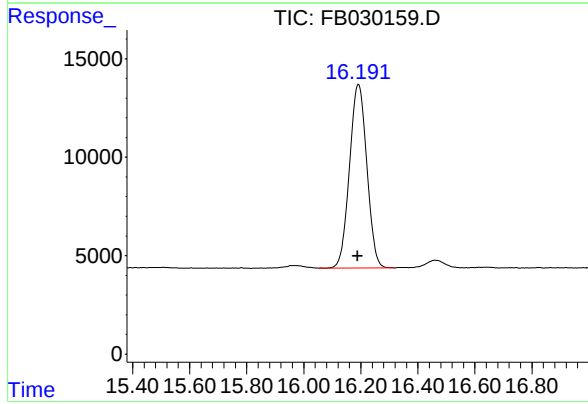

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.002 min
Response: 391100
Conc: 17.10 ng/ml