

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071123\
 Data File : FB030156.D
 Signal(s) : FID2B.CH
 Acq On : 11 Jul 2023 15:13
 Operator : YP/AJ
 Sample : BSF0711S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0711S2

Integration File: Calibration.e
 Quant Time: Jul 12 03:10:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
 Quant Title :
 QLast Update : Mon Jun 26 14:31:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	296424	22.557 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	509831	27.120 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	557712	26.522 ng/ml
3) t n-Heptane	7.752	201137	9.857 ng/ml
4) t Benzene	7.888	241993	9.875 ng/ml
6) t Toluene	10.620	708935	29.877 ng/ml
7) t Ethylbenzene	13.056	217303	9.656 ng/ml
8) t m-Xylene	13.189	428549	18.844 ng/ml
9) t O-Xylene	13.915	412072	18.175 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	382321	16.717 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071123\
Data File : FB030156.D
Signal(s) : FID2B.CH
Acq On : 11 Jul 2023 15:13
Operator : YP/AJ
Sample : BSF0711S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0711S2

Integration File: Calibration.e
Quant Time: Jul 12 03:10:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
Quant Title :
QLast Update : Mon Jun 26 14:31:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

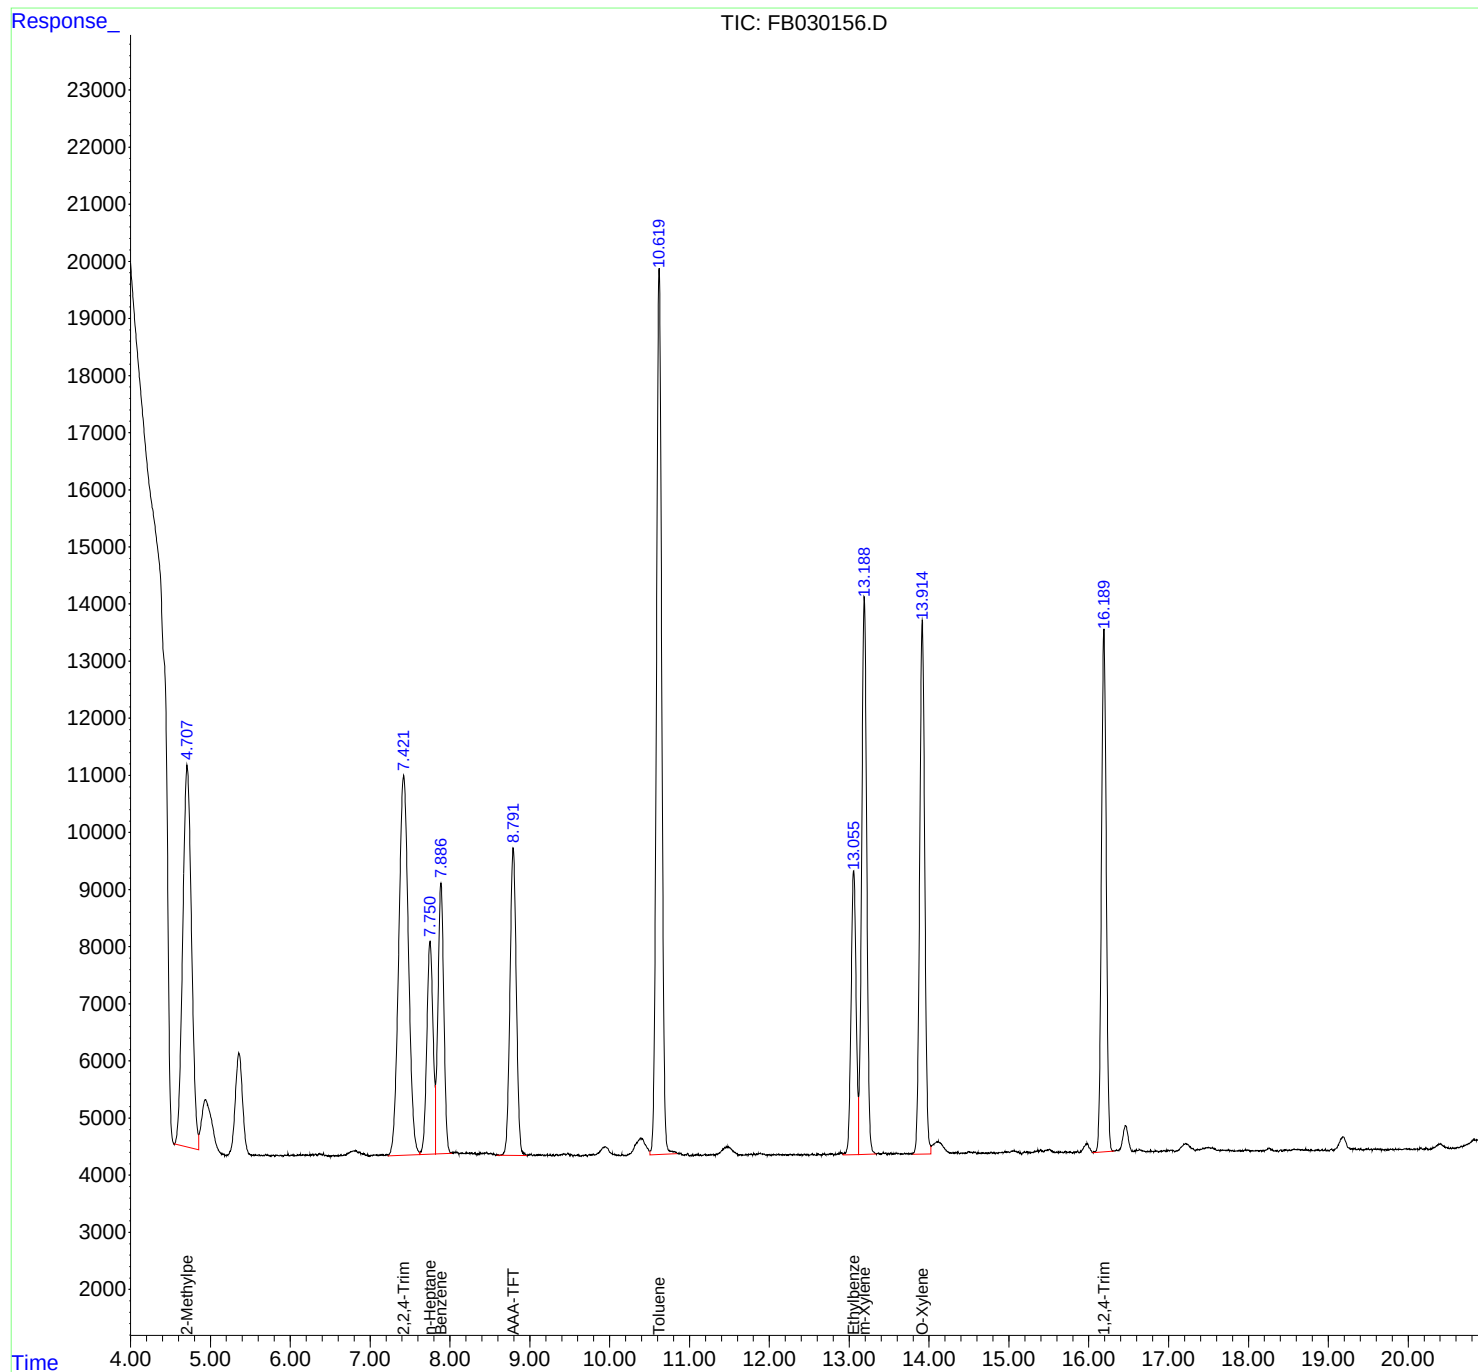


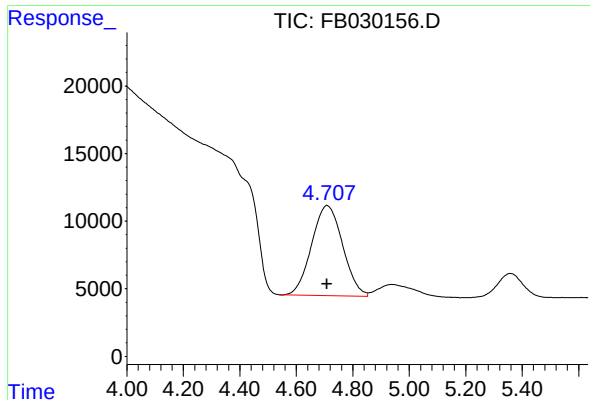

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 509831
Conc: 27.12 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0711S2

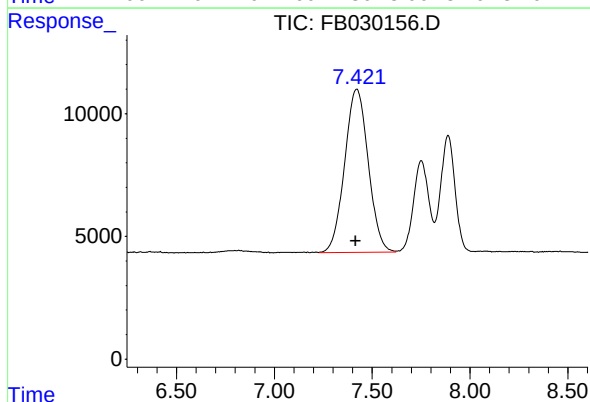


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.006 min
Response: 557712
Conc: 26.52 ng/ml

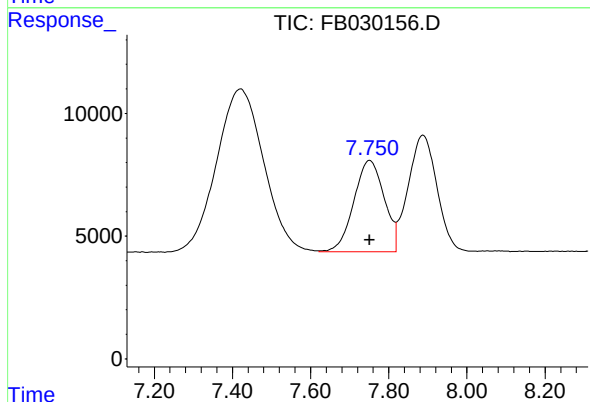


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 201137
Conc: 9.86 ng/ml

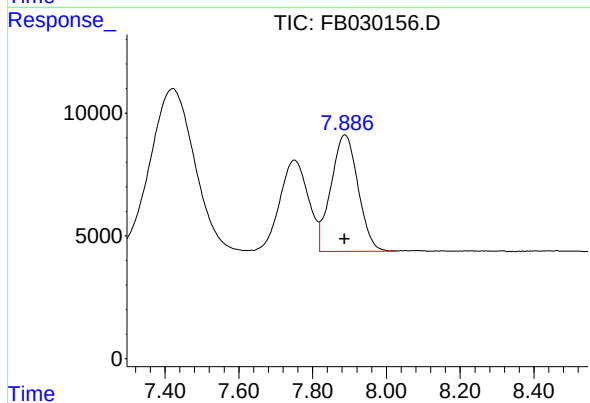

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.001 min
Response: 241993
Conc: 9.87 ng/ml

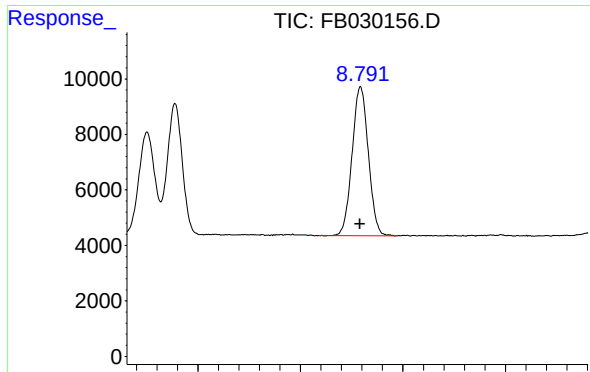

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 296424
Conc: 22.56 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0711S2

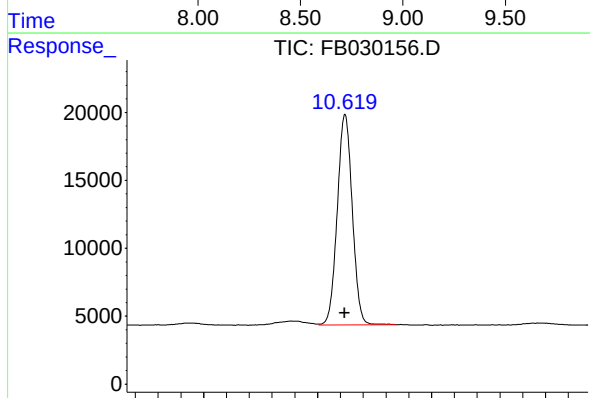


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.000 min
Response: 708935
Conc: 29.88 ng/ml

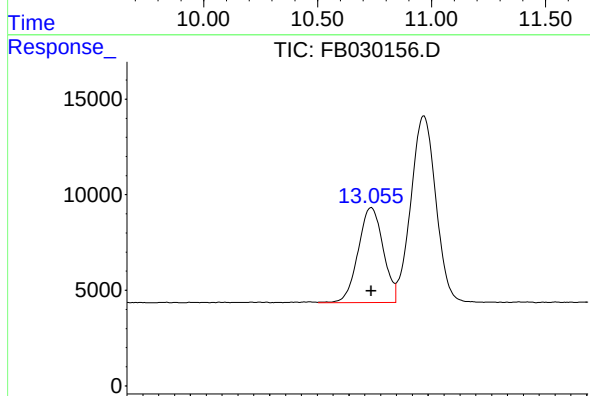


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 217303
Conc: 9.66 ng/ml

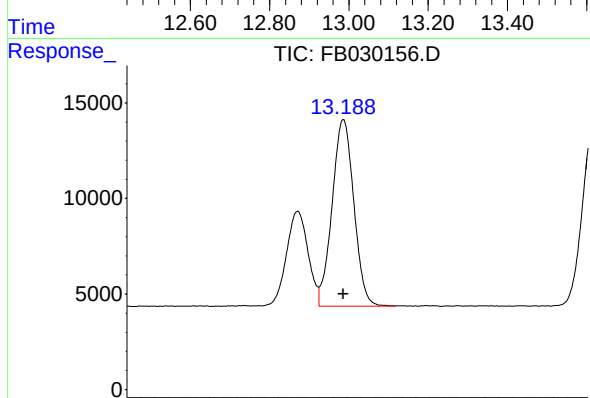

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 428549
Conc: 18.84 ng/ml

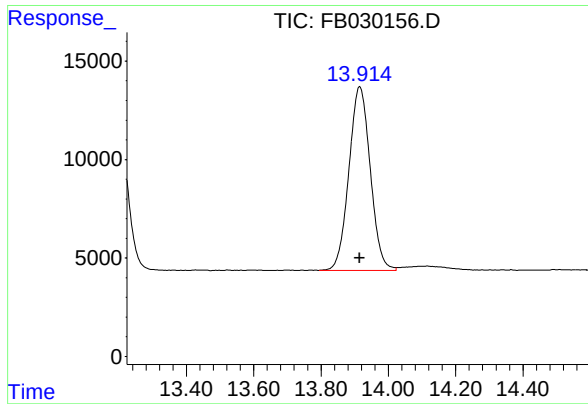

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: 0.000 min
Response: 412072
Conc: 18.18 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0711S2

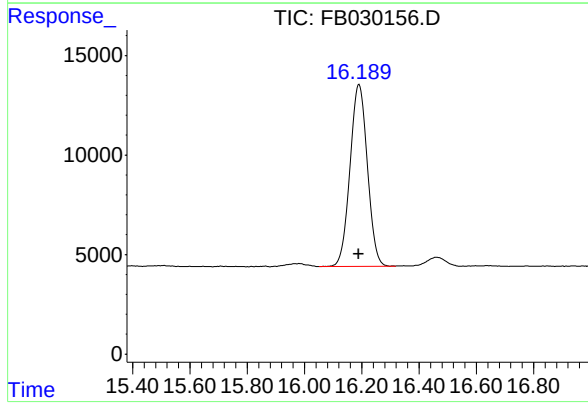

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: 0.000 min
Response: 382321
Conc: 16.72 ng/ml