

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071123\
 Data File : FB030160.D
 Signal(s) : FID2B.CH
 Acq On : 11 Jul 2023 18:28
 Operator : YP/AJ
 Sample : BSF0711W2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0711W2

Integration File: Calibration.e
 Quant Time: Jul 12 03:10:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
 Quant Title :
 QLast Update : Mon Jun 26 14:31:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	262710	19.991 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.714	603005	32.076 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	685973	32.622 ng/ml
3) t n-Heptane	7.753	233703	11.453 ng/ml
4) t Benzene	7.891	264931	10.811 ng/ml
6) t Toluene	10.623	773708	32.607 ng/ml
7) t Ethylbenzene	13.059	238806	10.611 ng/ml
8) t m-Xylene	13.192	470302	20.680 ng/ml
9) t O-Xylene	13.919	442815	19.532 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	424886	18.578 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071123\
Data File : FB030160.D
Signal(s) : FID2B.CH
Acq On : 11 Jul 2023 18:28
Operator : YP/AJ
Sample : BSF0711W2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0711W2

Integration File: Calibration.e
Quant Time: Jul 12 03:10:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
Quant Title :
QLast Update : Mon Jun 26 14:31:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

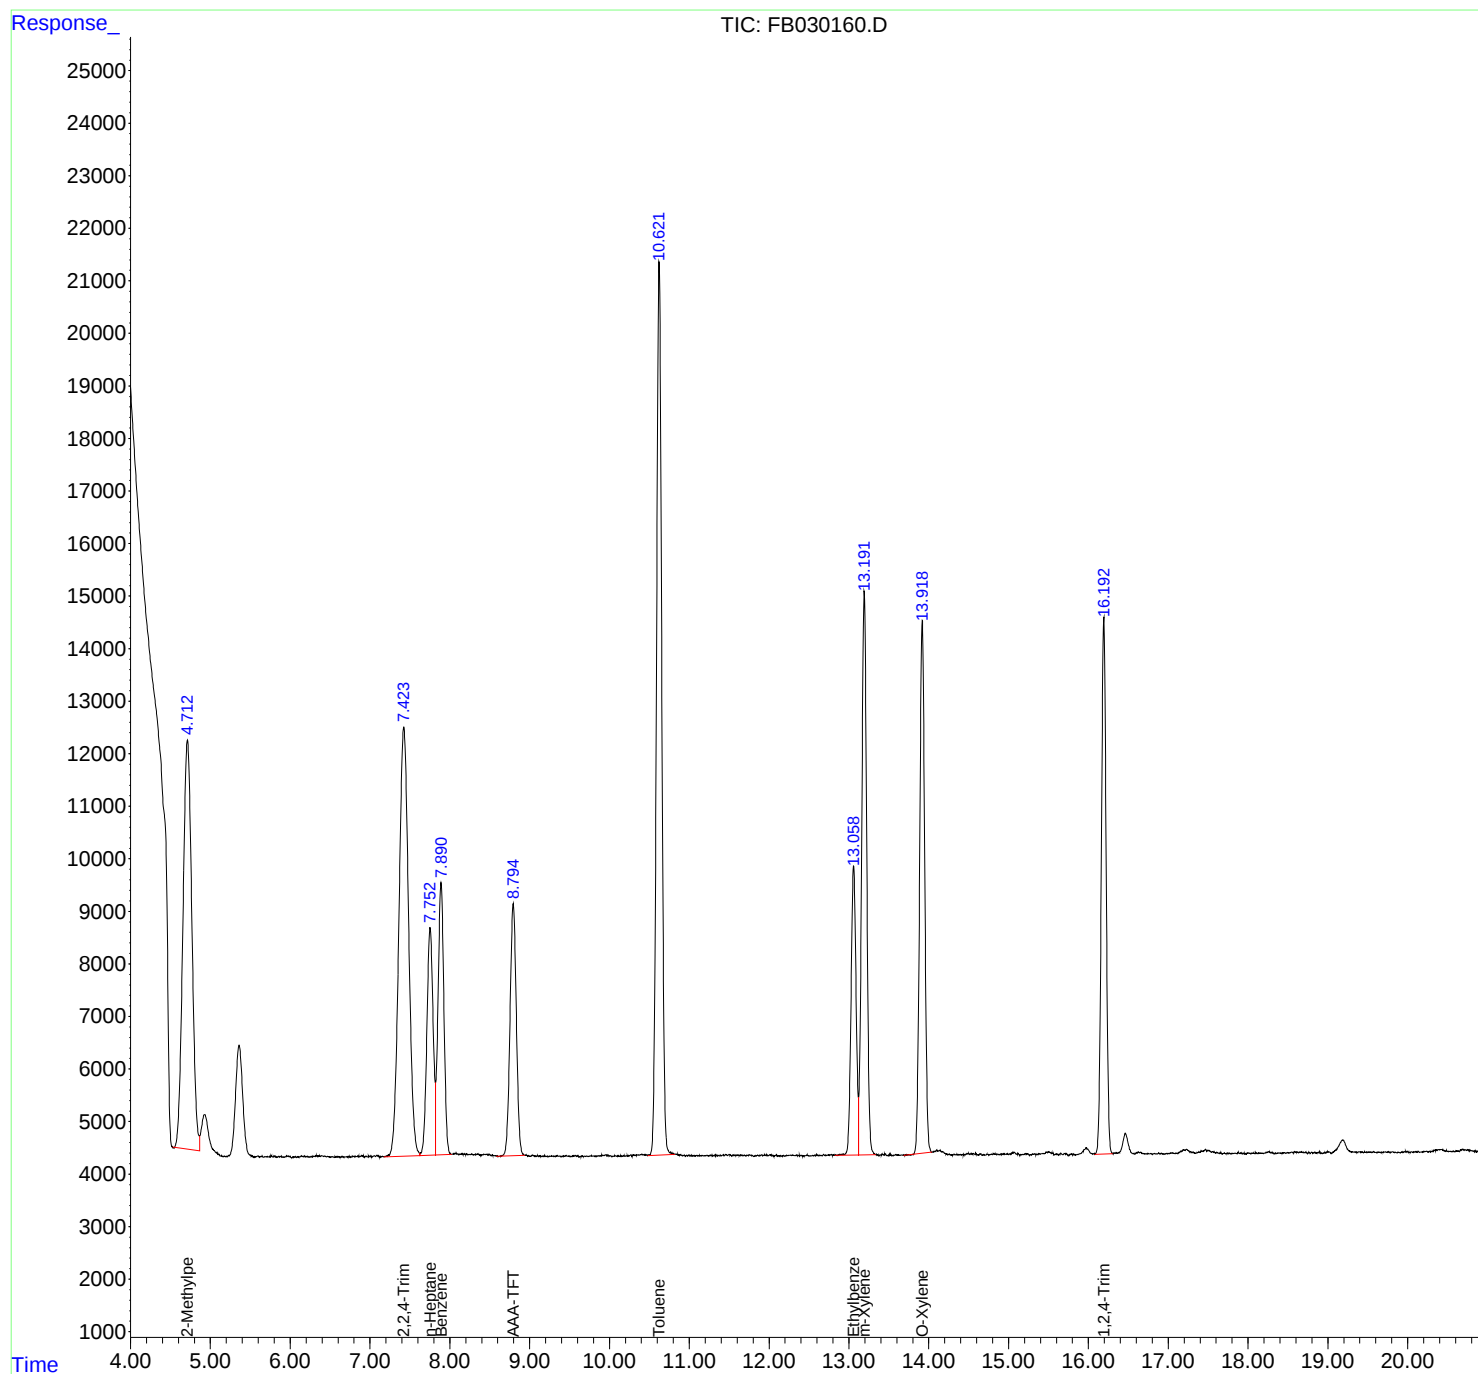


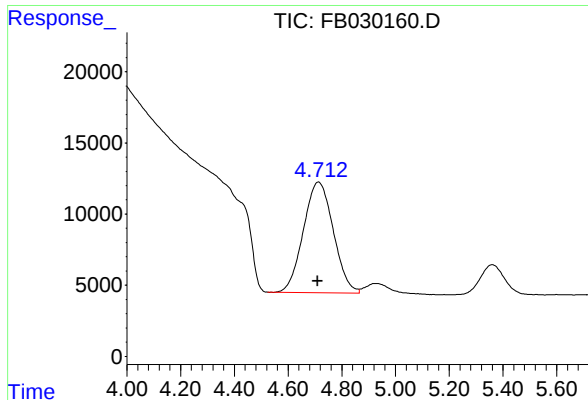

#1 2-Methylpentane


R.T.: 4.714 min
Delta R.T.: 0.005 min
Response: 603005
Conc: 32.08 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0711W2

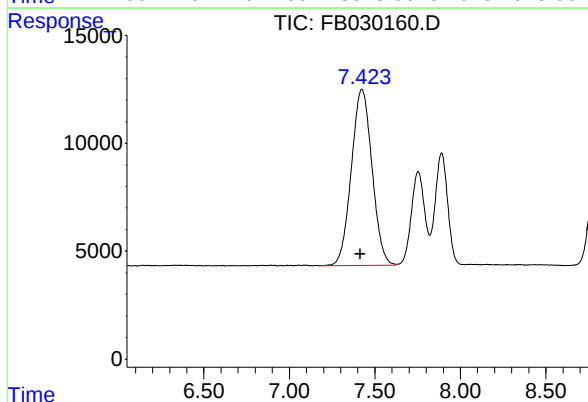


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: 0.009 min
Response: 685973
Conc: 32.62 ng/ml

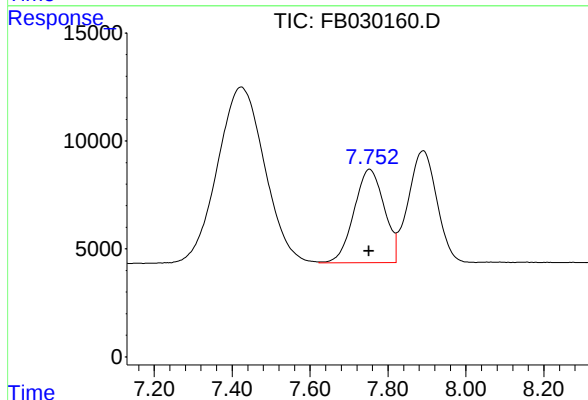


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.002 min
Response: 233703
Conc: 11.45 ng/ml

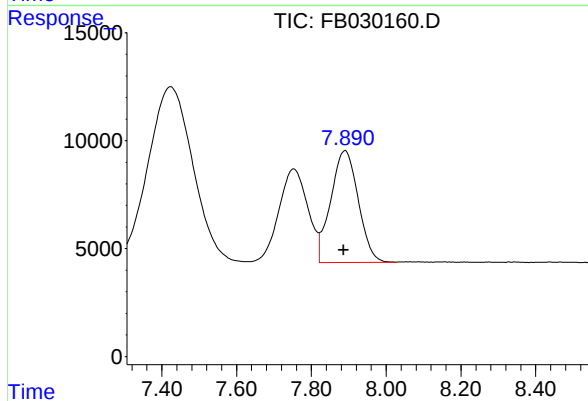

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.005 min
Response: 264931
Conc: 10.81 ng/ml

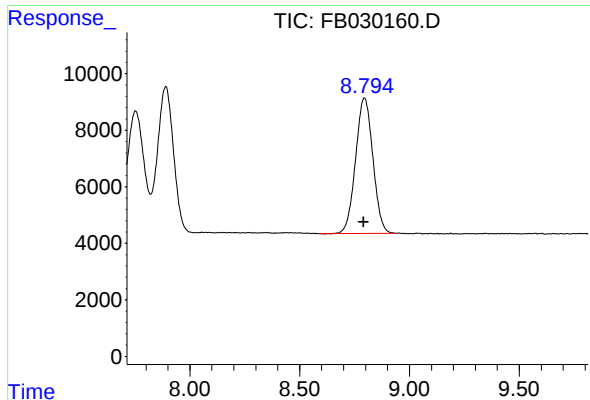

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.004 min
Response: 262710
Conc: 19.99 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0711W2

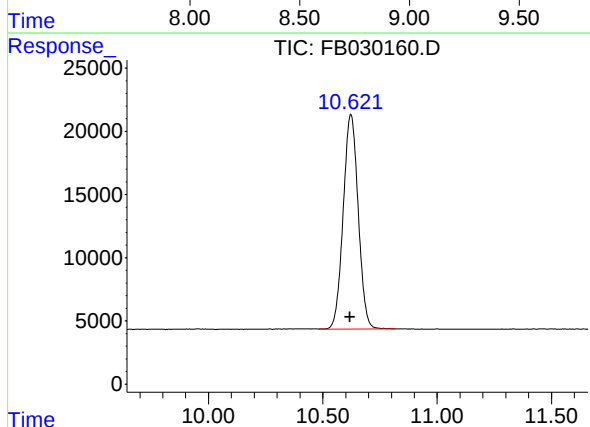


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.003 min
Response: 773708
Conc: 32.61 ng/ml

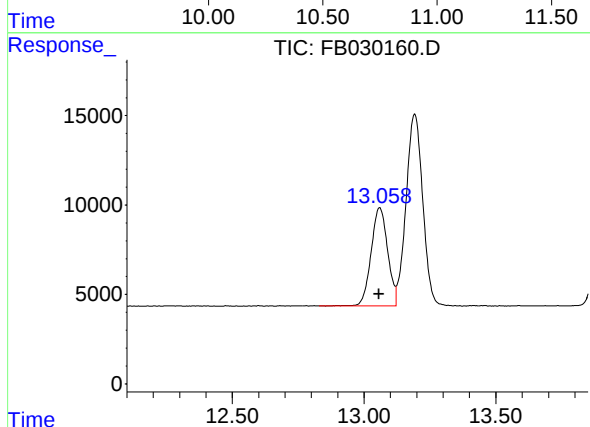


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.003 min
Response: 238806
Conc: 10.61 ng/ml

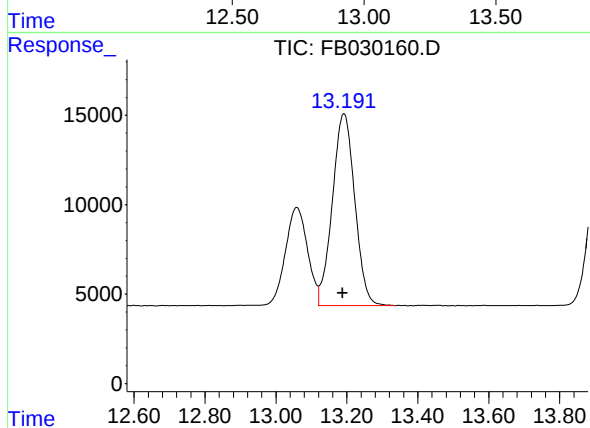

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.004 min
Response: 470302
Conc: 20.68 ng/ml

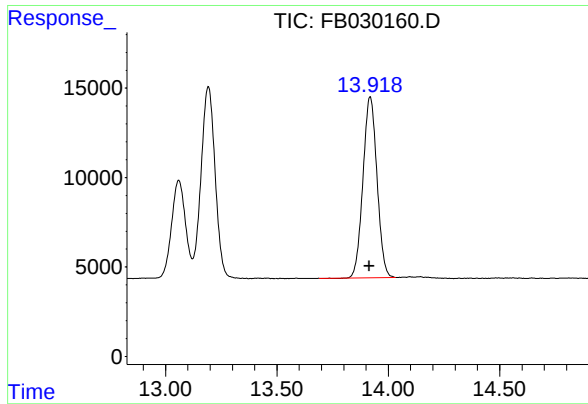

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.004 min
Response: 442815
Conc: 19.53 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0711W2

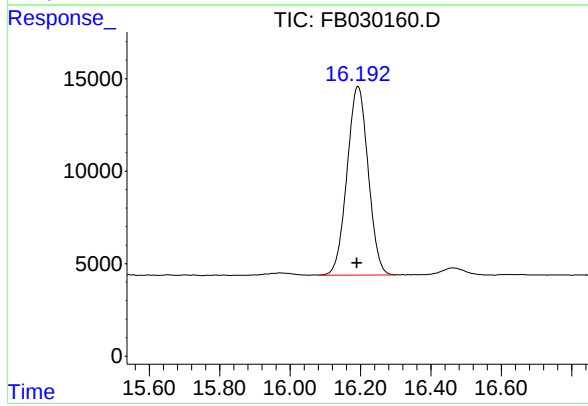

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.004 min
Response: 424886
Conc: 18.58 ng/ml