

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071123\
 Data File : FB030164.D
 Signal(s) : FID2B.CH
 Acq On : 11 Jul 2023 22:21
 Operator : YP/AJ
 Sample : BSF0711W3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0711W3

Integration File: Calibration.e
 Quant Time: Jul 12 03:11:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
 Quant Title :
 QLast Update : Mon Jun 26 14:31:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	230795	17.563 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	508980	27.075 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	566892	26.959 ng/ml
3) t n-Heptane	7.752	197351	9.672 ng/ml
4) t Benzene	7.888	237867	9.706 ng/ml
6) t Toluene	10.621	700904	29.539 ng/ml
7) t Ethylbenzene	13.057	214442	9.529 ng/ml
8) t m-Xylene	13.190	425166	18.695 ng/ml
9) t O-Xylene	13.917	409478	18.061 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	387838	16.958 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071123\
Data File : FB030164.D
Signal(s) : FID2B.CH
Acq On : 11 Jul 2023 22:21
Operator : YP/AJ
Sample : BSF0711W3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0711W3

Integration File: Calibration.e
Quant Time: Jul 12 03:11:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
Quant Title :
QLast Update : Mon Jun 26 14:31:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

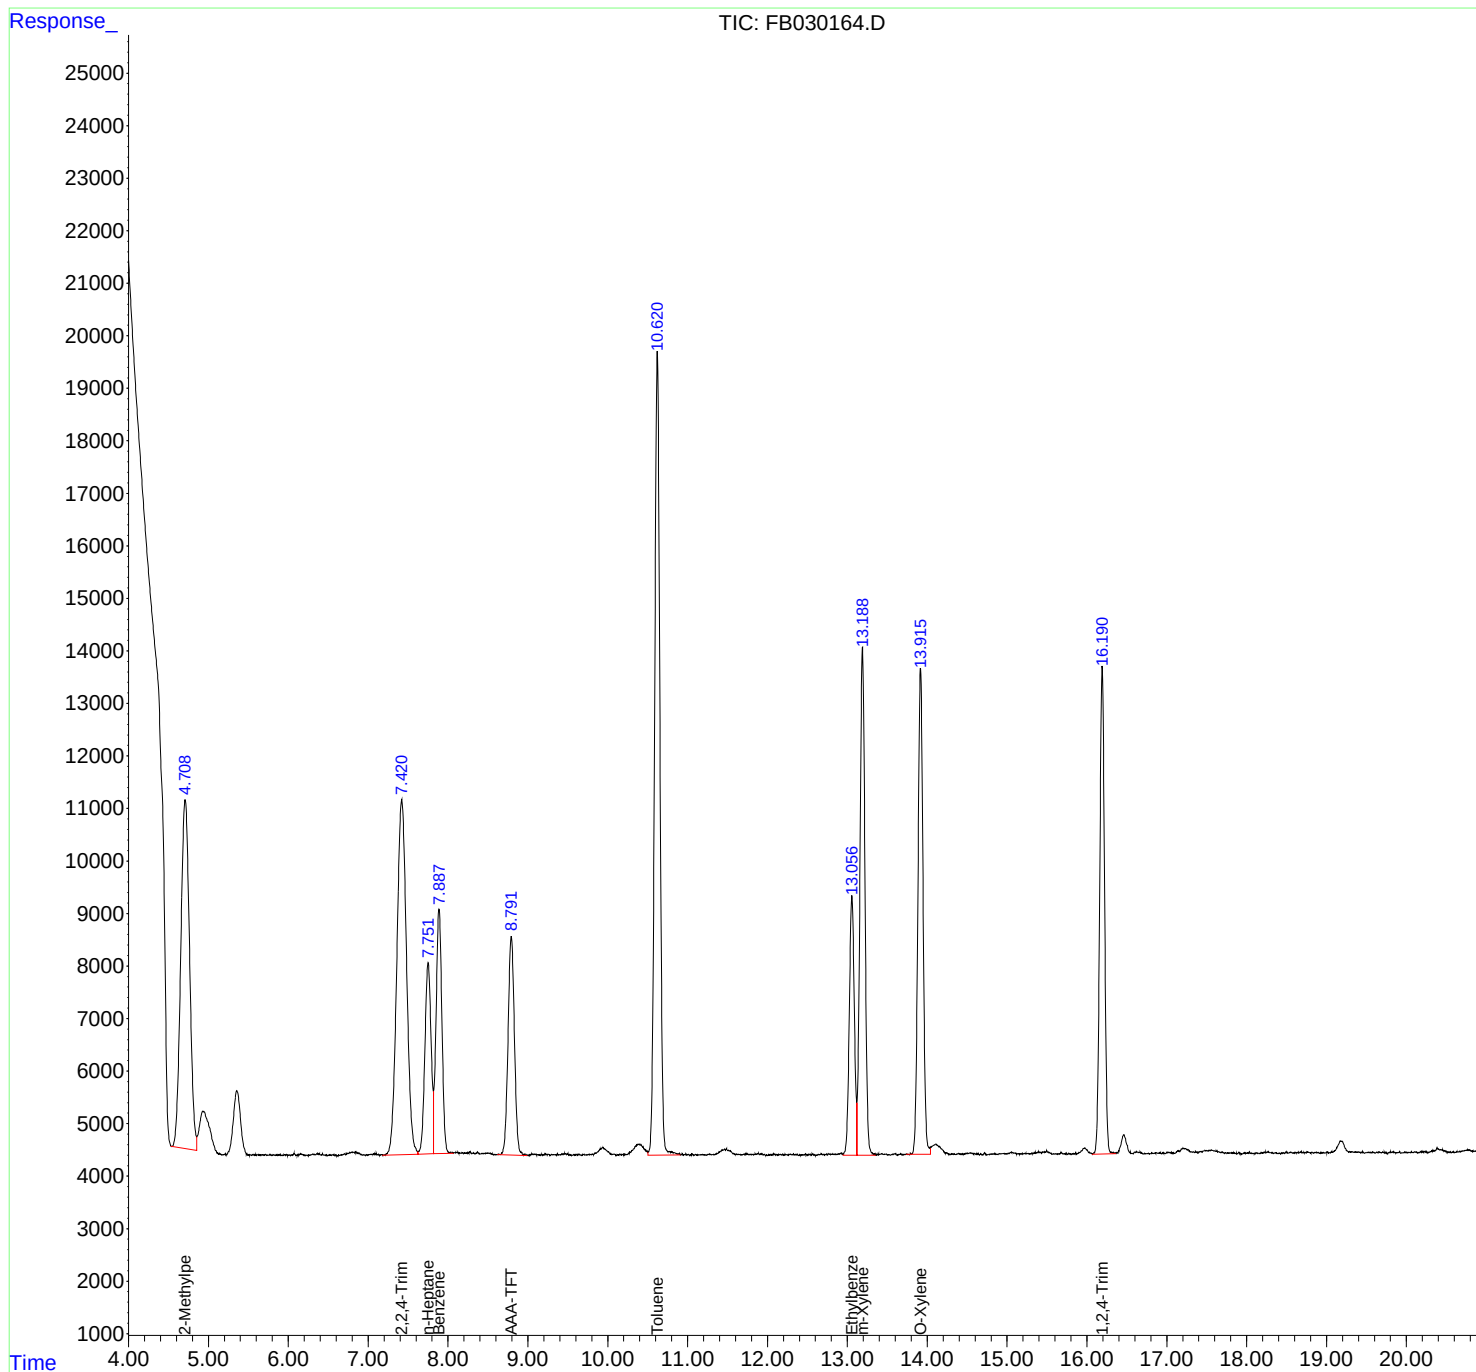


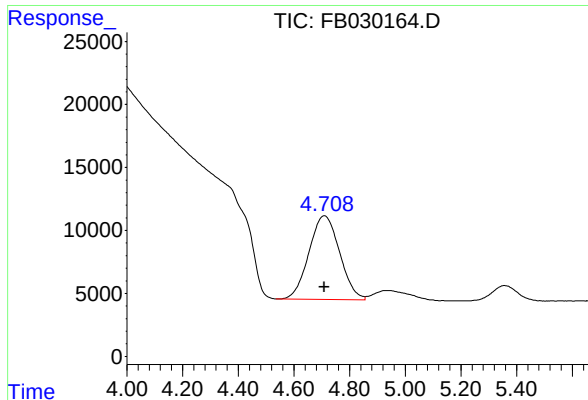

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 508980
Conc: 27.07 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0711W3

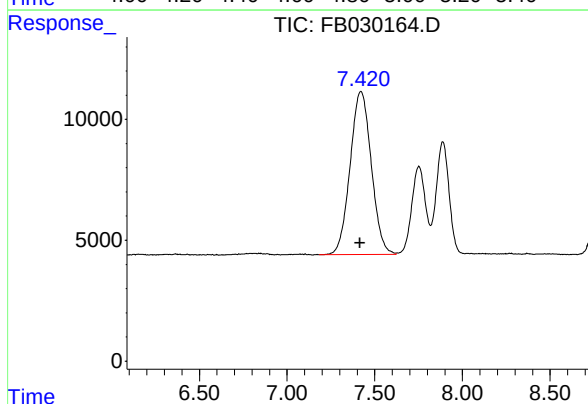


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: 0.006 min
Response: 566892
Conc: 26.96 ng/ml

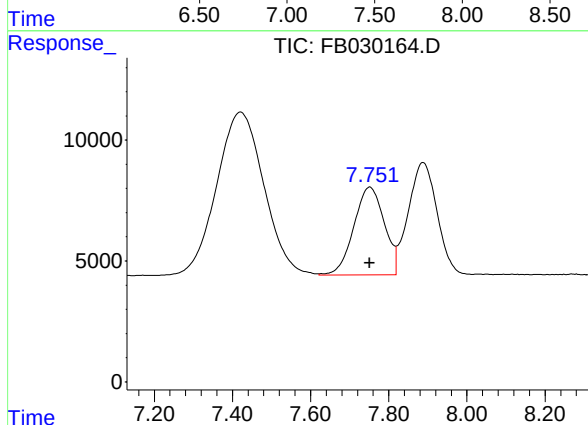


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 197351
Conc: 9.67 ng/ml

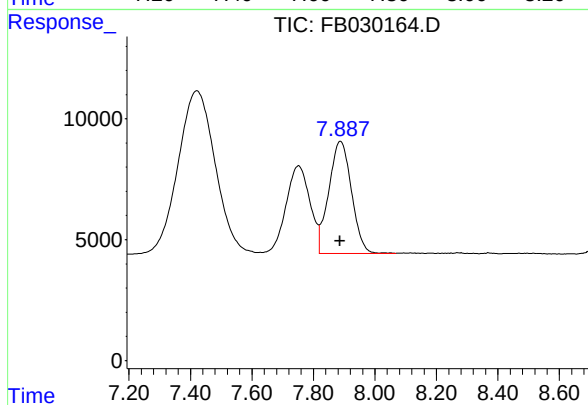

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.002 min
Response: 237867
Conc: 9.71 ng/ml

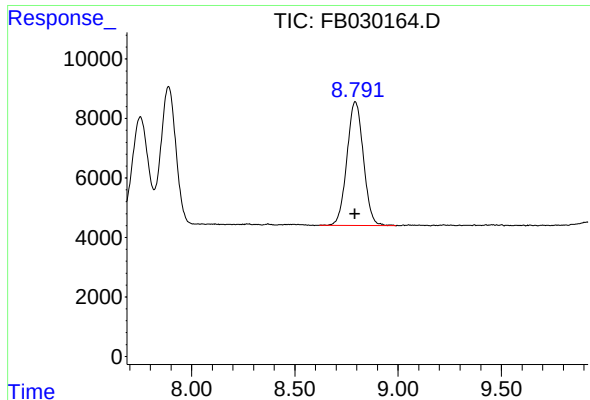

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 230795
Conc: 17.56 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0711W3

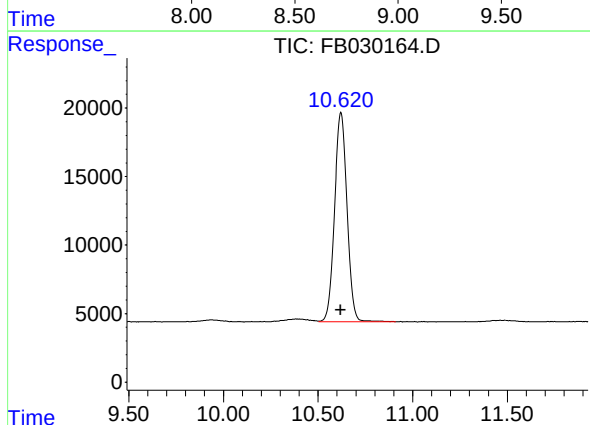


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.002 min
Response: 700904
Conc: 29.54 ng/ml

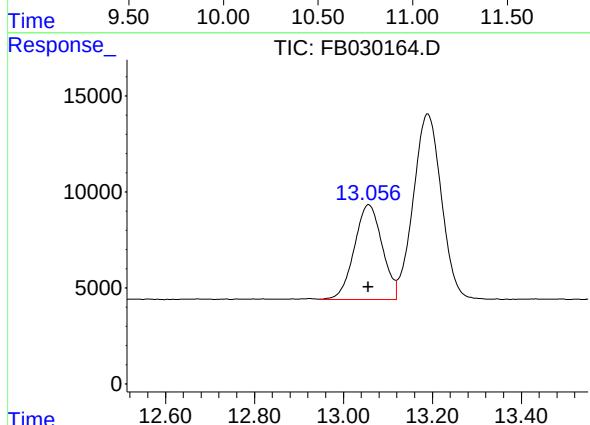


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.000 min
Response: 214442
Conc: 9.53 ng/ml

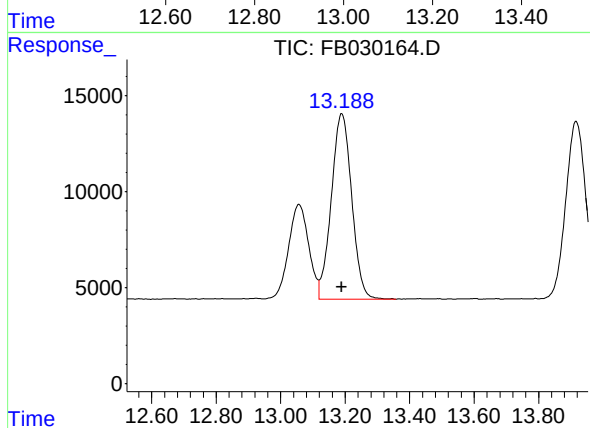

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.001 min
Response: 425166
Conc: 18.70 ng/ml

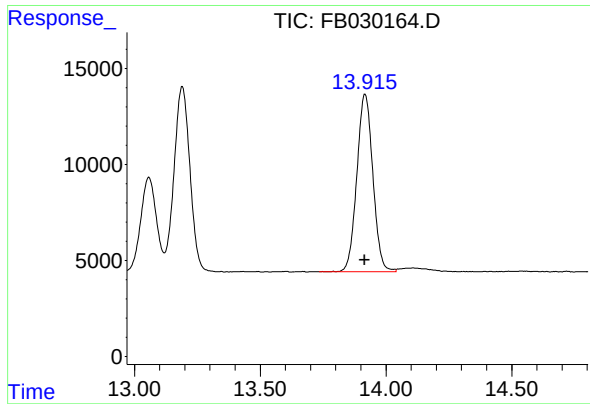

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.002 min
Response: 409478
Conc: 18.06 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0711W3

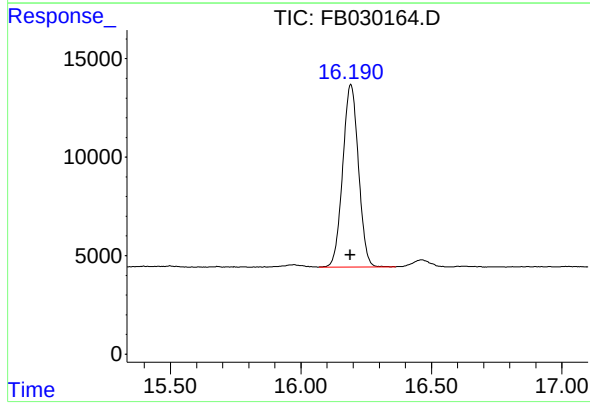

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.002 min
Response: 387838
Conc: 16.96 ng/ml