

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071218\
 Data File : FB016689.D
 Signal(s) : FID2B.CH
 Acq On : 12 Jul 2018 12:06
 Operator : MJ/SJ
 Sample : J3825-01MSD
 Misc : 5.00g/5.00ml DI water
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 12 17:19:39 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070918.M
 Quant Title :
 QLast Update : Mon Jul 09 13:06:15 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.112	134582	15.436 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.964	313483	21.579 ng/ml
2) t 2,2,4-Trimethylpentane	7.729	290643	20.896 ng/ml
3) t n-Heptane	8.070	90853	6.705 ng/ml
4) t Benzene	8.207	145701	7.852 ng/ml
6) t Toluene	10.962	350619	24.010 ng/ml
7) t Ethylbenzene	13.411	114891	7.822 ng/ml
8) t m-Xylene	13.544	240050	15.411 ng/ml
9) t O-Xylene	14.276	247029	14.924 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	288673	14.761 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071218\
Data File : FB016689.D
Signal(s) : FID2B.CH
Acq On : 12 Jul 2018 12:06
Operator : MJ/SJ
Sample : J3825-01MSD
Misc : 5.00g/5.00ml DI water
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 12 17:19:39 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070918.M
Quant Title :
QLast Update : Mon Jul 09 13:06:15 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

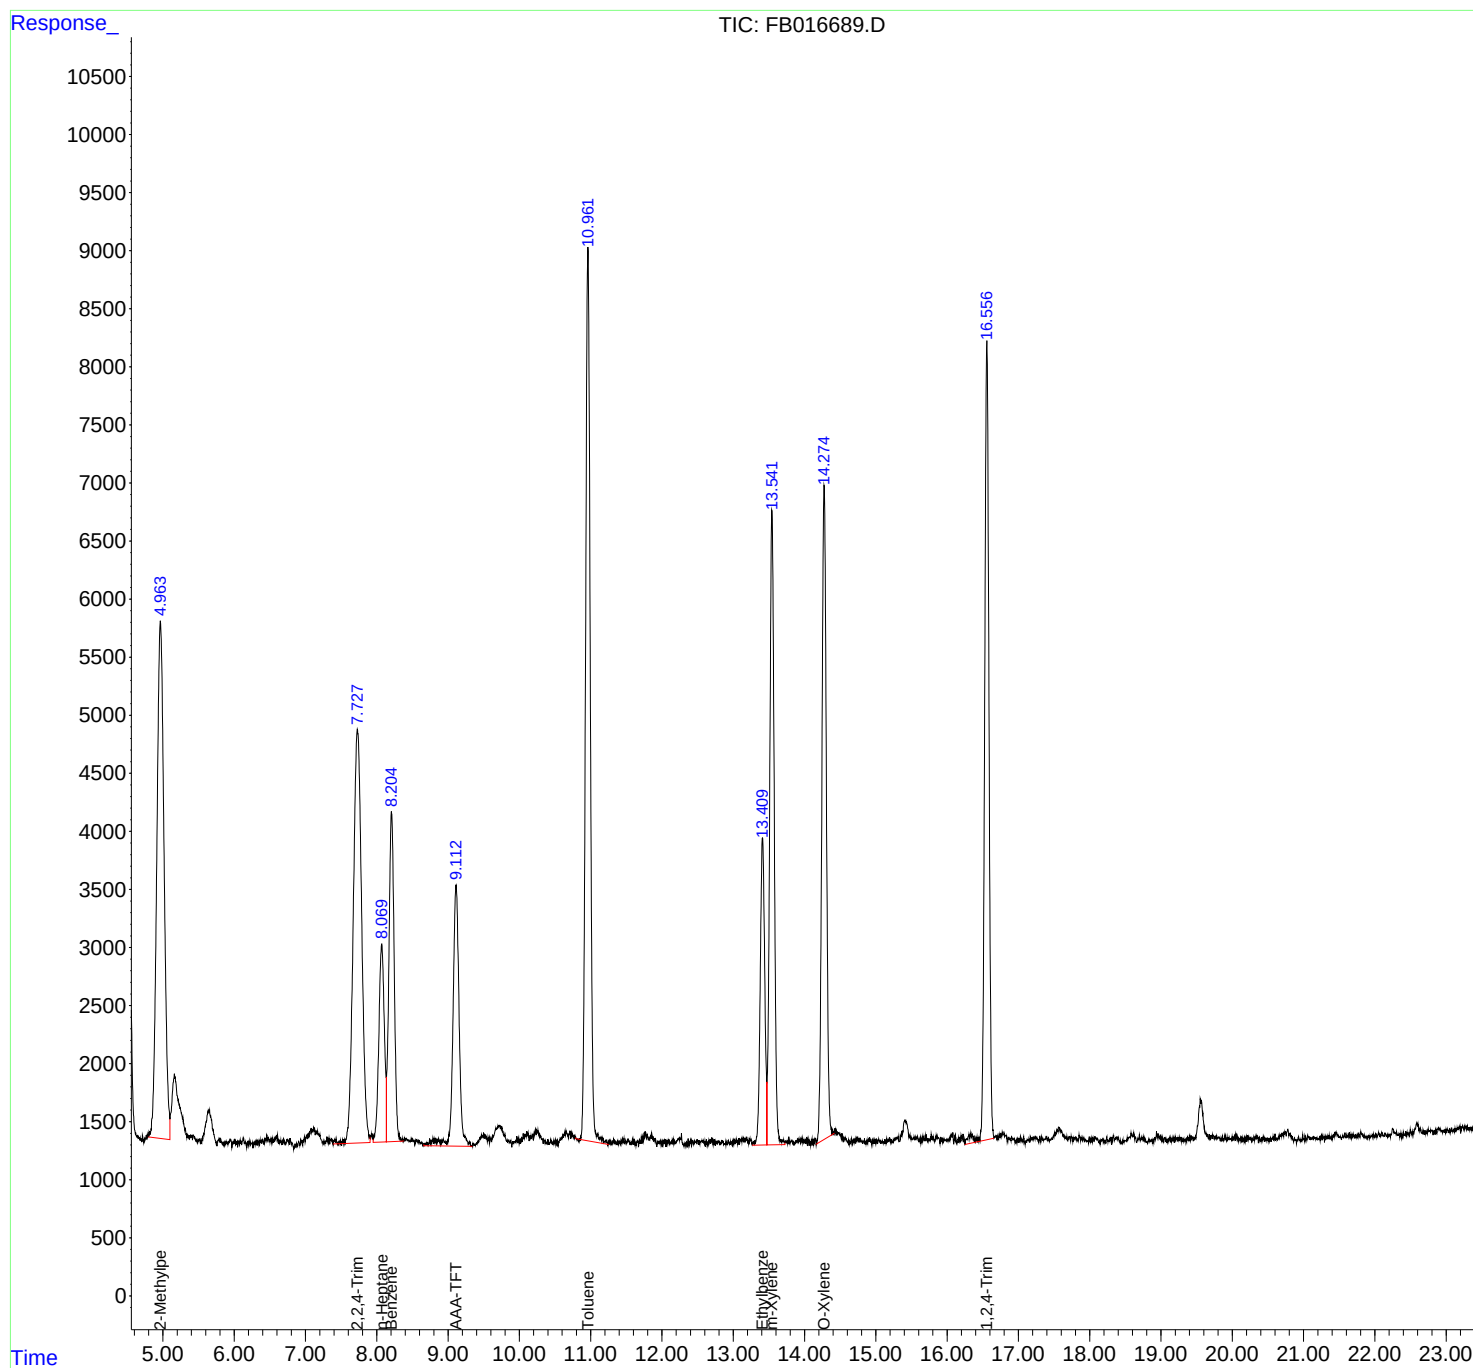

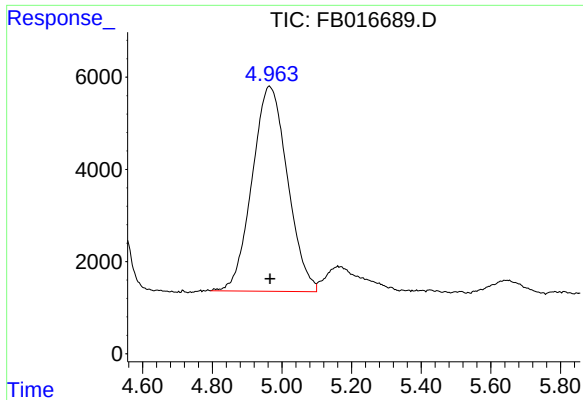


#1 2-Methylpentane

R.T.: 4.964 min
Delta R.T.: -0.002 min
Response: 313483
Conc: 21.58 ng/ml

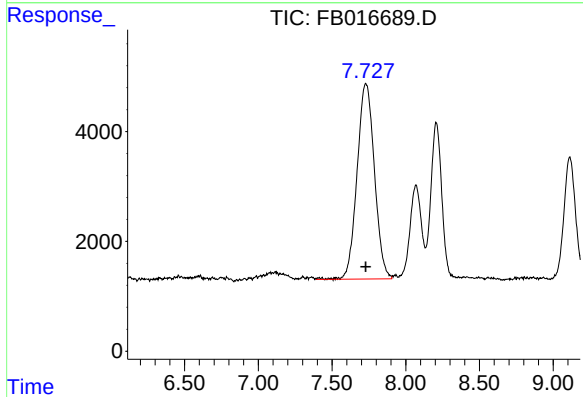


#2 2,2,4-Trimethylpentane

R.T.: 7.729 min
Delta R.T.: 0.000 min
Response: 290643
Conc: 20.90 ng/ml

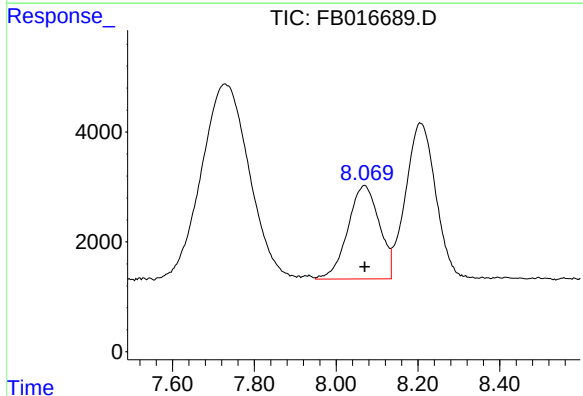


#3 n-Heptane

R.T.: 8.070 min
Delta R.T.: 0.000 min
Response: 90853
Conc: 6.70 ng/ml

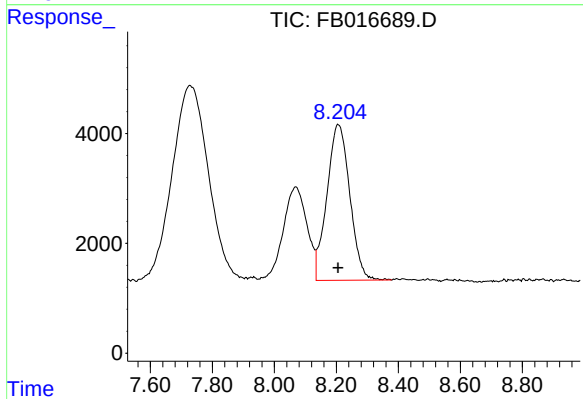


#4 Benzene

R.T.: 8.207 min
Delta R.T.: 0.002 min
Response: 145701
Conc: 7.85 ng/ml

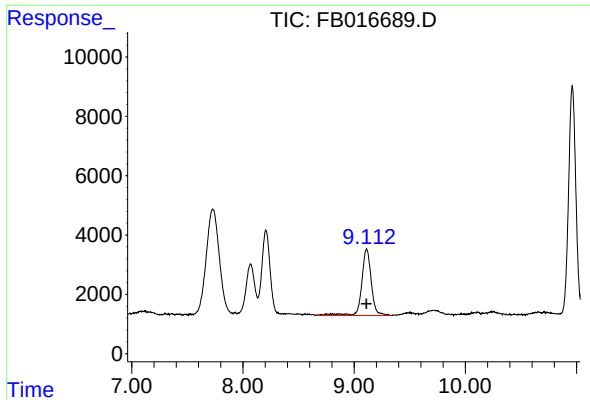


#5 AAA-TFT

R.T.: 9.112 min
Delta R.T.: 0.002 min
Response: 134582
Conc: 15.44 ng/ml

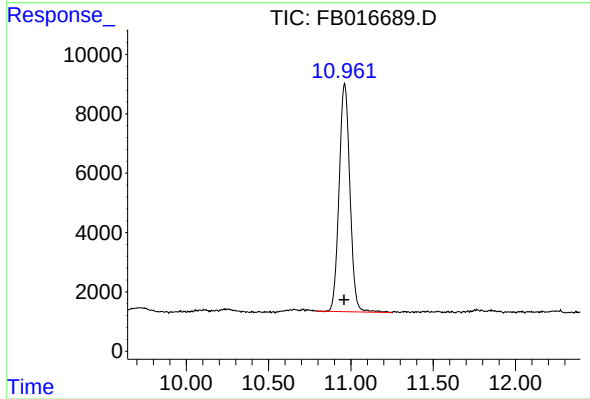


#6 Toluene

R.T.: 10.962 min
Delta R.T.: 0.003 min
Response: 350619
Conc: 24.01 ng/ml

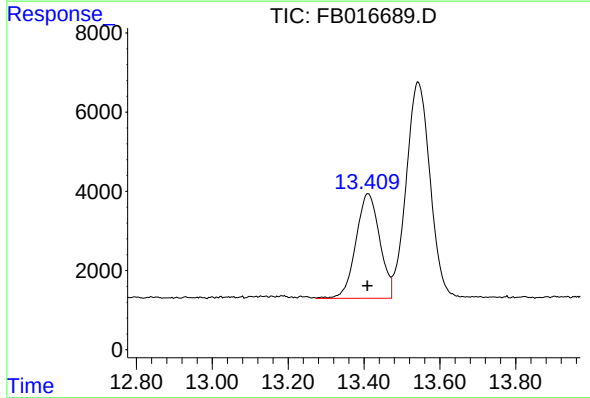


#7 Ethylbenzene

R.T.: 13.411 min
Delta R.T.: 0.003 min
Response: 114891
Conc: 7.82 ng/ml

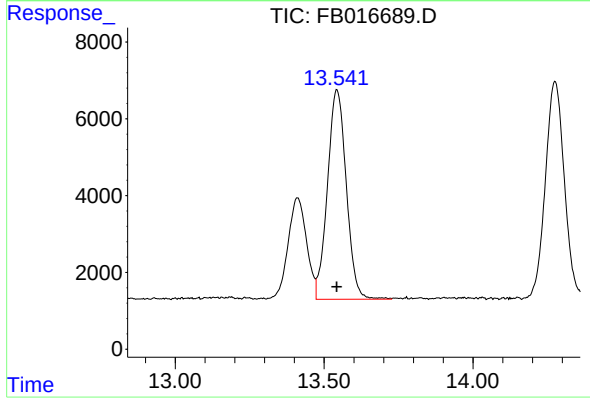


#8 m-Xylene

R.T.: 13.544 min
Delta R.T.: 0.001 min
Response: 240050
Conc: 15.41 ng/ml

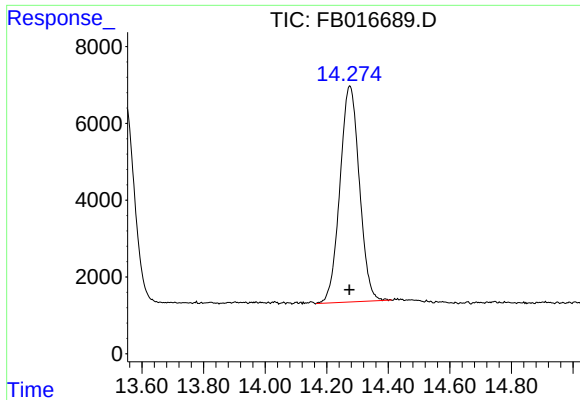

#9 O-Xylene

R.T.: 14.276 min
Delta R.T.: 0.002 min
Response: 247029
Conc: 14.92 ng/ml

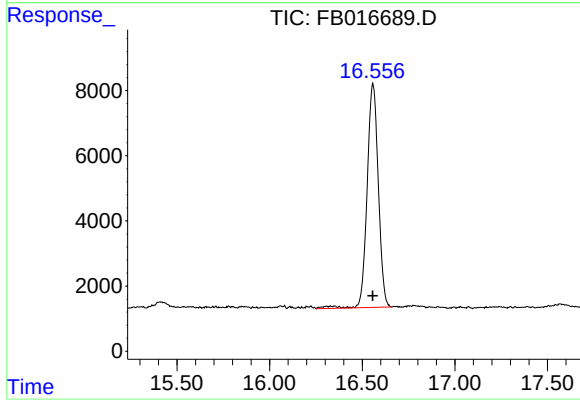

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.002 min
Response: 288673
Conc: 14.76 ng/ml