

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071321\
 Data File : FB026042.D
 Signal(s) : FID2B.CH
 Acq On : 13 Jul 2021 11:25
 Operator : AJ/MA
 Sample : BSF0713S1
 Misc : 5.00G/5.00ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 14 01:07:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071021.M
 Quant Title :
 QLast Update : Fri Jul 09 13:11:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.218	371854	19.713 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.174	771522	31.292 ng/ml
2) t 2,2,4-Trimethylpentane	7.873	647575	31.998 ng/ml
3) t n-Heptane	8.193	350922	10.269 ng/ml
4) t Benzene	8.344	375799	10.263 ng/ml
6) t Toluene	11.037	1046182	30.940 ng/ml
7) t Ethylbenzene	13.444	310671	10.362 ng/ml
8) t m-Xylene	13.574	595033	20.692 ng/ml
9) t O-Xylene	14.297	528958	20.727 ng/ml
10) t 1,2,4-Trimethylbenzene	16.549	320785	20.628 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071321\
Data File : FB026042.D
Signal(s) : FID2B.CH
Acq On : 13 Jul 2021 11:25
Operator : AJ/MA
Sample : BSF0713S1
Misc : 5.00G/5.00ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 14 01:07:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071021.M
Quant Title :
QLast Update : Fri Jul 09 13:11:34 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

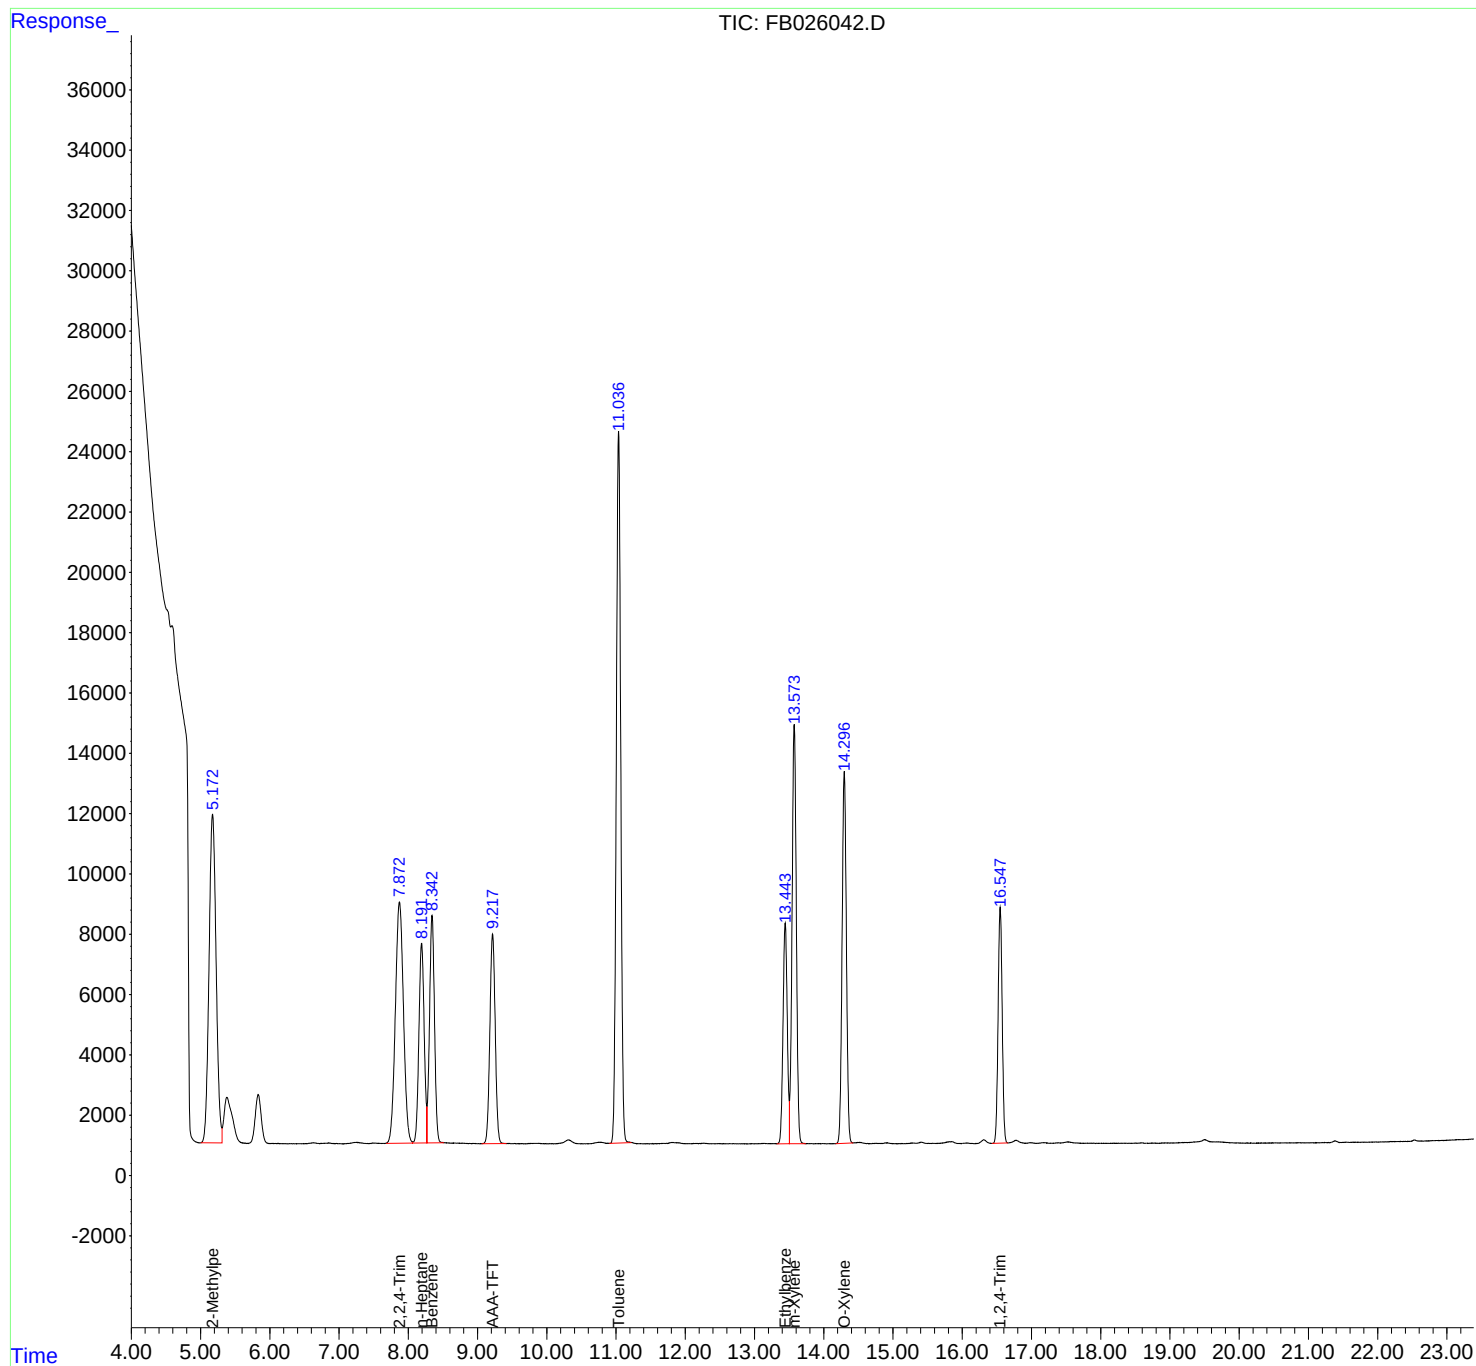

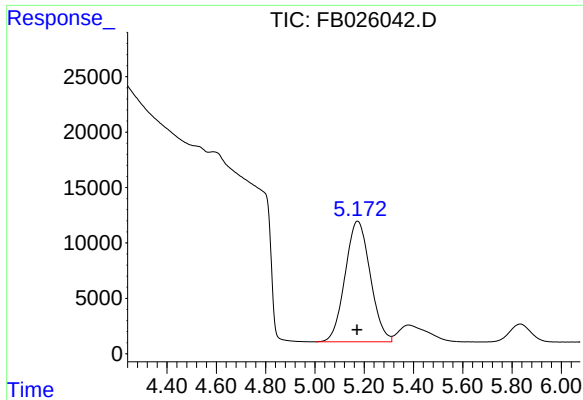


#1 2-Methylpentane

R.T.: 5.174 min
Delta R.T.: 0.002 min
Response: 771522
Conc: 31.29 ng/ml

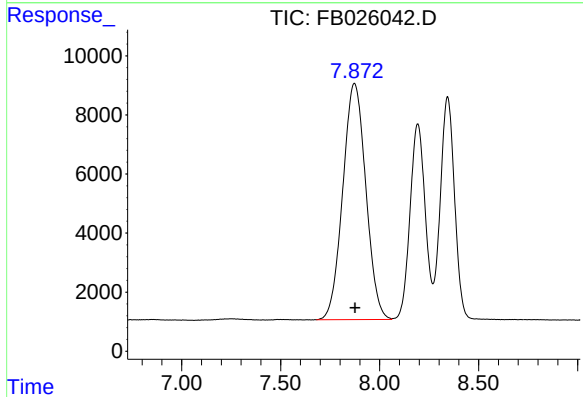


#2 2,2,4-Trimethylpentane

R.T.: 7.873 min
Delta R.T.: -0.003 min
Response: 647575
Conc: 32.00 ng/ml

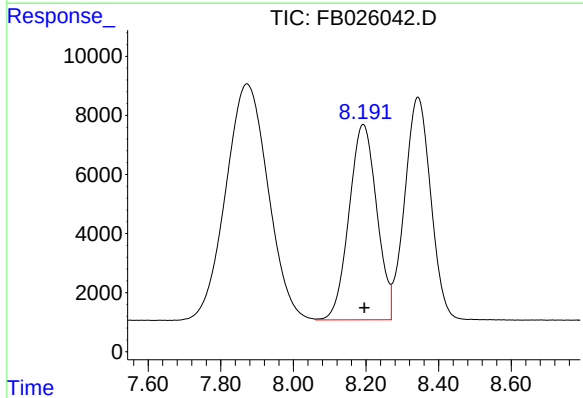


#3 n-Heptane

R.T.: 8.193 min
Delta R.T.: -0.003 min
Response: 350922
Conc: 10.27 ng/ml

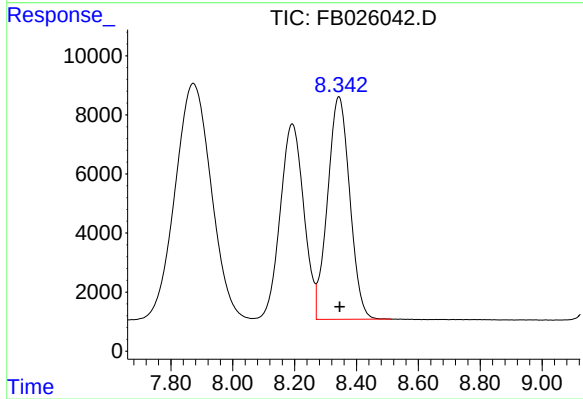


#4 Benzene

R.T.: 8.344 min
Delta R.T.: -0.003 min
Response: 375799
Conc: 10.26 ng/ml

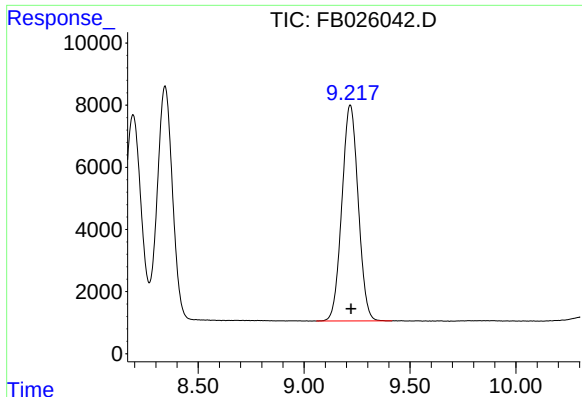


#5 AAA-TFT

R.T.: 9.218 min
Delta R.T.: -0.003 min
Response: 371854
Conc: 19.71 ng/ml

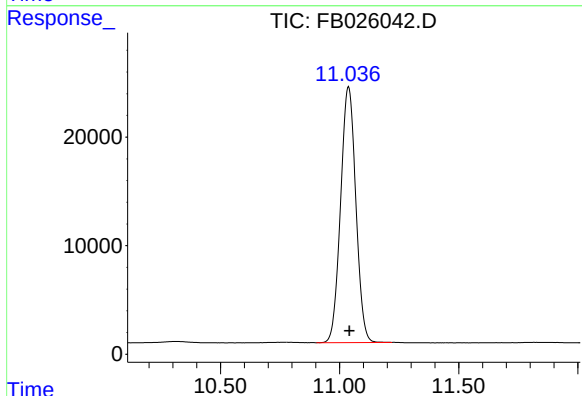


#6 Toluene

R.T.: 11.037 min
Delta R.T.: -0.004 min
Response: 1046182
Conc: 30.94 ng/ml

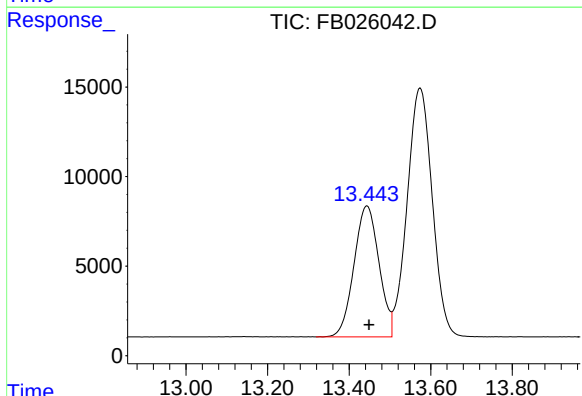


#7 Ethylbenzene

R.T.: 13.444 min
Delta R.T.: -0.005 min
Response: 310671
Conc: 10.36 ng/ml

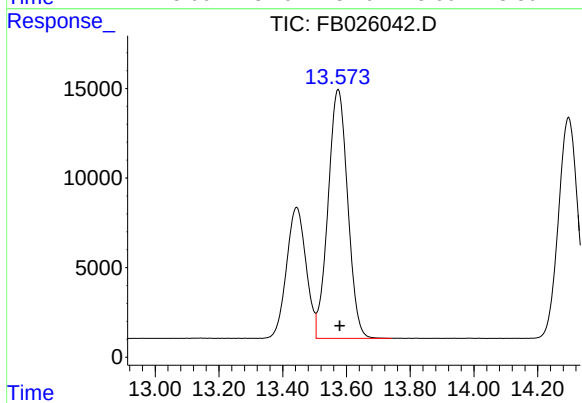


#8 m-Xylene

R.T.: 13.574 min
Delta R.T.: -0.005 min
Response: 595033
Conc: 20.69 ng/ml

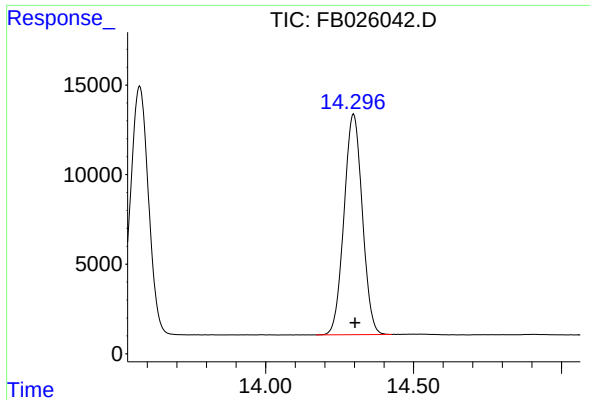

#9 O-Xylene

R.T.: 14.297 min
Delta R.T.: -0.005 min
Response: 528958
Conc: 20.73 ng/ml

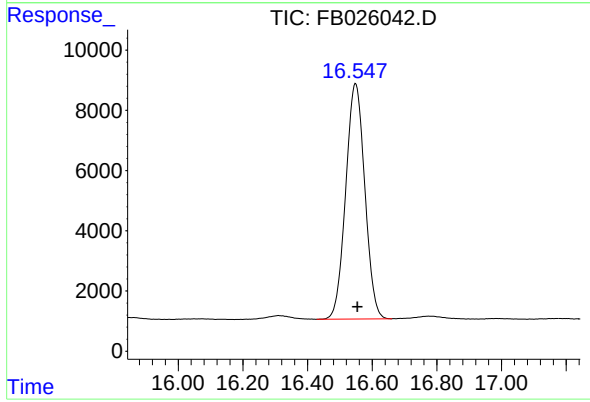

#10 1,2,4-Trimethylbenzene

R.T.: 16.549 min
Delta R.T.: -0.005 min
Response: 320785
Conc: 20.63 ng/ml