

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071321\
 Data File : FB026046.D
 Signal(s) : FID2B.CH
 Acq On : 13 Jul 2021 13:34
 Operator : AJ/MA
 Sample : M2940-03
 Misc : 5.02G/5.00ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 14 01:08:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071021.M
 Quant Title :
 QLast Update : Fri Jul 09 13:11:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.226	297906	15.792 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.193	36637	1.486 ng/ml
2) t 2,2,4-Trimethylpentane	7.879	34622	1.711 ng/ml
3) t n-Heptane	8.203	17614	0.515 ng/mlm
4) t Benzene	8.352	16359	0.447 ng/mlm
6) t Toluene	11.043	53336	1.577 ng/ml
7) t Ethylbenzene	13.446	15182	0.506 ng/mlm
8) t m-Xylene	13.579	29882	1.039 ng/ml
9) t O-Xylene	14.300	26265	1.029 ng/mlm
10) t 1,2,4-Trimethylbenzene	16.548	17529	1.127 ng/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071321\
Data File : FB026046.D
Signal(s) : FID2B.CH
Acq On : 13 Jul 2021 13:34
Operator : AJ/MA
Sample : M2940-03
Misc : 5.02G/5.00ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 14 01:08:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071021.M
Quant Title :
QLast Update : Fri Jul 09 13:11:34 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

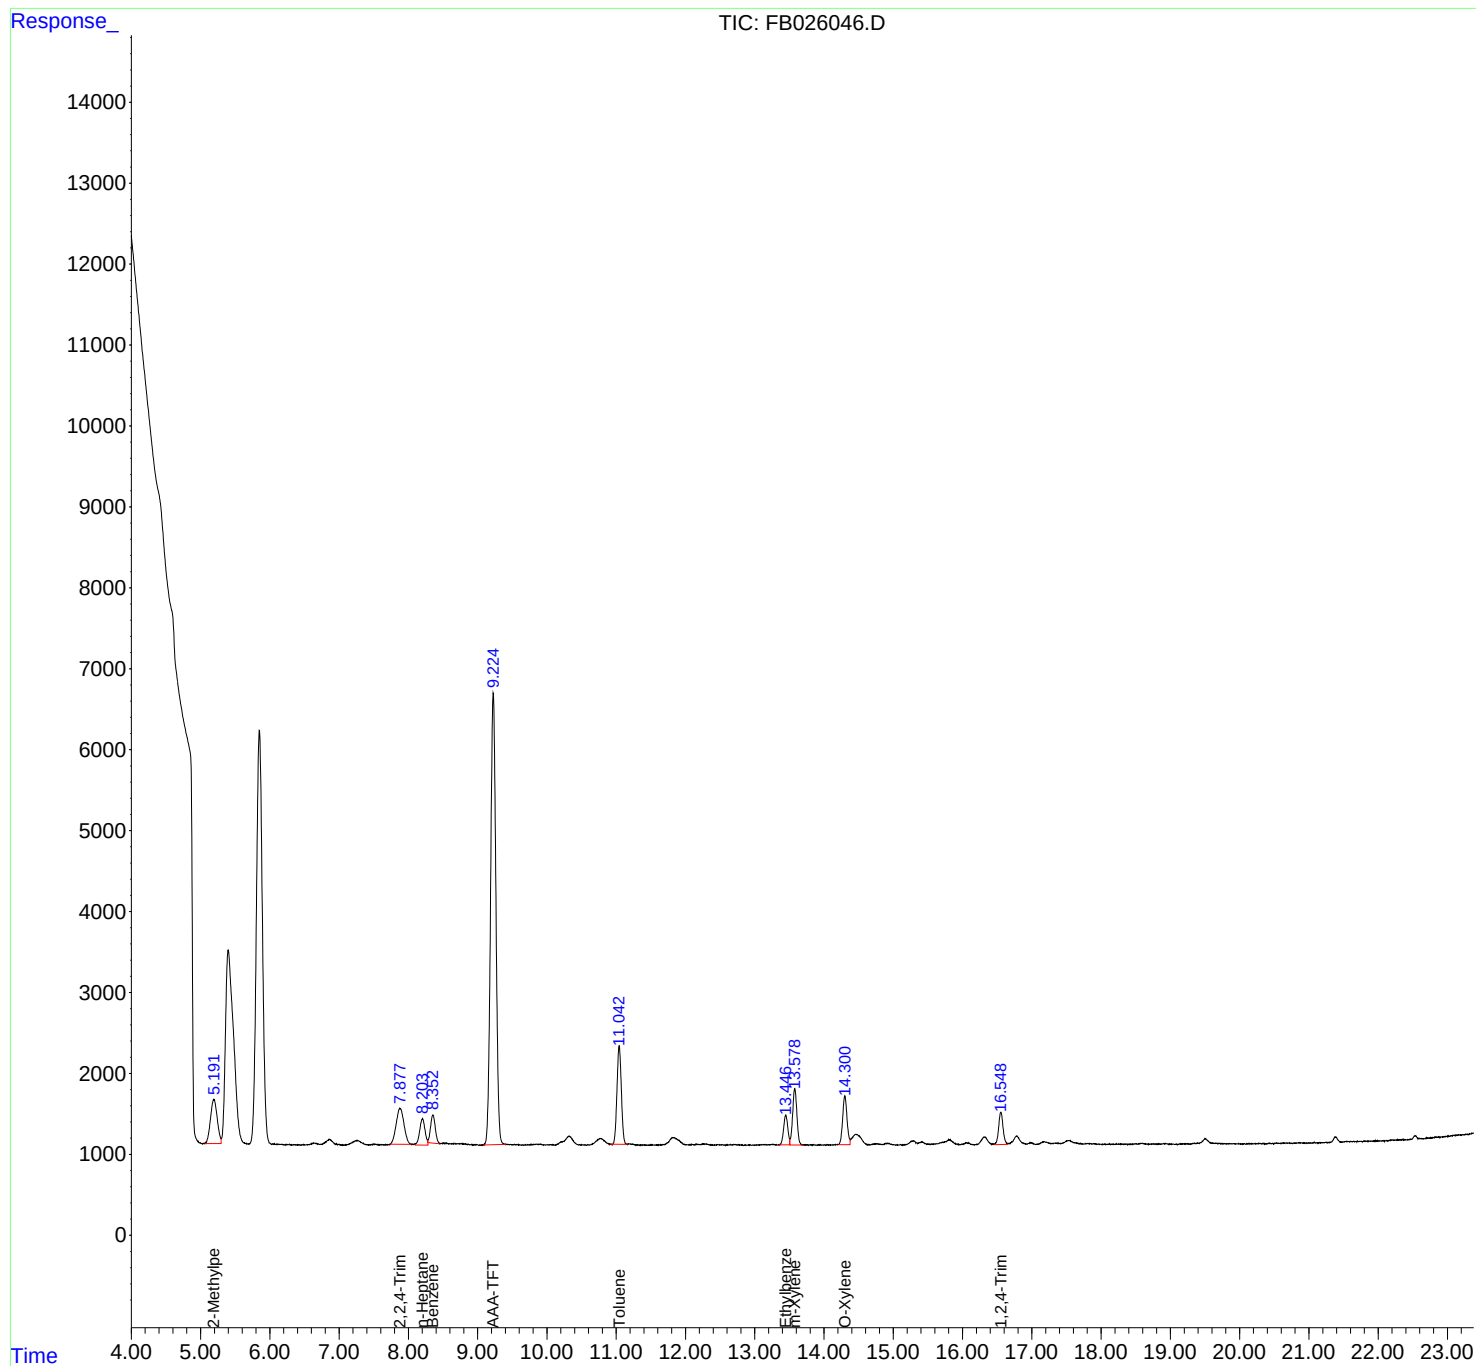

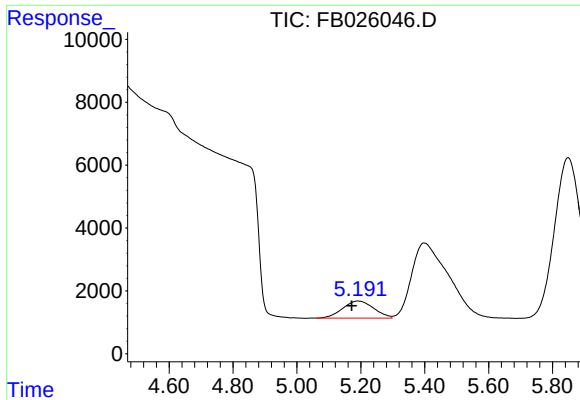


#1 2-Methylpentane

R.T.: 5.193 min
Delta R.T.: 0.021 min
Response: 36637
Conc: 1.49 ng/ml

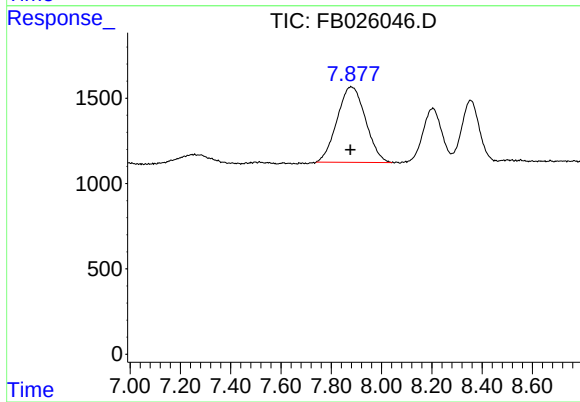


#2 2,2,4-Trimethylpentane

R.T.: 7.879 min
Delta R.T.: 0.003 min
Response: 34622
Conc: 1.71 ng/ml

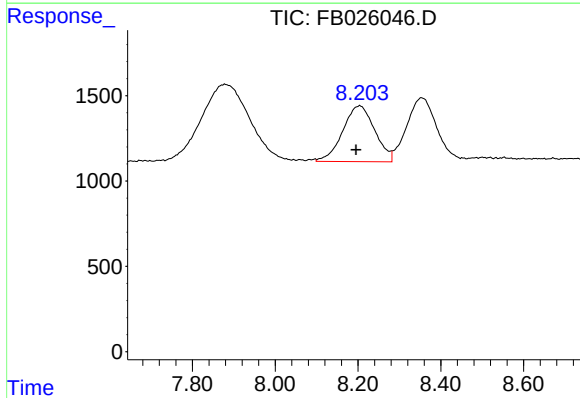


#3 n-Heptane

R.T.: 8.203 min
Delta R.T.: 0.008 min
Response: 17614
Conc: 0.52 ng/ml m

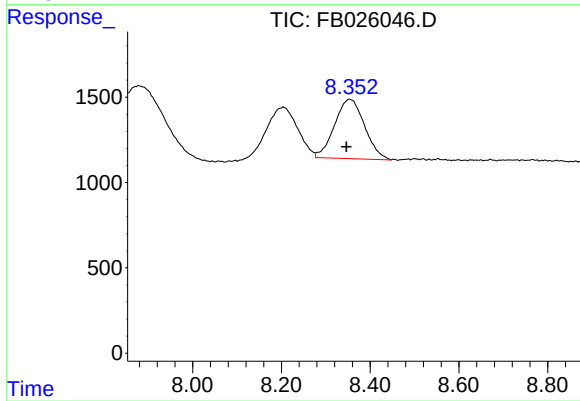


#4 Benzene

R.T.: 8.352 min
Delta R.T.: 0.005 min
Response: 16359
Conc: 0.45 ng/ml m

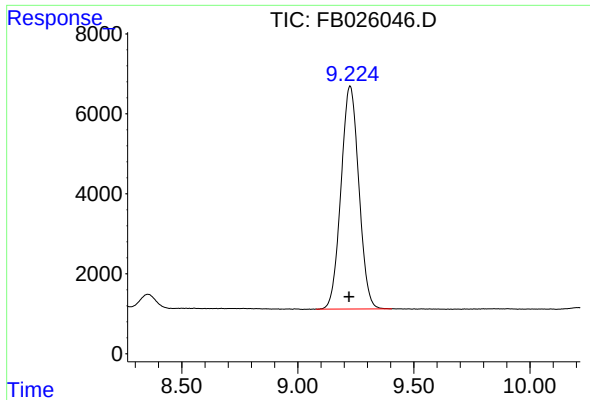


#5 AAA-TFT

R.T.: 9.226 min
Delta R.T.: 0.004 min
Response: 297906
Conc: 15.79 ng/ml

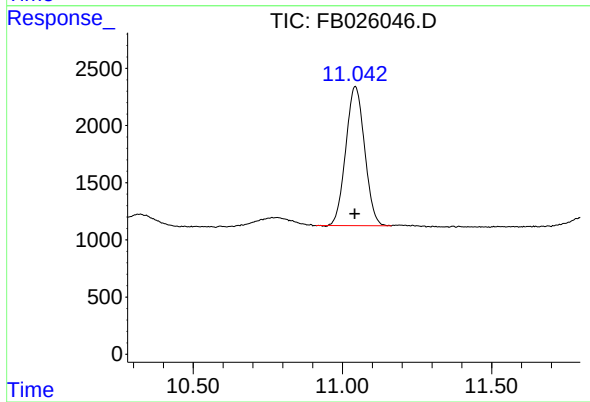


#6 Toluene

R.T.: 11.043 min
Delta R.T.: 0.002 min
Response: 53336
Conc: 1.58 ng/ml

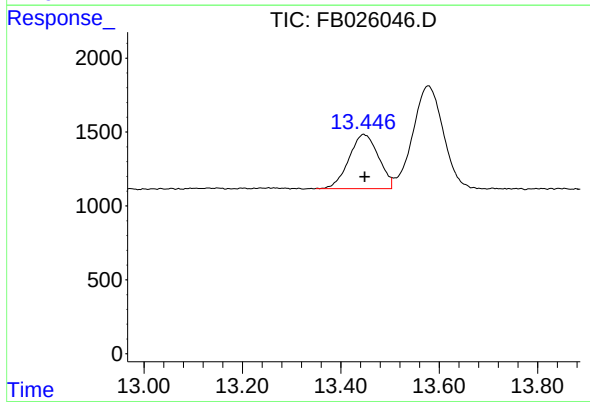


#7 Ethylbenzene

R.T.: 13.446 min
Delta R.T.: -0.003 min
Response: 15182
Conc: 0.51 ng/ml m

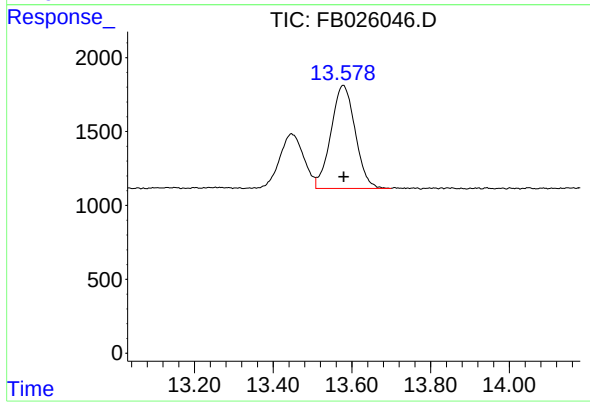


#8 m-Xylene

R.T.: 13.579 min
Delta R.T.: 0.000 min
Response: 29882
Conc: 1.04 ng/ml

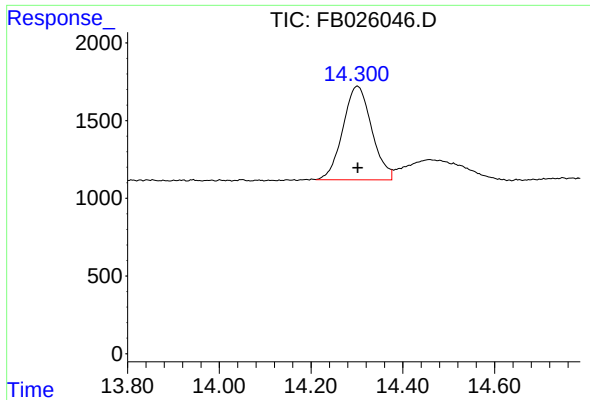

#9 O-Xylene

R.T.: 14.300 min
Delta R.T.: -0.002 min
Response: 26265
Conc: 1.03 ng/ml m

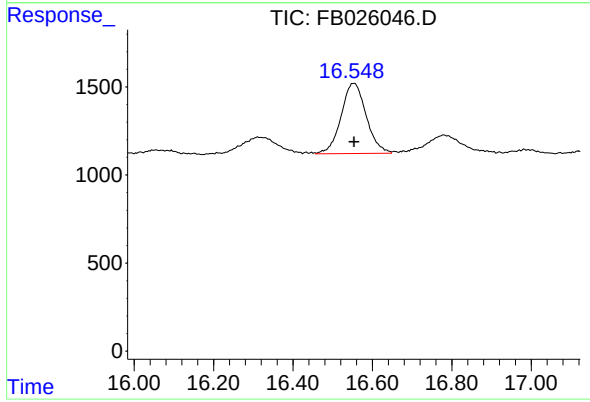

#10 1,2,4-Trimethylbenzene

R.T.: 16.548 min
Delta R.T.: -0.006 min
Response: 17529
Conc: 1.13 ng/ml m