

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071420\
 Data File : FB024590.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jul 2020 9:30
 Operator : DD/AJ
 Sample : BSF0714S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 15 00:43:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
 Quant Title :
 QLast Update : Thu Jul 09 10:49:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.797	385620	16.740 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.687	782794	26.452 ng/ml
2) t	2,2,4-Trimethylpentane	7.416	838437	26.781 ng/ml
3) t	n-Heptane	7.756	281357	9.049 ng/ml
4) t	Benzene	7.890	332013	8.710 ng/ml
6) t	Toluene	10.629	945798	25.867 ng/ml
7) t	Ethylbenzene	13.069	285144	8.348 ng/ml
8) t	m-Xylene	13.202	563596	16.701 ng/ml
9) t	O-Xylene	13.929	556035	16.918 ng/ml
10) t	1,2,4-Trimethylbenzene	16.207	464021	17.202 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071420\
Data File : FB024590.D
Signal(s) : FID2B.CH
Acq On : 14 Jul 2020 9:30
Operator : DD/AJ
Sample : BSF0714S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 15 00:43:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

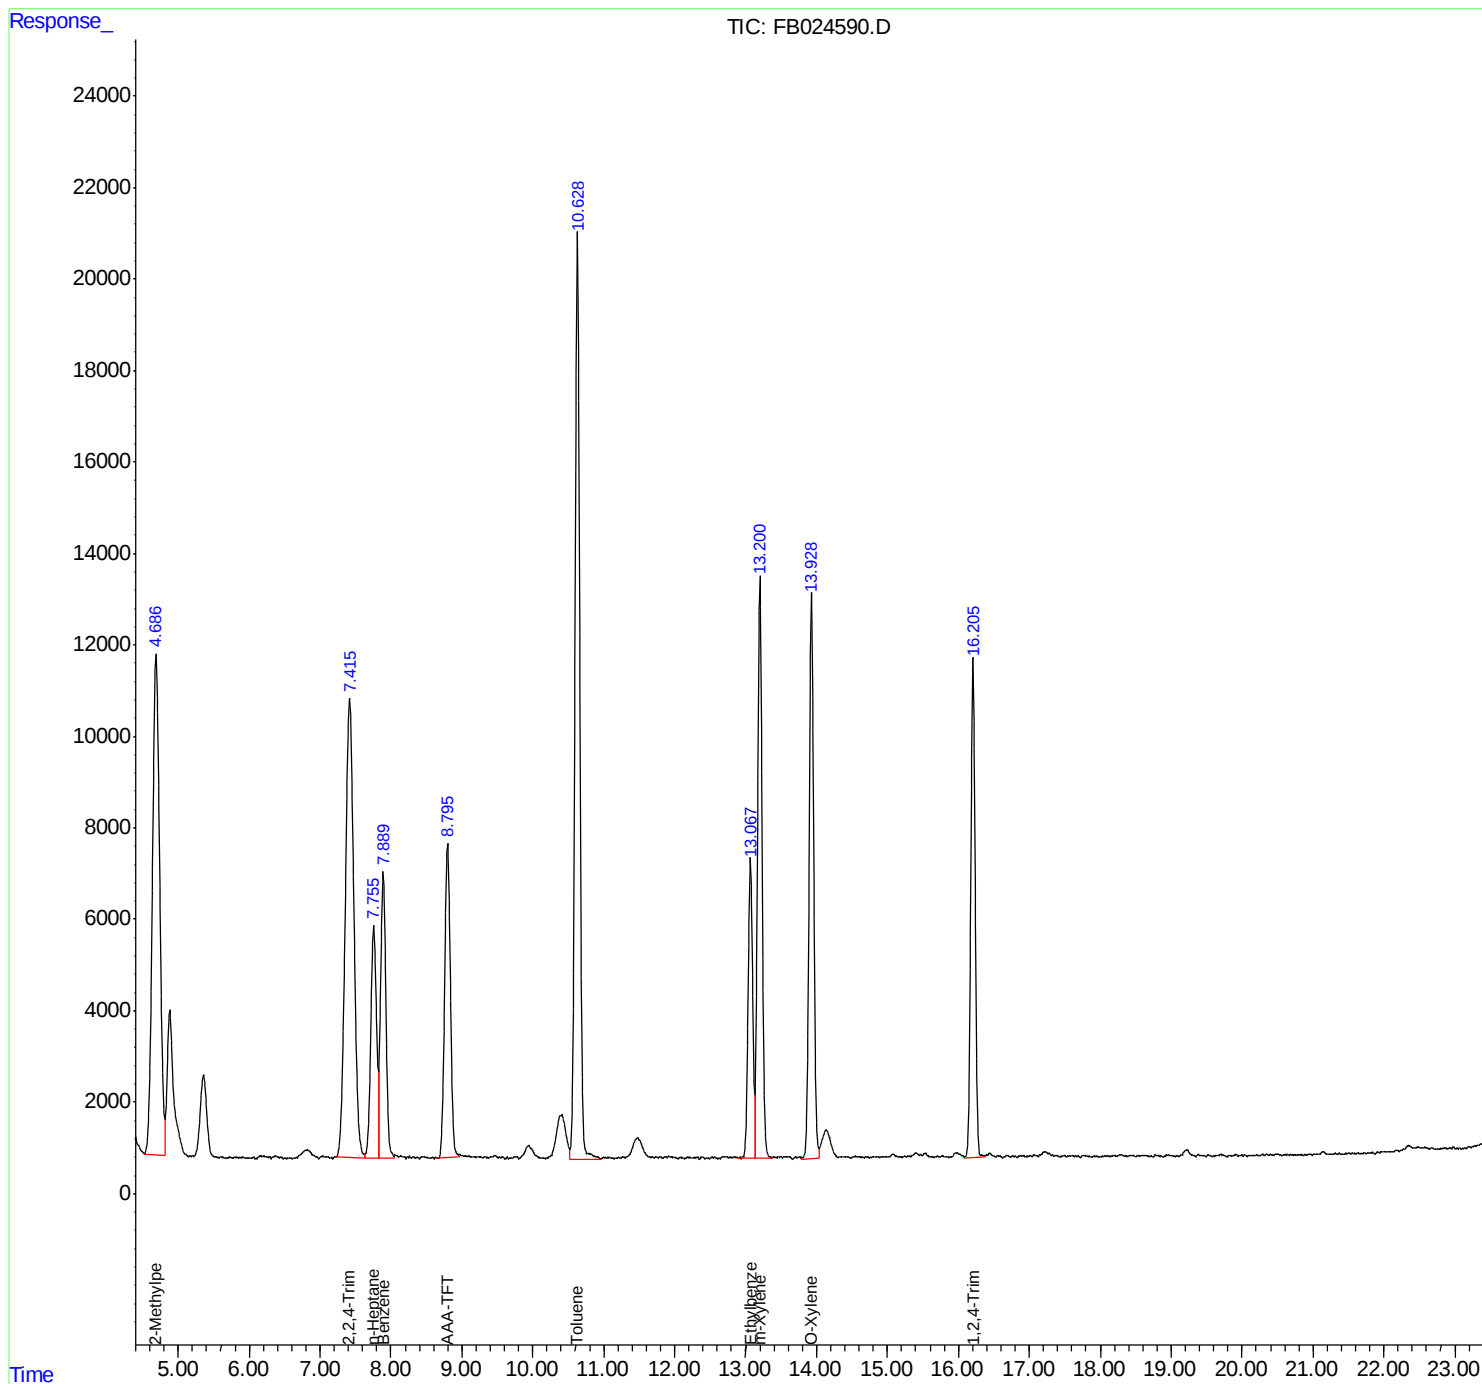

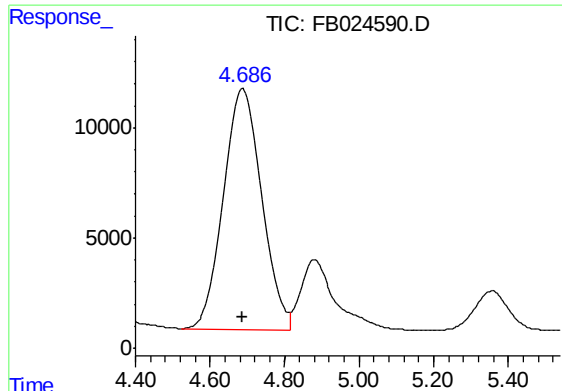


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 782794
Conc: 26.45 ng/ml

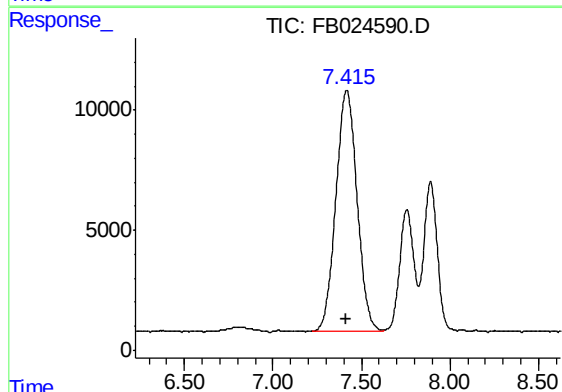


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 838437
Conc: 26.78 ng/ml

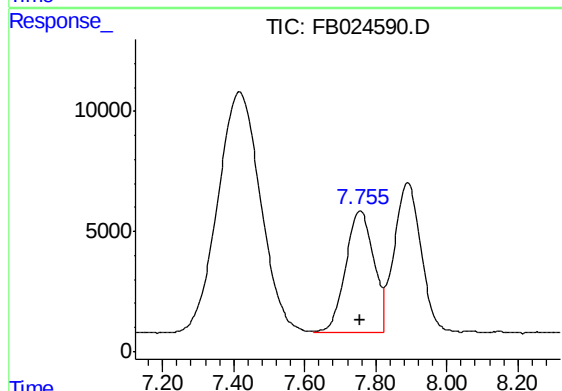


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 281357
Conc: 9.05 ng/ml

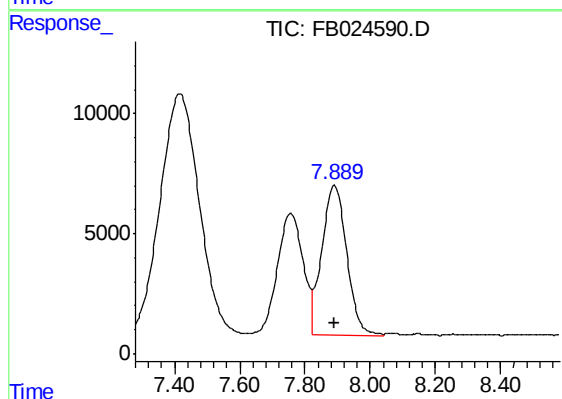


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.001 min
Response: 332013
Conc: 8.71 ng/ml

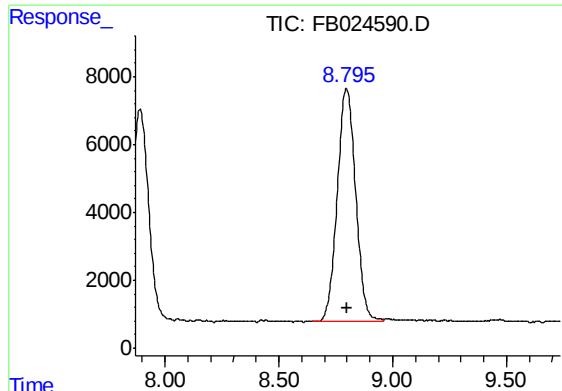


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 385620
Conc: 16.74 ng/ml

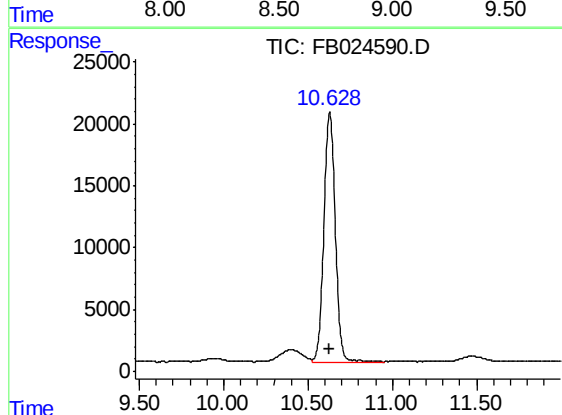


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.000 min
Response: 945798
Conc: 25.87 ng/ml

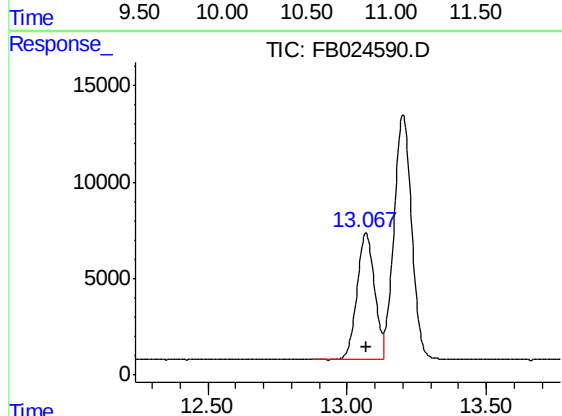


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.000 min
Response: 285144
Conc: 8.35 ng/ml

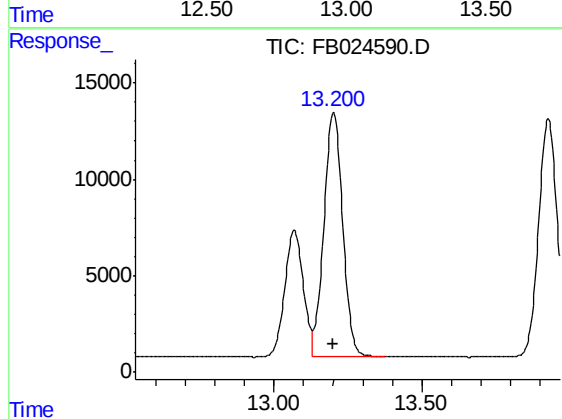


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: 0.000 min
Response: 563596
Conc: 16.70 ng/ml

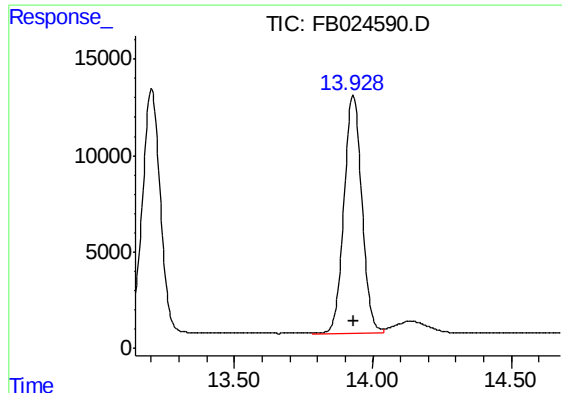

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.000 min
Response: 556035
Conc: 16.92 ng/ml

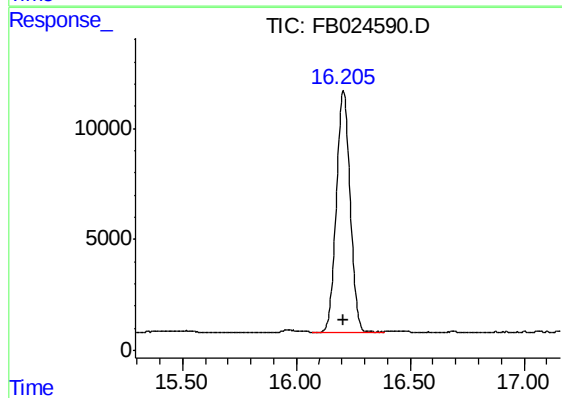

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: 0.000 min
Response: 464021
Conc: 17.20 ng/ml