

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071520\
 Data File : FB024603.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jul 2020 9:57
 Operator : DD/AJ
 Sample : BSF0715S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 16 00:59:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
 Quant Title :
 QLast Update : Thu Jul 09 10:49:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.797	362686	15.745 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.689	724428	24.480 ng/ml
2) t	2,2,4-Trimethylpentane	7.415	789779	25.227 ng/ml
3) t	n-Heptane	7.755	264191	8.497 ng/ml
4) t	Benzene	7.890	320348	8.404 ng/ml
6) t	Toluene	10.627	901340	24.651 ng/ml
7) t	Ethylbenzene	13.067	291333	8.529 ng/ml
8) t	m-Xylene	13.200	570154	16.895 ng/ml
9) t	O-Xylene	13.927	555660	16.906 ng/ml
10) t	1,2,4-Trimethylbenzene	16.205	464817	17.232 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071520\
Data File : FB024603.D
Signal(s) : FID2B.CH
Acq On : 15 Jul 2020 9:57
Operator : DD/AJ
Sample : BSF071551
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 16 00:59:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

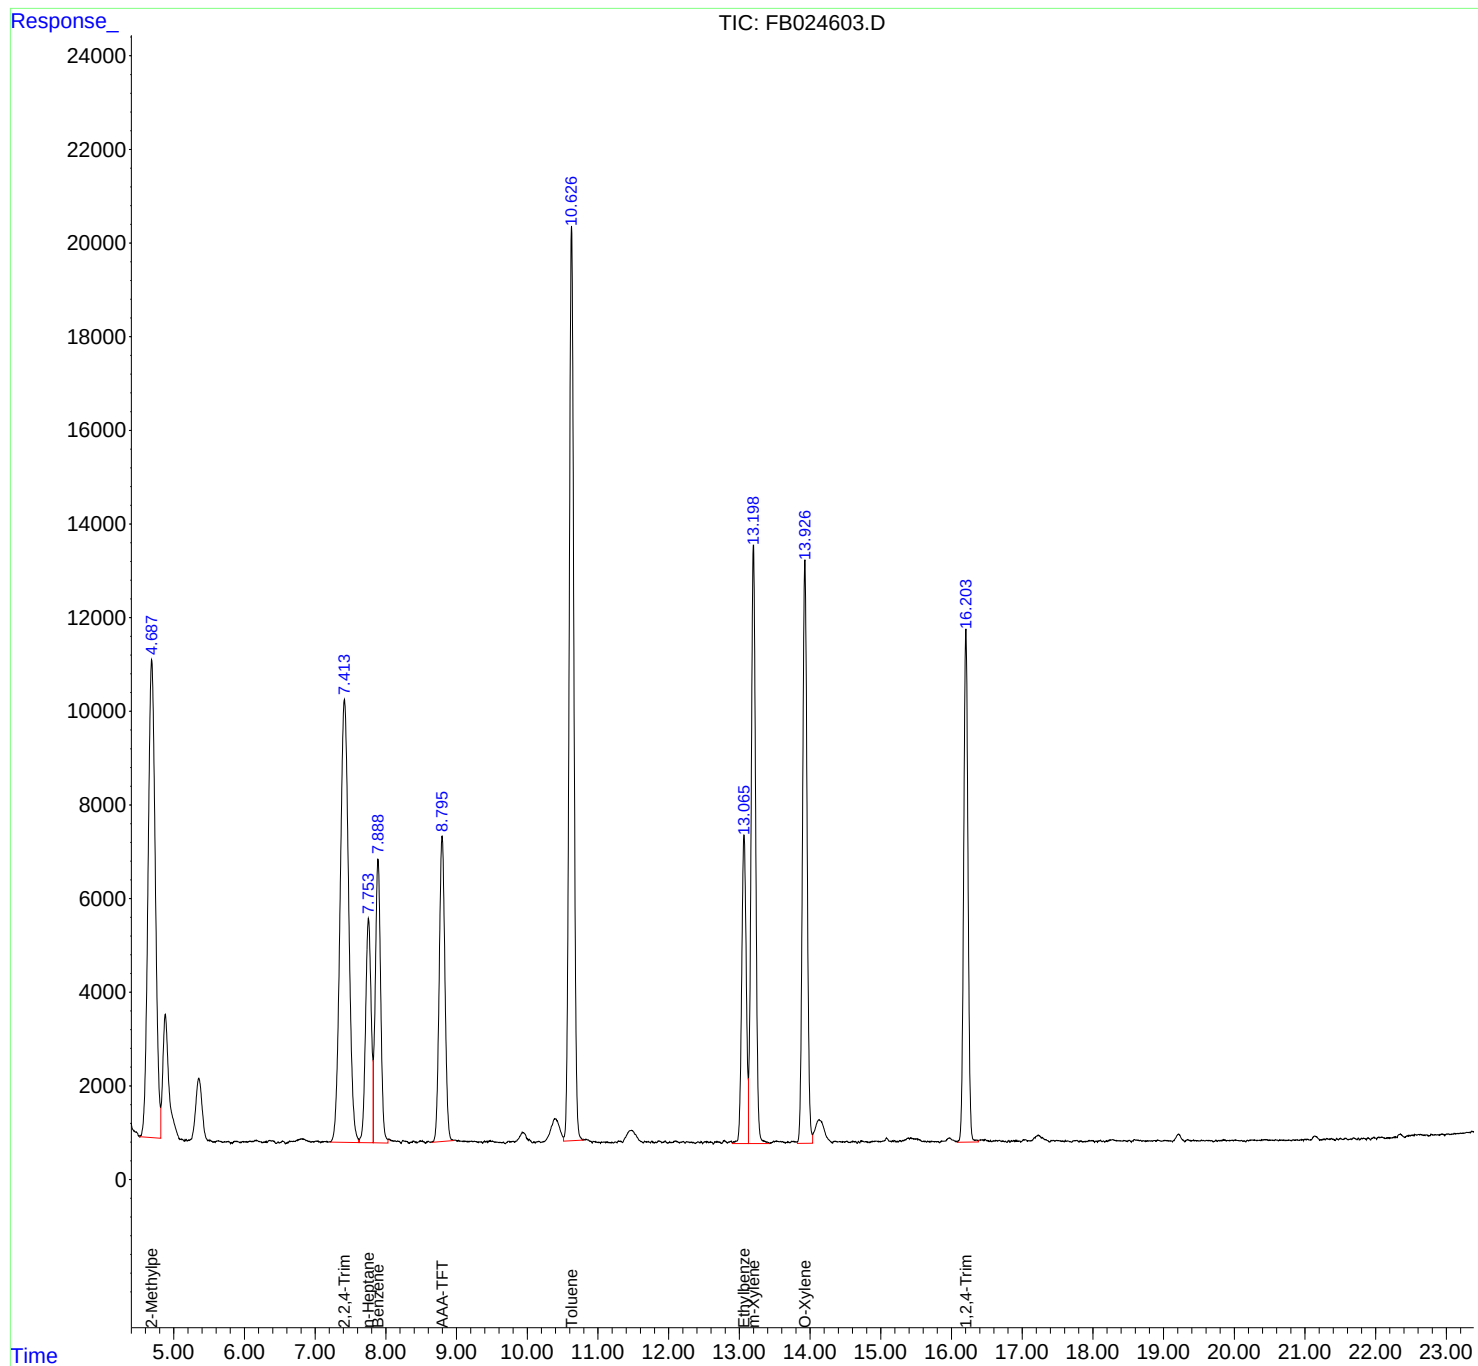

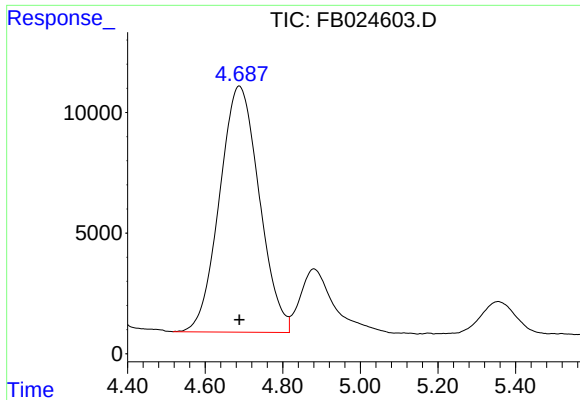


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 724428
Conc: 24.48 ng/ml

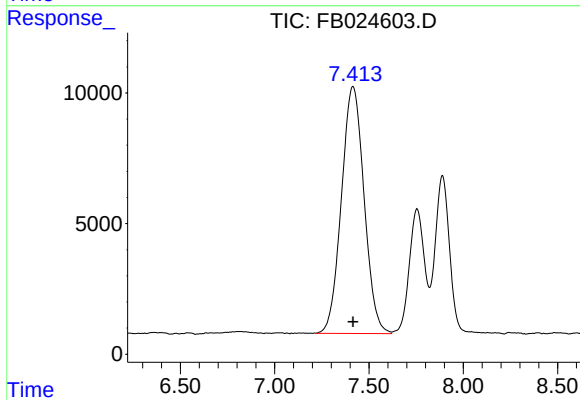


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.001 min
Response: 789779
Conc: 25.23 ng/ml

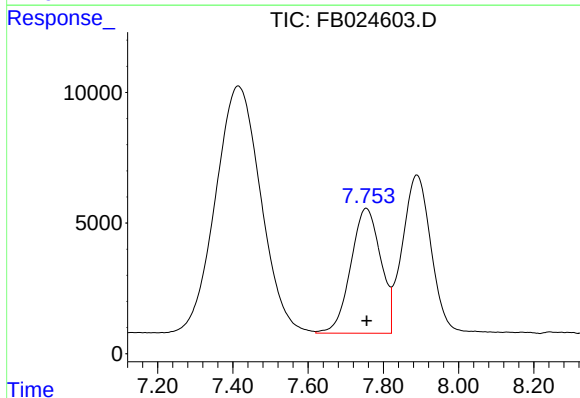


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.001 min
Response: 264191
Conc: 8.50 ng/ml

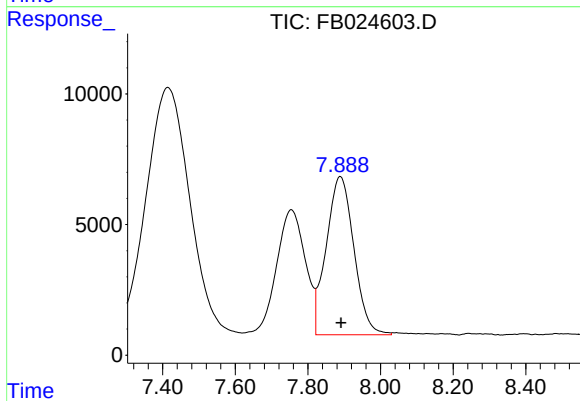


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 320348
Conc: 8.40 ng/ml

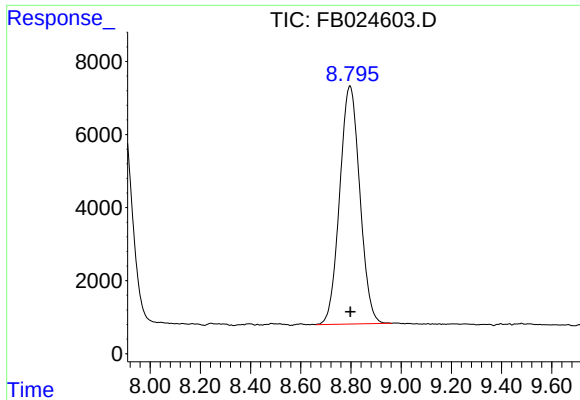


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.001 min
Response: 362686
Conc: 15.74 ng/ml

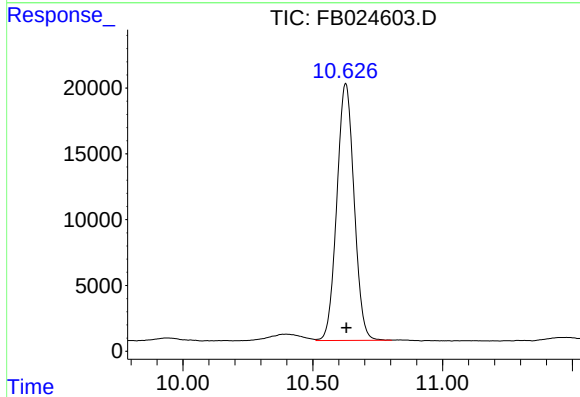


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.002 min
Response: 901340
Conc: 24.65 ng/ml

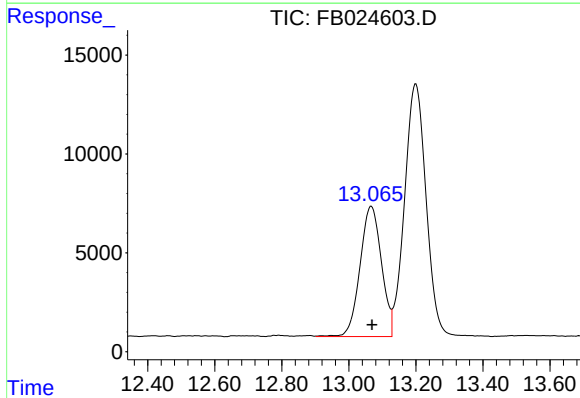


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.002 min
Response: 291333
Conc: 8.53 ng/ml

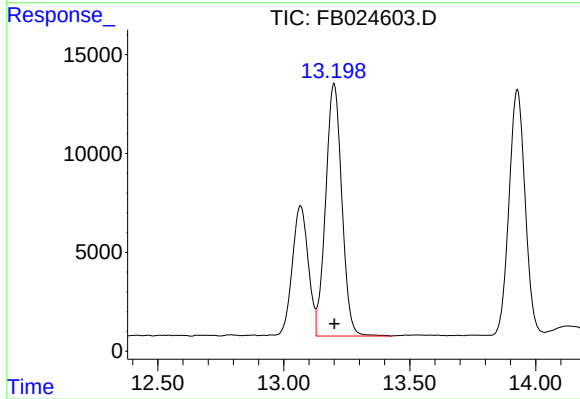


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.002 min
Response: 570154
Conc: 16.90 ng/ml

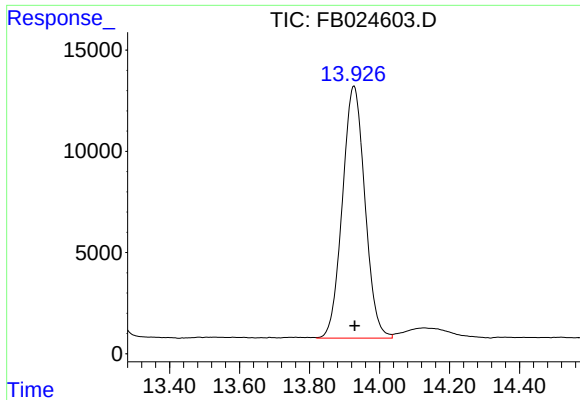

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.002 min
Response: 555660
Conc: 16.91 ng/ml

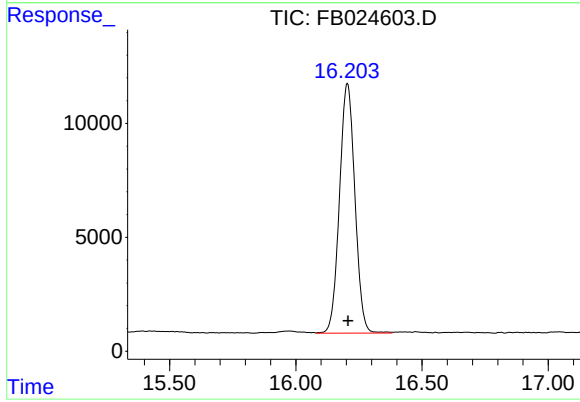

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.002 min
Response: 464817
Conc: 17.23 ng/ml