

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071520\
 Data File : FB024607.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jul 2020 11:59
 Operator : DD/AJ
 Sample : L3188-08MS
 Misc : 5.08g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 16 00:59:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
 Quant Title :
 QLast Update : Thu Jul 09 10:49:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	426954	18.535 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	669993	22.640 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	686552	21.930 ng/ml
3) t n-Heptane	7.757	227362	7.312 ng/ml
4) t Benzene	7.891	318166	8.347 ng/ml
6) t Toluene	10.628	851511	23.288 ng/ml
7) t Ethylbenzene	13.069	254265	7.444 ng/ml
8) t m-Xylene	13.201	494058	14.640 ng/ml
9) t O-Xylene	13.929	486152	14.792 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	376550	13.959 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB071520\
Data File : FB024607.D
Signal(s) : FID2B.CH
Acq On : 15 Jul 2020 11:59
Operator : DD/AJ
Sample : L3188-08MS
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 16 00:59:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB070920.M
Quant Title :
QLast Update : Thu Jul 09 10:49:06 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

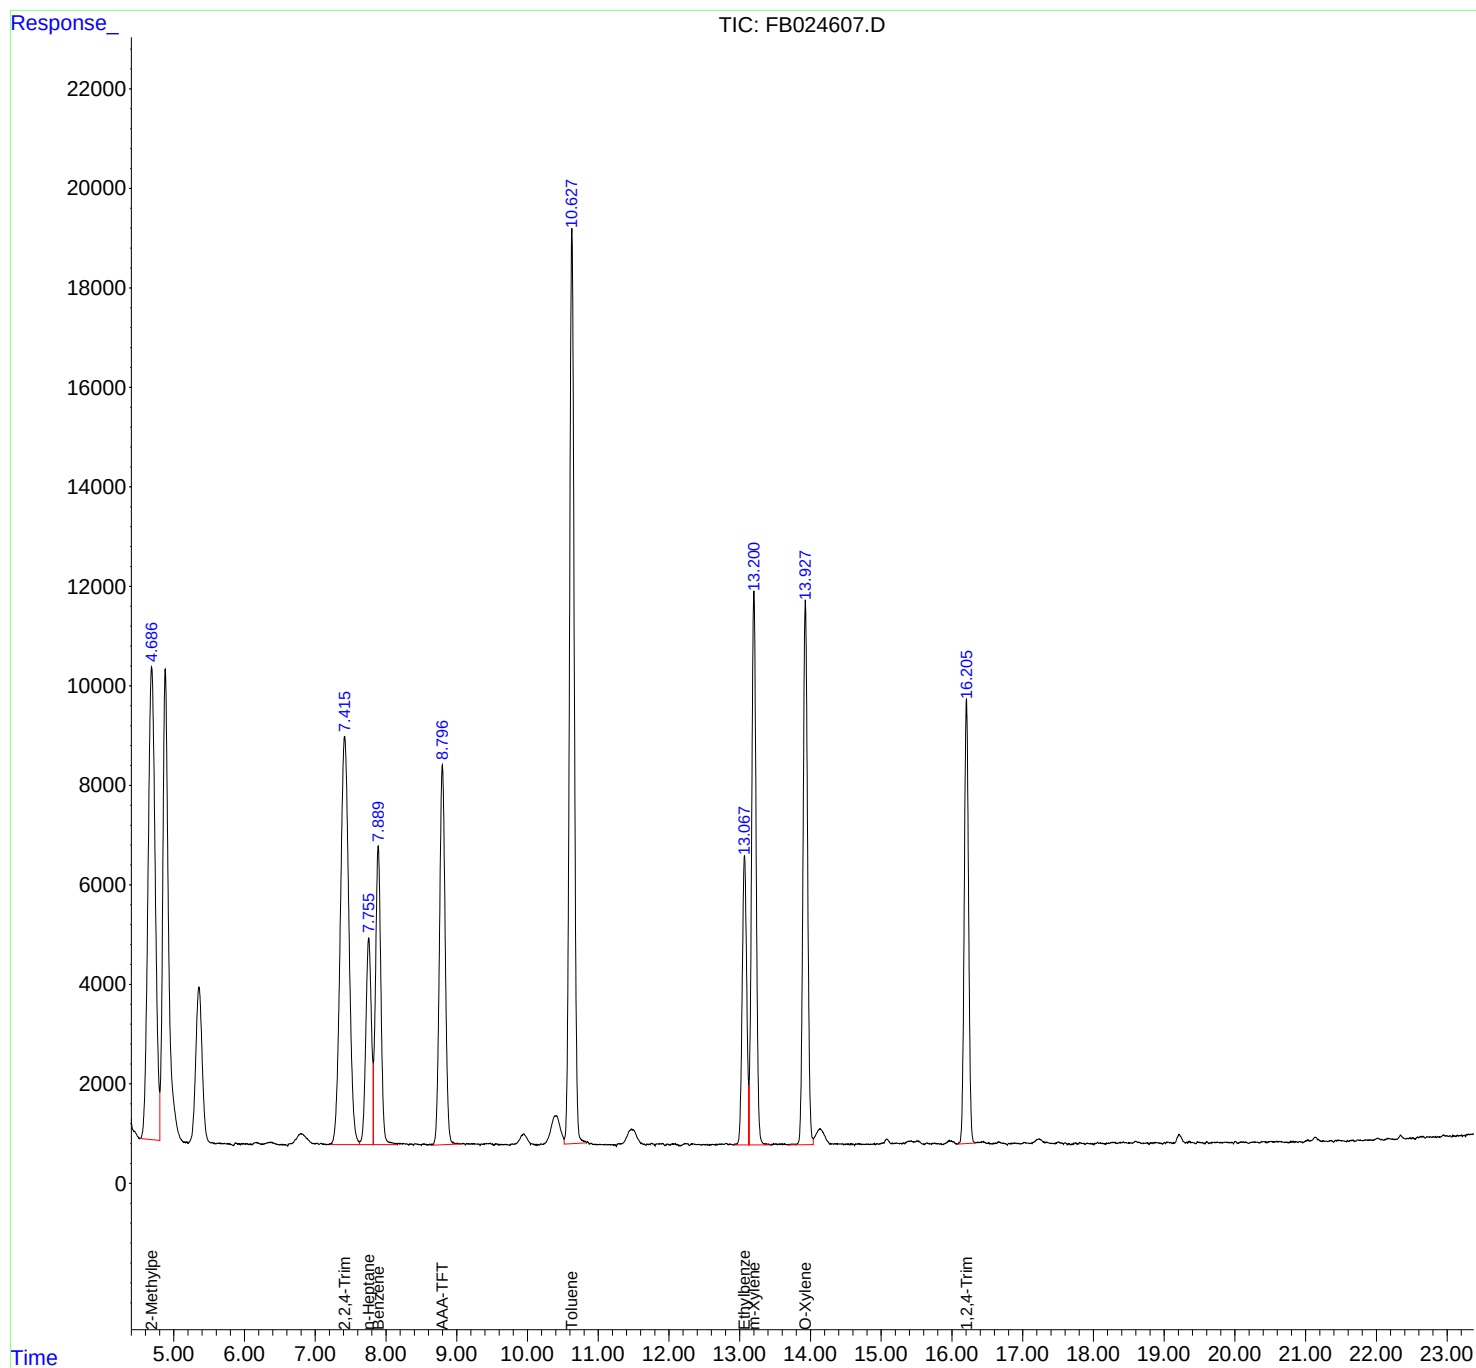

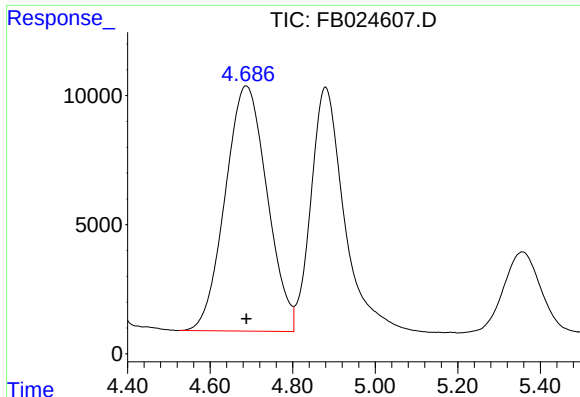


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 669993
Conc: 22.64 ng/ml

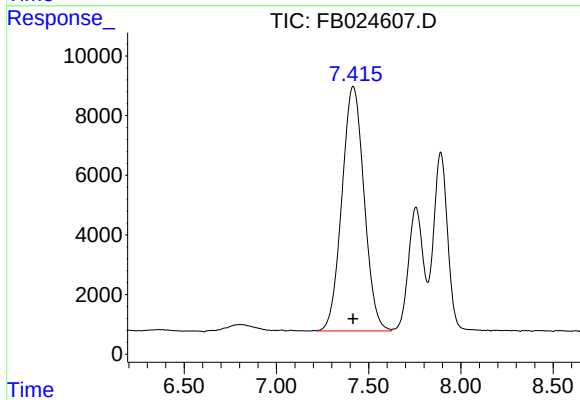


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 686552
Conc: 21.93 ng/ml

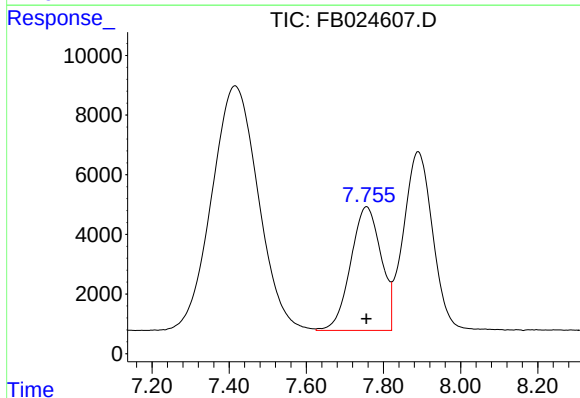


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 227362
Conc: 7.31 ng/ml

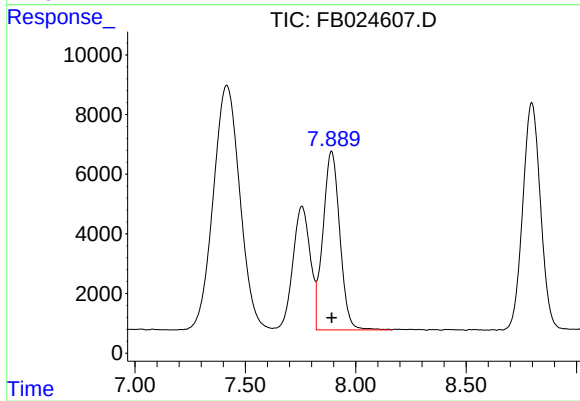


#4 Benzene

R.T.: 7.891 min
Delta R.T.: -0.001 min
Response: 318166
Conc: 8.35 ng/ml

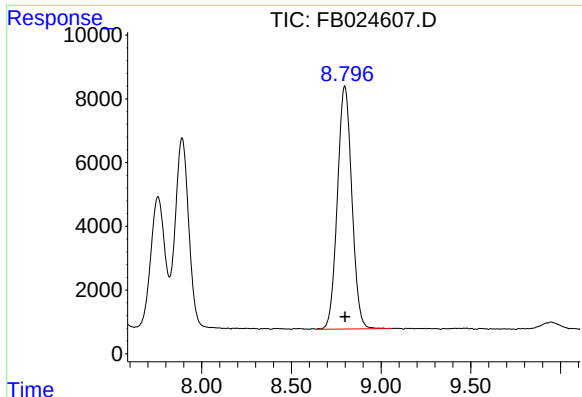


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 426954
Conc: 18.53 ng/ml

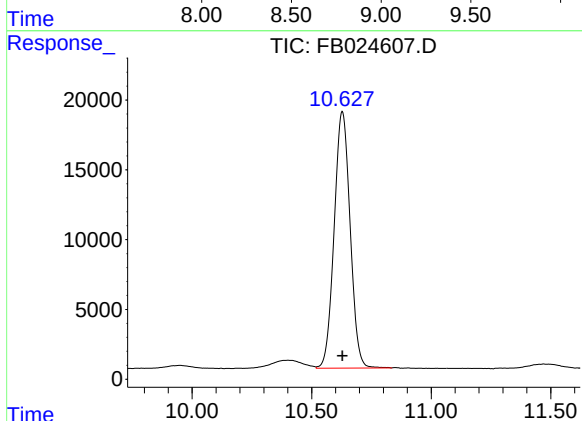


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.000 min
Response: 851511
Conc: 23.29 ng/ml

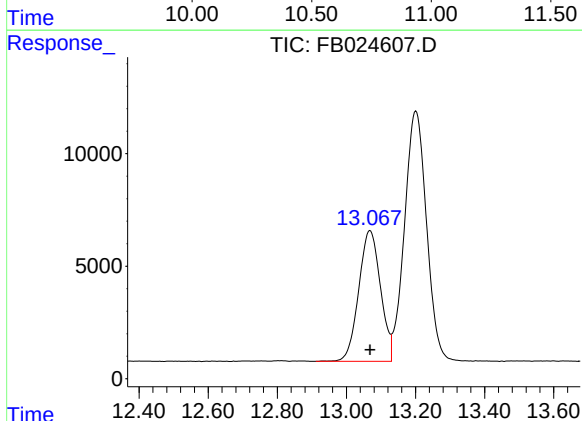


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.000 min
Response: 254265
Conc: 7.44 ng/ml

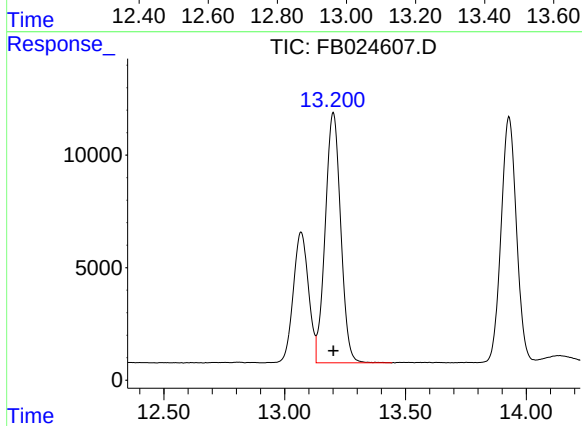


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: 0.000 min
Response: 494058
Conc: 14.64 ng/ml

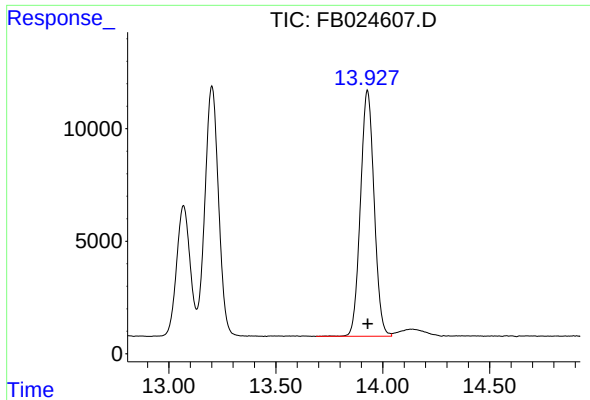

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.000 min
Response: 486152
Conc: 14.79 ng/ml

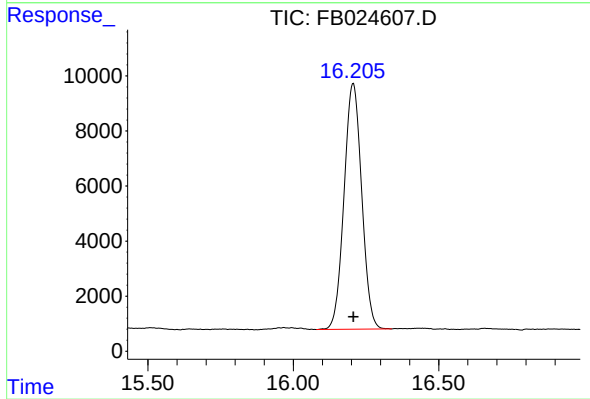

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.000 min
Response: 376550
Conc: 13.96 ng/ml